

# 742A Series

Resistance Standards

Instruction Manual

## LIMITED WARRANTY AND LIMITATION OF LIABILITY

Each Fluke product is warranted to be free from defects in material and workmanship under normal use and service. The warranty period is one year and begins on the date of shipment. Parts, product repairs, and services are warranted for 90 days. This warranty extends only to the original buyer or end-user customer of a Fluke authorized reseller, and does not apply to fuses, disposable batteries, or to any product which, in Fluke's opinion, has been misused, altered, neglected, contaminated, or damaged by accident or abnormal conditions of operation or handling. Fluke warrants that software will operate substantially in accordance with its functional specifications for 90 days and that it has been properly recorded on non-defective media. Fluke does not warrant that software will be error free or operate without interruption.

Fluke authorized resellers shall extend this warranty on new and unused products to end-user customers only but have no authority to extend a greater or different warranty on behalf of Fluke. Warranty support is available only if product is purchased through a Fluke authorized sales outlet or Buyer has paid the applicable international price. Fluke reserves the right to invoice Buyer for importation costs of repair/replacement parts when product purchased in one country is submitted for repair in another country.

Fluke's warranty obligation is limited, at Fluke's option, to refund of the purchase price, free of charge repair, or replacement of a defective product which is returned to a Fluke authorized service center within the warranty period.

To obtain warranty service, contact your nearest Fluke authorized service center to obtain return authorization information, then send the product to that service center, with a description of the difficulty, postage and insurance prepaid (FOB Destination). Fluke assumes no risk for damage in transit. Following warranty repair, the product will be returned to Buyer, transportation prepaid (FOB Destination). If Fluke determines that failure was caused by neglect, misuse, contamination, alteration, accident, or abnormal condition of operation or handling, including overvoltage failures caused by use outside the product's specified rating, or normal wear and tear of mechanical components, Fluke will provide an estimate of repair costs and obtain authorization before commencing the work. Following repair, the product will be returned to the Buyer transportation prepaid and the Buyer will be billed for the repair and return transportation charges (FOB Shipping Point).

THIS WARRANTY IS BUYER'S SOLE AND EXCLUSIVE REMEDY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. FLUKE SHALL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL, OR CONSEQUENTIAL DAMAGES OR LOSSES, INCLUDING LOSS OF DATA, ARISING FROM ANY CAUSE OR THEORY.

Since some countries or states do not allow limitation of the term of an implied warranty, or exclusion or limitation of incidental or consequential damages, the limitations and exclusions of this warranty may not apply to every buyer. If any provision of this Warranty is held invalid or unenforceable by a court or other decision-maker of competent jurisdiction, such holding will not affect the validity or enforceability of any other provision.

Fluke Corporation  
P.O. Box 9090  
Everett, WA 98206-9090  
U.S.A.

Fluke Europe B.V.  
P.O. Box 1186  
5602 BD Eindhoven  
The Netherlands

11/99

To register your product online, visit [register.fluke.com](http://register.fluke.com)

# Table of Contents

Title	Page
Introduction.....	1
Specifications .....	2
Design and Construction Notes.....	3
Features .....	3
Operating Notes .....	5
Connecting to the 742A Series.....	5
Cable Recommendations .....	5
Operating Temperature Range.....	6
How Temperature Correction Factors are Calculated .....	6
Storage Temperature Range.....	8
Care and Maintenance .....	9
Cleaning the 742A Series.....	9
Precautions for Handling .....	9
Servicing Information.....	9
Recertification.....	9



## **Introduction**

The 742A Series are small, light, rugged resistance standards. The standards require no temperature-controlled air or oil bath. The 742A Series are well suited for use as the following:

- Working standards
- Portable transfer standards
- Calibration support for the Fluke 5700A Calibrator

Stability and temperature coefficients of the 742A Series make them ideal for easy transport to and operation in any working environment within the range of 18 to 28 °C. The standards come with six-month and one-year uncertainty specifications. Depending on the accuracy required, a 742A can be recertified at intervals based on either specification.

Each 742A comes with a Report of Calibration and a rear panel label showing the measured value. The rear panel also has a Fluke Primary Standards Lab calibration label, labels that show temperature coefficient alpha and beta centered on 23 °C, and the standard's serial number.

### *Note*

*Refer to “How Temperature Correction Factors are Calculated,” further on in this manual for definitions of alpha and beta.*

## Specifications

Table 1 lists specification for the available 742A Series Resistance Standards.

**Table 1. 742A Series Resistance Standard Specifications**

Model	Nominal Resistance at 23 °C	Time Stability		Calibration Uncertainty	Maximum Deviation from the 23 °C Value (18 to 28 °C)	Maximum Current (Voltage)	+1 PPM Error Adder When Current Exceeds the Following
		180 Day	1 Year				
742A-1	1 Ω	±5.0 ppm	±8.0 ppm	±1.0 ppm	3.0 ppm	500 mA (500 mV)	200 mA
742A-1.9	1.9 Ω	±5.0 ppm	±8.0 ppm	±1.0 ppm	3.0 ppm	200 mA (380 mV)	100 mA
742A-10	10 Ω	±5.0 ppm	±8.0 ppm	±1.0 ppm	3.0 ppm	100 mA (1 V)	20 mA
742A-100	100 Ω	±4.0 ppm	±6.0 ppm	±1.0 ppm	3.0 ppm	20 mA (2 V)	5 mA
742A-1 k	1 kΩ	±4.0 ppm	±6.0 ppm	±1.5 ppm	2.0 ppm	10 mA (10 V)	2 mA
742A-10 k	10 Ω	±2.5 ppm	±4.0 ppm	±1.0 ppm	1.5 ppm	3 mA (30 V)	600 μA
742A-19 k	19 Ω	±2.5 ppm	±4.0 ppm	±1.5 ppm	2.0 ppm	1.5 mA (28.5 V)	600 μA
742A-100 k	100 kΩ	±4.0 ppm	±6.0 ppm	±2.5 ppm	2.0 ppm	1 mA (100 V)	400 μA
742A-1 M	1 MΩ	±6.0 ppm	±8.0 ppm	±5.0 ppm	2.0 ppm	100 μA (100 V)	100 μA
742A-10 M	10 MΩ	±6.0 ppm	±9.0 ppm	±10.0 ppm	3.0 ppm	20 μA (200 V)	20 μA
742A-19 M	19 MΩ	±8.0 ppm	±10.0 ppm	±20.0 ppm	4.0 ppm	10 μA (190 V)	10 μA

**General Specifications:**

**Accuracy:** The initial resistance is trimmed to ±2 ppm of nominal. The measured value is printed on the rear panel.

**Retrace Error (Hysteresis):** 23 °C-18 °C-23 °C cycle: Negligible resistance shift  
 23 °C-28 °C-23 °C cycle: Negligible resistance shift  
 23 °C-0 °C-23 °C cycle: <2 ppm resistance shift  
 23 °C-40 °C-23 °C cycle: <2 ppm resistance shift

**Operating Temperature Range:** 23 ±5 °C

**Storage Temperature Range:** 0 to 40 °C

**Report of Calibration:** The report of calibration includes a table of resistance values in 0.5° increments from 18 to 28 °C.

**Size:** 8.6 cm H x 10.5 cm W x 12.7 cm L (including binding posts)  
 (3.4 in H x 4.15 in W x 5 in L (including binding posts))  
 Binding posts; 2.5 cm (1.0 in)

**Weight:** 0.68 to 0.91 kg (1.5 to 2.0 lbs), depending on model


## Design and Construction Notes

The 742A Series are constructed of arrays of Fluke wirewound precision hermetically-sealed resistors. No adjustable resistors of any kind are used.

Each 742A is built with a temperature coefficient near zero at 23 °C. To further reduce errors caused by temperature changes, the binding posts are constructed of low-thermal emf material.

## Features


Figure 1 shows a front panel view. Figure 2 shows a rear panel view. Table 2 describes binding post functions. Table 3 describes the rear panel labels.

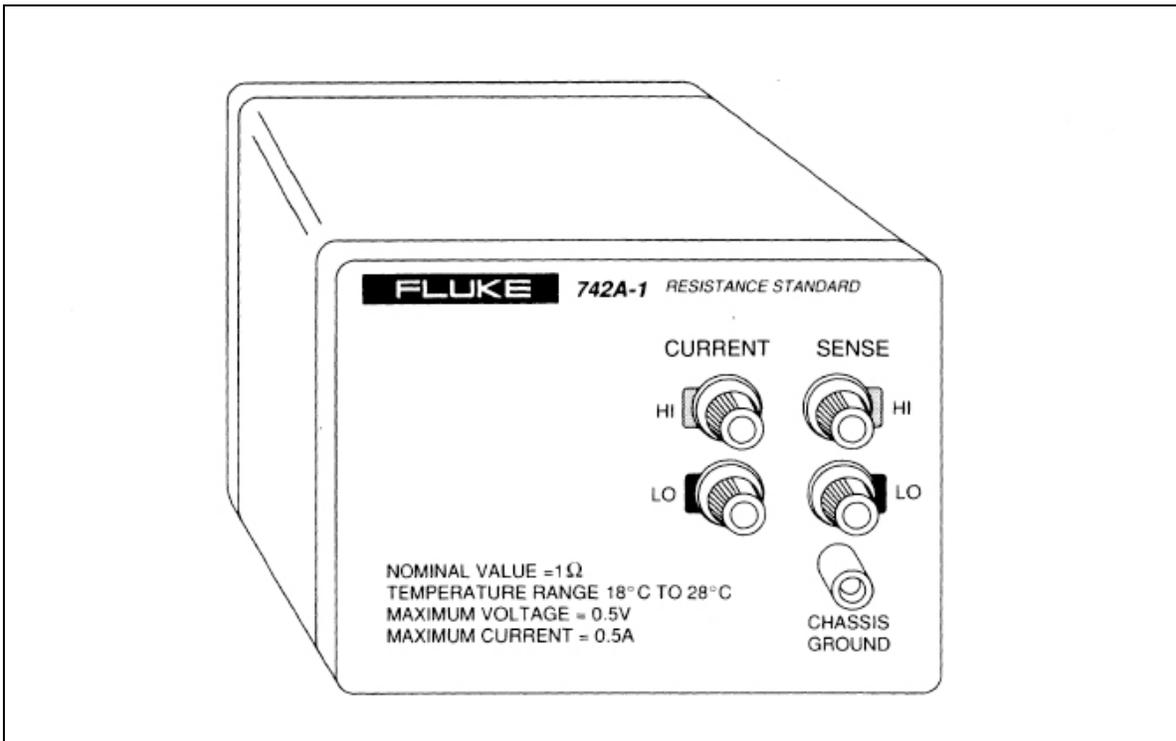

**Figure 1. Typical Front Panel View**

**Table 2. Functions of the Binding Posts**

742A Binding Post	Function
CURRENT HI	Input for the current source from an ohmmeter
CURRENT LO	Input for the current source from an ohmmeter
SENSE HI	Measurement point for a four-wire ohmmeter
SENSE LO	Measurement point for a four-wire ohmmeter
CHASSIS GROUND	Connected to the case for shielding

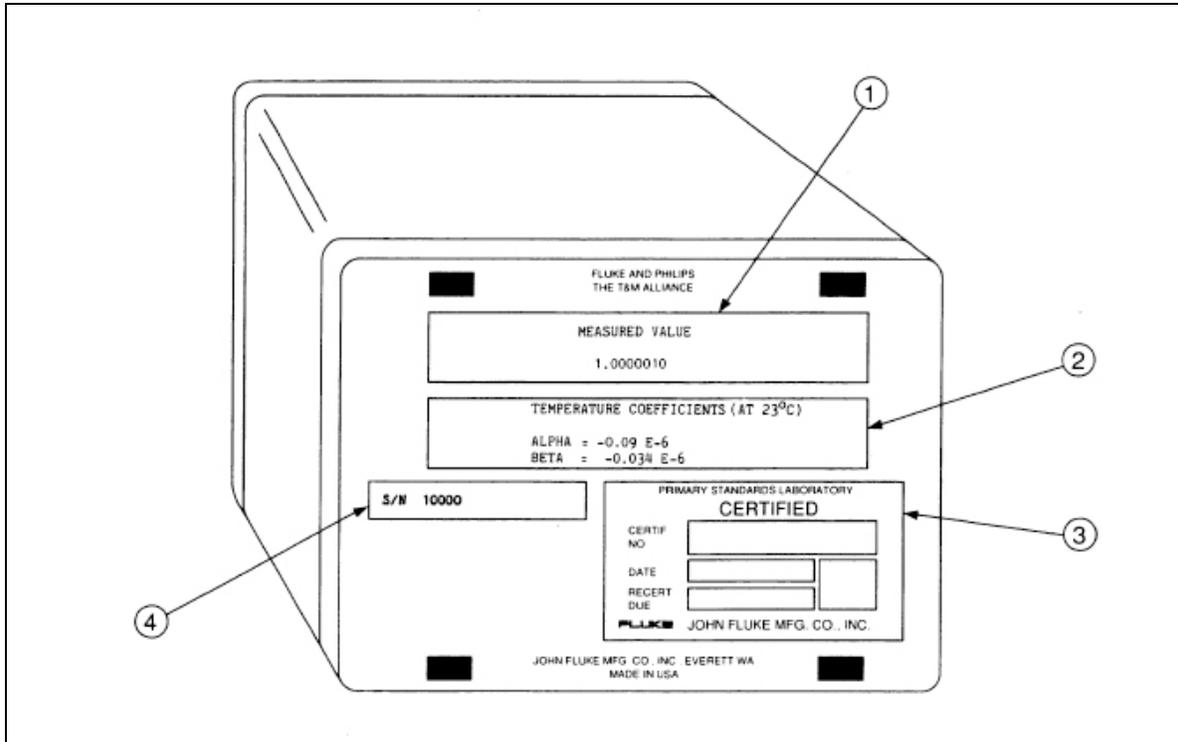

**Figure 2. Typical Rear Panel View**

**Table 3. Contents of the Rear Panel Labels**

Ref No.	Label Information
①	Measured value label. Shows the measured value at $23 \pm 0.6^\circ$ ; the same as on the Report of Calibration.
②	Temperature coefficient label. Shows alpha and beta centered on $23^\circ\text{C}$ . Refer to "How Temperature Correction Factors are Calculated," further on in this manual for definitions of alpha and beta, and the formula to predict exact resistance at different temperatures.
③	Fluke Primary Standards Lab Calibration Label documents traceability to the U.S. National Bureau of Standards.
④	Serial number label. Shows the standard's serial number. This number and the full model number (i.e., 742A-1) positively identify a particular unit.

## Operating Notes

This part of the manual explains operational and environmental considerations for the 742A Series. Follow these guidelines when operating or storing the resistance standard. Precautions for handling are under “Care and Maintenance.”

### Connecting to the 742A Series

#### ⚠ Caution

**Do not apply voltages above the maximum voltage printed on the front panel. Excessive voltage can cause a permanent shift in resistance values or damage.**

The specifications for models with CURRENT and SENSE binding posts require four-wire connections to the standard. Use these binding posts as described in Table 2.

For the case to act as a shield, the CHASSIS GROUND binding post must be connected to earth ground or instrumental guard at some point in a calibration system. Normally when two or more instruments with guards are connected together, the use of a single common grounding point avoids ground loops. If applicable, ground the 742A CHASSIS GROUND binding post to that common grounding point.

Figure 3 shows a typical connection to a four-wire ohmmeter. Figure 4 shows the connection used to calibrate the 1  $\Omega$  internal resistance standard in the 5700A.

### Cable Recommendations

For optimum results, use two sets of the Fluke 5440A-7004 Low Thermal Test Leads, which are designed to reduce errors caused by thermal emfs.

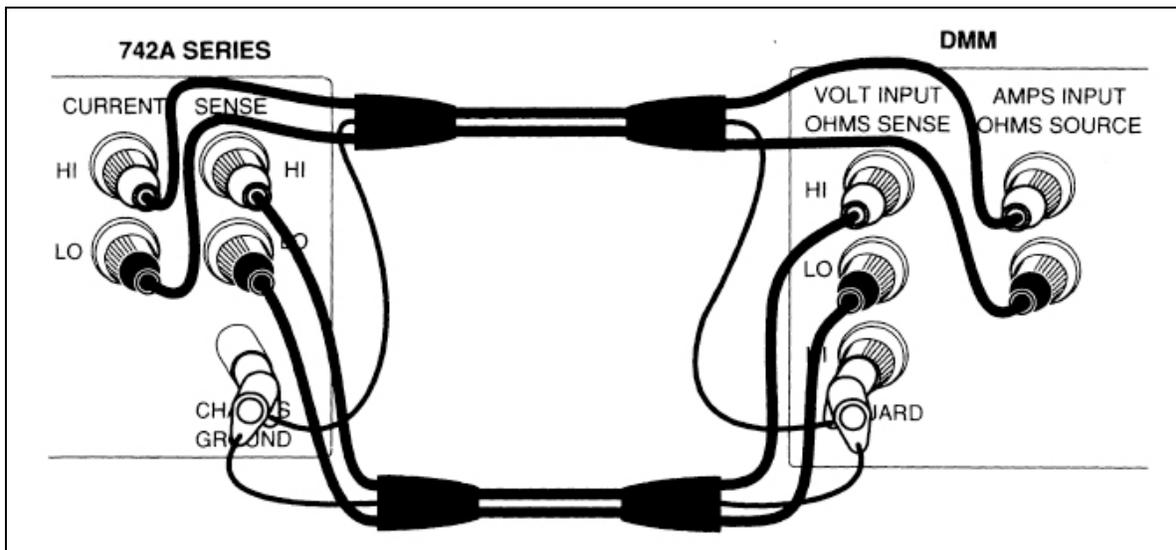


Figure 3. Connection to a Four-Wire Ohmmeter

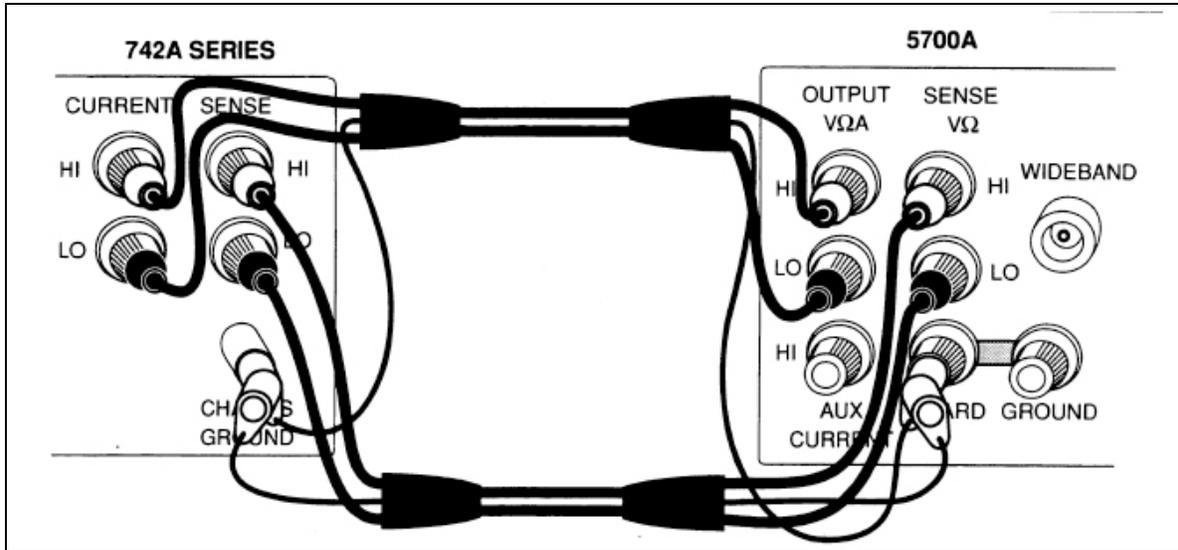


Figure 4. Connection to Calibrate the 5700A

### Operating Temperature Range

You can use the 742A Series in ambient temperatures between 18 and 28 °C. To predict the deviation from the nominal at temperatures other than 23 °C, use the temperature characterization table provided with each unit. The table shows the calculated value and the deviation from nominal at temperatures between 18 and 28 °C in half-degree increments. An example of this table is included as Table 4.

### How Temperature Correction Factors are Calculated

A label on the rear panel shows temperature coefficient factors alpha and beta centered on 23 °C. (See Figure 2 for the label location.) The values of alpha and beta are individualized for each 742A. Alpha and beta are established by measurement in the Fluke Primary Standards Lab at 18 °C, 23 °C, and 28 °C. The temperature characterization table is generated from these three measurements and the following formula:

$$R_t = R_{23} [1 + \alpha (t - 23) + \beta (t - 23)^2]$$

Where,  $R_t$  = Resistance at t°C

$R_{23}$  = Resistance at 23°C

$\alpha$  = Slope of the curve (ppm/°C) at 23°C

$\beta$  = Rate of change of slope of the curve (ppm/°C<sup>2</sup>)

$\alpha$  and  $\beta$  are constants which do not change appreciably over time and hence need to be determined only once.

In the case of the example 742A-1 used in this manual,  $\alpha$  and  $\beta$  are calculated as follows:

$$\alpha = \frac{(R_{28} - R_{18})}{\Delta t} = \frac{-0.9 \text{ E } - 6}{10} = -0.09 \text{ E } - 6$$

$$\beta = \frac{\frac{(R_{28} + R_{18})}{2} - R_{23}}{\left(\frac{\Delta t}{2}\right)^2} = \frac{-0.85 \text{ E } - 6}{25} = -0.034 \text{ E } - 6$$

Where,

$R_{28}$  = Resistance at 28 °C

$R_{18}$  = Resistance at 18 °C

$R_{23}$  = Resistance at 23 °C

$\Delta t$  = (28 - 18) = 10


**Table 4. Example 742A-1 Temperature Characterization Chart**

Test Number: XXXX	Serial No.: XXXXXX
Date: 04-Aug-88	Alpha = -0.090 E-6
Page 2 of 2	Beta = -0.034 E-6

Temp (Celsius)	Resistance (Ohms)	Dev from nominal (in ppm)
18.0	1.000006	0.6
18.5	1.000007	0.7
19.0	1.000008	0.8
19.5	1.000009	0.9
20.0	1.000010	1.0
20.5	1.000010	1.0
21.0	1.000010	1.0
21.5	1.000011	1.1
22.0	1.000011	1.1
22.5	1.000010	1.0
23.0	1.000010	1.0
23.5	1.000009	0.9
24.0	1.000009	0.9
24.5	1.000008	0.8
25.0	1.000007	0.7
25.5	1.000006	0.6
26.0	1.000004	0.4
26.5	1.000003	0.3
27.0	1.000001	0.1
27.5	0.999999	-0.1
28.0	0.999997	-0.3

Figure 5 shows a graph of the value of the 742A-1 represented by the sample temperature characterization chart (Table 4). To illustrate use of the formula, calculations for resistance at 20 °C and 26 °C are shown. You can see that using the formula shown with alpha and beta you get the same value as in the characterization table.

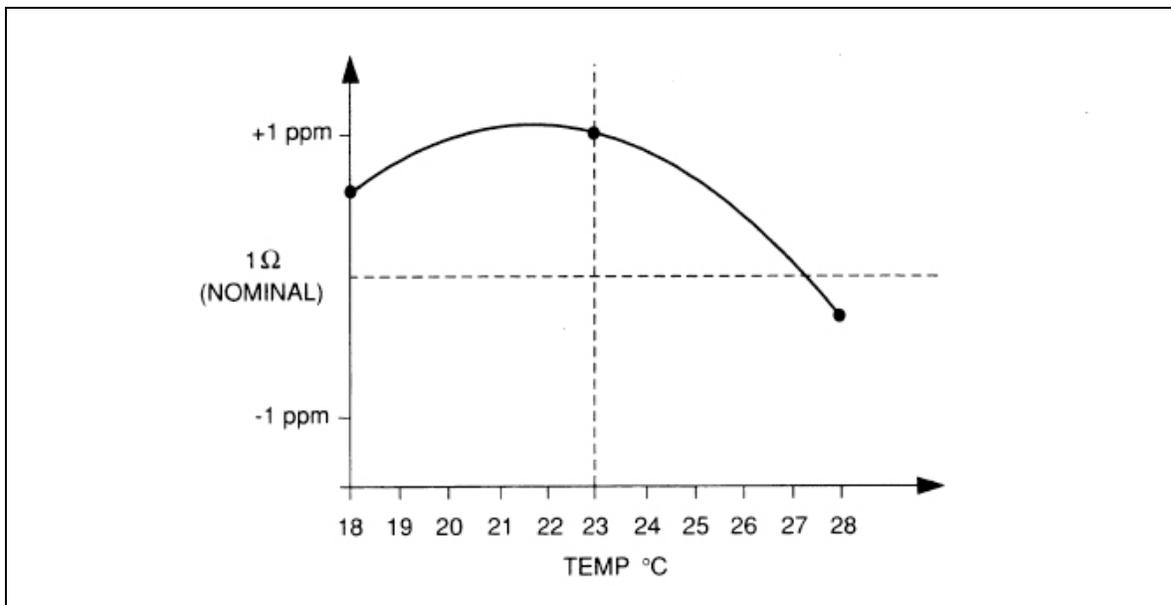

**Figure 5. Graph of Resistance VS. Temperature for Sample 742A-1**

$$\begin{aligned}
 R_t &= R_{23} [ 1 + \alpha (t - 23) + \beta (t - 23)^2 ] \\
 A_t &= 20 \text{ }^\circ\text{C}, \\
 R_{20} &= 1.00000010 [ 1 + (-0.09 \text{ E-}6) (-3) + (-0.034 \text{ E-}6) (-3)^2 ] \\
 &= 1.00000010 (1.0000003 - 0.0000003 ) \\
 &= 1.00000010 (1.0000000 ) \\
 &= 1.00000010 \text{ } \Omega
 \end{aligned}$$

$$\begin{aligned}
 R_t &= R_{23} [ 1 + \alpha (t - 23) + \beta (t - 23)^2 ] \\
 A_t &= 26 \text{ }^\circ\text{C}, \\
 R_{26} &= 1.00000010 [ 1 + (-0.09 \text{ E-}6) (3) + (-0.034 \text{ E-}6) (3)^2 ] \\
 &= 1.00000010 (1 - 0.0000003 - 0.0000003 ) \\
 &= 1.00000010 (1 - 0.0000006 ) \\
 &= 1.00000004 \text{ } \Omega
 \end{aligned}$$

**Storage Temperature Range**

To maintain accuracy within the specified limits, do not subject the 742A Series to temperatures below 0 °C or above 40 °C. If exposure to temperatures outside this range is unavoidable, you can minimize the adverse effects by doing the following:

- Keep the standards in the optional transit case (Option 742A-7002). The transit case is insulated and helps protect the standards during short-term temperature extremes.
- Keep exposure to temperature extremes brief.

## **Care and Maintenance**

The only maintenance procedure for the 742A Series is occasional cleaning. The following text gives cleaning instructions and precautions for handling.

### **Cleaning the 742A Series**

To keep the 742A Series looking like new, clean the outer surfaces using a soft cloth slightly dampened with water or a non-abrasive mild cleaning solution that does not harm plastics.

#### **⚠ Caution**

**Do not use aromatic hydrocarbons or chlorinated solvents for cleaning. They can damage the plastic materials used in the resistance standard.**

### **Precautions for Handling**

The 742A Series are designed for mechanical stability, but do not abuse the standard with excessive shock. Avoid temperature extremes as mentioned under “Storage Temperature Range”. When you transport the standard, it is recommended that you use the Option 742A-7002 Transit Case for shock and temperature protection. The case holds two 742A Series Resistance Standards.

## **Servicing Information**

Because the 742A Series are certified and non-adjustable resistance standards, they are considered non-user repairable. If the unit is damaged, it must be returned to the factory for repair and calibration.

## **Recertification**

For recertification, send the resistance standard to a Fluke technical center. For a nominal fee, Fluke will remeasure and recertify the value of our 742A based on comparison to standards traceable to the U.S. National Bureau of Standards. A new temperature characterization chart is provided on recertification. If you wish, you can record the changes at each recertification and use this data to more closely predict the performance of you 742A.

