Reference EMI Receiver Series

HP 8542E/HP 8546A EMI Receiver HP 85422E/HP 85462A Receiver RF Section



Notice

The information contained in this document is subject to change without notice.

Hewlett-Packard makes no warranty of any kind with regard to this material, including but not limited to, the implied warranties of merchantability and fitness for a particular purpose. Hewlett-Packard shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

[©] Copyright Hewlett-Packard Company 1994, 1995, 1996, 1999 All Rights Reserved. Reproduction, adaptation, or translation without prior written permission is prohibited, except as allowed under the copyright laws.

Certification

Hewlett-Packard Company certifies that this product met its published specifications at the time of shipment from the factory. Hewlett-Packard further certifies that its calibration measurements are traceable to the United States National Institute of Standards and Technology, to the extent allowed by the Institute's calibration facility, and to the calibration facilities of other International Standards Organization members.

Regulatory Information

Regulatory information is located in the *EMI Receiver Series Reference* at the end of Chapter 1, "Specifications and Characteristics."

Warranty

This Hewlett-Packard instrument product is warranted against defects in material and workmanship for a period of one year from date of shipment. During the warranty period, Hewlett-Packard Company will, at its option, either repair or replace products which prove to be defective.

For warranty service or repair, this product must be returned to a service facility designated by Hewlett-Packard. Buyer shall prepay shipping charges to Hewlett-Packard and Hewlett-Packard shall pay shipping charges to return the product to Buyer. However, Buyer shall pay all shipping charges, duties, and taxes for products returned to Hewlett-Packard from another country.

Hewlett-Packard warrants that its software and firmware designated by Hewlett-Packard for use with an instrument will execute its programming instructions when properly installed on that instrument. Hewlett-Packard does not warrant that the operation of the instrument, or software, or firmware will be uninterrupted or error-free.

LIMITATION OF WARRANTY

The foregoing warranty shall not apply to defects resulting from improper or inadequate maintenance by Buyer, Buyer-supplied software or interfacing, unauthorized modification or misuse, operation outside of the environmental specifications for the product, or improper site preparation or maintenance.

NO OTHER WARRANTY IS EXPRESSED OR IMPLIED. HEWLETT-PACKARD SPECIFICALLY DISCLAIMS THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.

EXCLUSIVE REMEDIES

THE REMEDIES PROVIDED HEREIN ARE BUYER'S SOLE AND EXCLUSIVE REMEDIES. HEWLETT-PACKARD SHALL NOT BE LIABLE FOR ANY DIRECT, INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, WHETHER BASED ON CONTRACT, TORT, OR ANY OTHER LEGAL THEORY.

Assistance

Product maintenance agreements and other customer assistance agreements are available for Hewlett-Packard products. For any assistance, contact your nearest Hewlett-Packard Sales and Service Office.

Compliance

This instrument has been designed and tested in accordance with IEC Publication 348, Safety Requirements for Electronic Measuring Apparatus, and has been supplied in a safe condition. The instruction documentation contains information and warnings which must be followed by the user to ensure safe operation and to maintain the instrument in a safe condition.

Safety Notes

The following safety notes are used throughout this manual. Familiarize yourself with each of the notes and its meaning before operating this instrument.

WARNING

Warning denotes a hazard. It calls attention to a procedure which, if not correctly performed or adhered to, could result in injury or loss of life. Do *not* proceed beyond a warning note until the indicated conditions are fully understood and met.

CAUTION

Caution denotes a hazard. It calls attention to a procedure that, if not correctly performed or adhered to, would result in damage to or destruction of the instrument. Do *not* proceed beyond a caution sign until the indicated conditions are fully understood and met.

General Safety Considerations

WARNING

- No operator serviceable parts inside. Refer servicing to qualified personnel. To prevent electrical shock, do not remove covers.
- If this instrument is used in a manner not specified by Hewlett-Packard Company, the protection provided by the instrument may be impaired.
- For continued protection against fire hazard, replace line fuse only with same type and rating ([F 5A/250V]). The use of other fuses or material is prohibited.

CAUTION

- Before switching on this instrument, make sure that the line voltage selector switch is set to the voltage of the power supply and the correct fuse is installed.
- Always use the three-prong ac power cord supplied with this instrument. Failure to ensure adequate earth grounding by not using this cord may cause instrument damage.



The instruction documentation symbol. The product is marked with this symbol when it is necessary for the user to refer to the instructions in the documentation.

CE

The CE mark is a registered trademark of the European Community. (If accompanied by a year, it is when the design was proven.)

ISM1-A

This is a symbol of an Industrial Scientific and Medical Group 1 Class A product.

CSA

The CSA mark is a registered trademark of the Canadian Standards Association.

Manual Conventions

(Front-Panel Key)

This represents a key physically located on the instrument.

Softkey

This indicates a "softkey," a key whose label is determined by the firmware of the instrument.

Screen Text

This indicates text displayed on the instrument's screen.

EMI Receiver Series Documentation Description

The following documents are provided with either the HP 8542E/HP 8546A EMI receiver or the HP 85422E/HP 85462A receiver RF section.

- Installation and Verification provides information for installing your instrument, verifying instrument operation, and customer support.
- *User's Guide* describes instrument features and how to make measurements with your EMI receiver or receiver RF section.
- Reference provides specifications and characteristics, menu maps, error messages, and key descriptions.
- Programmer's Guide provides information on remote control instrument configuration, creating programs, and parameters for each of the programming commands available.

Contents

,	Definitions of Terms
,	General Specifications: HP 8542E EMI Receiver
(General Specifications: HP 8542E EMI Receiver
	(continued)
(General Specifications: HP 8542E EMI Receiver
	(continued)
η	Tuning Specifications
ç	Swept Frequency Specifications
1	Amplitude Specifications
-	Amplitude Specifications (continued)
	Amplitude Specifications (continued)
	Amplitude Specifications (continued)
	Amplitude Specifications (continued)
,	Amplitude Specifications (continued)
n	Cracking Generator Specifications
Ţ	Frequency Characteristics
1	Amplitude Characteristics
r	Tracking Generator Characteristics
	Physical Characteristics
	Physical Characteristics (continued)
	General Specifications: HP 85422E Receiver RF Section .
	General Specifications: HP 85422E Receiver RF Section
•	
η	(continued)
	(continued)
5	(continued)
5	(continued)
5	(continued)
	(continued)
	(continued)
	(continued) Funing Specifications Swept Frequency Specifications Amplitude Specifications Amplitude Specifications (continued) Amplitude Specifications (continued) Amplitude Specifications (continued) Tracking Generator Specifications
	(continued)
S	(continued) Funing Specifications Swept Frequency Specifications Amplitude Specifications Amplitude Specifications (continued) Amplitude Specifications (continued) Aracking Generator Specifications Bracking Generator Specifications (continued) Brequency Characteristics
	(continued)
	(continued) Funing Specifications Swept Frequency Specifications Amplitude Specifications Amplitude Specifications (continued) Amplitude Specifications (continued) Fracking Generator Specifications Fracking Generator Specifications (continued) Frequency Characteristics Amplitude Characteristics (continued)
	(continued) Cuning Specifications Swept Frequency Specifications Amplitude Specifications Amplitude Specifications (continued) Amplitude Specifications (continued) Amplitude Specifications (continued) Cracking Generator Specifications Cracking Generator Specifications (continued) Cracking Generator Specifications (continued) Cracking Characteristics Amplitude Characteristics (continued) Cracking Generator Characteristics
	(continued) Funing Specifications Swept Frequency Specifications Amplitude Specifications (continued) Amplitude Specifications (continued) Amplitude Specifications (continued) Fracking Generator Specifications Fracking Generator Specifications (continued) Frequency Characteristics Amplitude Characteristics Amplitude Characteristics Fracking Generator Characteristics Chysical Characteristics
	(continued) Cuning Specifications Swept Frequency Specifications Amplitude Specifications Amplitude Specifications (continued) Amplitude Specifications (continued) Amplitude Specifications (continued) Cracking Generator Specifications Cracking Generator Specifications (continued) Cracking Generator Specifications (continued) Cracking Characteristics Amplitude Characteristics (continued) Cracking Generator Characteristics

2.	HP 8546A/HP 85462A Specifications and Characterist	
	Definitions of Terms	
	General Specifications: HP 8546A EMI Receiver	2-2
	General Specifications: HP 8546A EMI Receiver	
	(continued)	2-3
	General Specifications: HP 8546A EMI Receiver	
	(continued)	. 2-4
	Tuning Specifications	2-5
	Swept Frequency Specifications	
	Amplitude Specifications	2-7
	Amplitude Specifications (continued)	2-8
	Amplitude Specifications (continued)	
	Amplitude Specifications (continued)	
	Amplitude Specifications (continued)	2-11
	Amplitude Specifications (continued)	
	Tracking Generator Specifications	2-13
	Frequency Characteristics	
	Amplitude Characteristics	2-15
	Tracking Generator Characteristics	$\frac{1}{2-16}$
	Physical Characteristics	
	Physical Characteristics (continued)	
	General Specifications: HP 85462A Receiver RF Section	
	General Specifications: HP 85462A Receiver RF Section	. 220
	(continued)	2-21
	Tuning Specifications	
	Swept Frequency Specifications	$\frac{2-22}{2-23}$
	Amplitude Specifications	2-23
	Amplitude Specifications (continued)	$\frac{2-24}{2-25}$
	Amplitude Specifications (continued)	$\frac{2-25}{2-26}$
	Amplitude Specifications (continued)	2-20 2-27
	Amplitude Specifications (continued)	2-27
	Tracking Generator Specifications	
	Tracking Generator Specifications (continued)	
	Frequency Characteristics	
	Amplitude Characteristics	
	Amplitude Characteristics (continued)	
	Tracking Generator Characteristics	2-34
	Physical Characteristics	
	Physical Characteristics (continued)	2-36
	Regulatory Information	
	Notice for Germany: Noise Declaration	2-40
3.	Key Menus	
	User Defined Keys	. 3-1
	W Dr. C. D. C.	
4.	Key Dictionary Reference	4.0
	Service Functions	4-2
	Service Calibration Functions	
	Service Diagnostic Functions	
	Key Functions	
	% AM	. 4-4
	ϕ LOCKON OFF	. 4-4
	μ A/m	. 4-5
	11 V/m	4-5

0-2.9 Gz BAND 0 .																4-5
2v REF DETECTOR .																4-6
2.75-6.5 BAND 1 .																4-6
3 dB POINTS																4-7
3rd ORD MEAS																4-7
6 dB POINTS																4-8
9 kHz - 150 kHz .																4-8
9 kHz EMI BW																4-8
+10V REF DETECTOR																4-9
-10V REF DETECTOR																4-9
30 MHz - 300 MHz .																4-9
99% PWR BW																4-10
120 kHz EMI BW																4-10
150 kHz - 30 MHz .																4-10
200 Hz EMI BW																4-11
200 MHz - 1 GHz .																4-11
A<>B																4-11
A-B -> A ON OFF .																4-12
A -> C																4-12
ABCDEF																4-13
ABORT																4-13
ACTIVE																4-13
ADD TO LIST																4-13
Adjust Color																4-14
ADVISORY																4-14
ALC INT EXT																4-14
AMPL SCL LOG LIN .																4-15
(AMPLITUDE)			•													4-15
Amptd Units			•	•	•	•	•	•	•	•	•	•	•	•	•	4-16
ANNOTATN			•	•	•	•	•	•	•	•	•	•	•	•	•	4-16
ANNOTATN ON OFF .				•	•	•	•	•	•	•	•	•		•	•	4-16
ANTENNA -> DISK .	•														•	4-17
Antenna Factors .			•	•					•		•				•	4-17
ANTENNA ON OFF			•	•					•			•		•	•	4-17
Antenna Units			•	•	•	•	•	•	•	•	•	•		•	•	4-18
APND CAT ITEM			•	•					•		•				•	4-18
ATTEN AUTO MAN			•	•	•			•	•	•	•				•	4-18
AUTO ALL			•													4-19
AUTO CAL ON OFF .																4-19
(AUTO COUPLE)	•		•	•	•	•	•	•	•	•	•	٠	•	٠	•	4-20
AUTO-MEASURE																4-20

(AUTO RANGE)		•	•	•		•		•						•		•	4-21
AUTOEXEC ON OFF	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-21
AUTORANG ON OFF	٠																4-21
Aux Conn Control																	4-22
(AUX CTRL)				•						•		•		•		•	4-22
AV DWELL TIME .	•															•	4-22
(AVERAGE)	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	٠	4-23
AVG BW AUTO MAN	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	4-23
AV/IF BW RATIO .	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	4-23
B -> C	•			•									٠	•		•	4-24
B <> C										•		•					4-24
B-DL -> B																	4-24
BACKGRND																	4-24
Band Lock																	4-25
BAUD RATE																	4-25
BLACK FILL																	4-26
BLACK LEVEL																	4-26
BLANK A																	4-26
BLANK B	-	-		-		-		-		-		-	-	-		-	4-27
BLANK C	·		•		•		•		•	•	•	•	•		•		4-27
BLUE		•	•	•	•	•	•	•	•	•	•	•	•	•	•		4-27
BLUE FILL	٠	•	•	•	•	•	•	•	•	•	•	•	٠	•	•	•	4-27
	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-28
	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	
BRIGHT	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	4-28 4-29
CABLE -> DISK .	•	•	•	•	•	•	•	•	•	•	•	•	٠	•	•	•	4-29 4-29
Cable Factors .	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-29
	•	•	•	•	•	•	•	•	•	•	•	•	٠	•	•	•	4-30
CABLE ON OFF	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	
CAL 85422	•	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	4-30
CAL 85462	٠	٠	•	٠	•	٠	•	٠	•	•	•	•	٠	٠	•	•	4-30
CAL ALL	٠	•	•	•	•	•	•	•	•	•	•	•	٠	•		•	4-30
CAL AMP										•		•				•	4-31
Cal At Time										•		•					4-31
(CAL CHECK)	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-31
CAL FETCH	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	4-31
CAL FREQ	•			•									٠	•		•	4-32
(CALIBRATE)	٠	٠	•	•	•	٠	•	٠	•	•	•	•	٠	•	•	•	4-32
CAL INPUT 1	٠	٠	•	٠	•	٠	•	٠	•	•	•	•	٠	٠	•	•	4-32
CAL INPUT 2	•	•	•	•	•	•	•	•	•	•	•	•	٠	•		•	4-32
CAL MXR		•		•	•	•	•	•	•		•			•		•	4-33
CAL STORE																•	4-33
CAL TIMEBASE																	4-33

CAL TRK GEN																	4-34
CAL YTF																	4-34
CATALOG ALL																	4-34
CATALOG DISK																	4-35
Catalog Internal																	4-35
CATALOG PREFIX .																	4-37
CATALOG REGISTER																	4-37
CATALOG VARIABLS																	4-38
CENTER FREQ																	4-38
CF STEP AUTO MAN																•	4-38
Change Prefix .																	4-39
Change Title																•	4-40
CLEAR ANNOTATN .																•	4-41
CLEAR MARK																	4-41
CLEAR WRITE A .																•	4-41
CLEAR WRITE B .																	4-42
CLEAR WRITE C .																	4-43
CLR ALL MARKS .																	4-43
CNTL A O 1																	4-44
CNTL B O 1																	4-44
CNTL C O 1																	4-44
CNTL D O 1																	4-45
COARSE TUNE DAC																	4-45
COLOR BARS																	4-45
COLOR MONOCHRM .																	4-46
COMPLMNT MARKS .																	4-46
CONFIG									•	•						•	4-46
CONFIG DONE	•	•	٠	•	•	•	•	•	•	•	•	٠	•	•	•	•	4-47 4-47
COPY DEV PRNT PLT	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-47
COPY SCREEN		•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-50
CORRECT ON OFF .	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-50
Correctn Factors	•	•	•	٠	•	•	•	•	•	•	•	•	•	•	•	•	4-50
CORRECTN ON OFF	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-51
COUPLE AC DC	•	•	•	٠	•	•	•	•	•	•	•	•	•	•	•	•	4-51
CNT RES AUTO MAN	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-51
(CTRL)						•					•		•	•			4-52
DACS																	4-53
DATEMODE MDY DMY																	4-53
dBm																	4-53
dBmV																	4-54

$\mathtt{dB}\mu\mathtt{V}$	•										4-54
DEFAULT CAL DATA											4-54
DEFAULT COLORS .											4-55
DEFAULT CONFIG .											4-55
Define List											4-56
Define Report .											4-56
DEFINE USER KEY											4-56
DELETE ALL SIGS										•	4-57
DELETE FACTORS .										•	4-57
DELETE FILE											4-57
DELETE LIMIT										•	4-59
DELETE MARKED .										•	4-59
DELETE POINT											4-59
DELETE SEGMENT .											4-60
DELETE SIGNAL .											4-60
Delete Signals .										•	4-61
DELTA MEAS										•	4-61
DEMOD AM FM											4-61
DEMOD ON OFF											4-62
DESKJET											4-62
DESKJET 500										•	4-62
DESKJET 500C											4-63
DESKJET 550C										•	4-63
DETECTOR PK QP AV	000 000 000 000 000 000										4-63
DETECTOR SMP PK										•	4-64
Disk Config											4-64
DISPLAY)				•							4-64
DISPLAY -> DISK		•								•	4-65
DISPLAY CAL DATA		•									4-65
DISPLAY CNTL I .											4-65
Display Config .											4-66
Display Sys Data											4-66
DISPOSE USER KEY											4-66
Dispose User Mem											4-66
DR00P											4-67
DSP LINE ON OFF											4-67
DWELL TIME										•	4-68
EDIT ANNOTATN .											4-68
EDIT ANTENNA											4-68
EDIT CABLE											4-69

EDIT CAT ITEM .		•					٠			4-69
Edit Colors	•	•							•	4-69
EDIT DONE									•	4-70
EDIT FLATNESS .										4-71
EDIT LAST										4-71
Edit Limit										4-72
EDIT LIMIT										4-72
EDIT LIST										4-72
EDIT LOWER		•							•	4-73
EDIT MID/DELT .										4-73
EDIT OTHER										4-74
EDIT PA FLTNESS										4-74
EDIT UP/LOW										4-74
EDIT UPPER										4-75
EDIT UPR LWR										4-75
Editor										4-76
EMI RECEIVER										4-76
EPSON MX										4-77
ERASE STATEALL .										4-77
ERASE TRACEALL .										4-77
ERRORS										4-77
EXECUTE TITLE .										4-78
EXIT		•							•	4-78
EXIT CATALOG										4-78
EXIT EDIT										4-79
EXIT GRAPH										4-79
EXIT LAST CAL .										4-80
EXIT MEASURE										4-80
EXIT SHOW										4-80
EXTERNAL										4-81
EXTERNAL PREAMPG										4-81
FAST STP ON OFF										4-81
FFT MEAS										4-82
FINE TUNE DAC .		•							•	4-82
FLAT										4-83
Flatness Data .		•							•	4-83
FM COIL DRIVE .										4-84
FM GAIN										4-84
FM OFFSET										4-84
FM SPAN										4-85

FORMAT DOS DISK .												4-85
FORMAT LIF DISK .												4-85
FREE RUN				•		•						4-86
FREQ DIAG				•		•						4-86
FRQ DISC NORM OFF				•		•						4-86
FREQ OFFSET				•		•						4-87
FREQ SCL LOG LIN .												4-87
FREQ STEP												4-88
(FREQUENCY)												4-88
FRQ SCAN ON OFF .									•		•	4-89
FULL SPAN				•		•						4-89
FULL WHITE				•		•						4-89
Gauss				•		•						4-90
GEO DST TEST												4-90
GHIJKL				•		•						4-90
GND REF DETECTOR .												4-90
GRAT ON OFF												4-91
GRATICUL												4-91
GRAY SCALE												4-91
GREEN												4-92
GREEN FILL				•		•						4-92
GRID												4-92
HALF FILL												4-93
HI VOLT TEST												4-93
HOLD												4-93
HORIZ LINES												4-93
HSL RGB												4-94
HUE												4-94
IDNUM												4-94
IF BW AUTO MAN												4-95
IF GAINS												4-95
INIT FLT												4-95
INPT LCK ON OFF .												4-96
(INPUT)												4-96
Input	•											4-96
INPUT 1												4-96
INPUT 1 9k-50M												4-97
INPUT 1 PREAMP				•	•	•	•	•		•		4-97
INPUT 2				•	•	•	•	•		•		4-97
INPUT 2 20M-2.9G .												4-97
INPUT 2 1-6.5G												4-98

INPUT 2 BYPASS	4-98
INPUT 2 PREAMP	4-98
INPUT Z 50Ω 75Ω	4-99
Inst Setup	4-99
INTENSITY	4-99
INTERNAL -> STATE	4-100
Internal -> Trace	4-100
LASERJET	4-101
LASERJET II	4-101
LASERJET III	4-101
Last Cal	4-101
Last Hrd Key Menu	4-102
LAST SPAN	4-102
Limit 1	4-102
LIMIT 1 ON OFF	4-103
Limit 2	4-103
LIMIT 2 ON OFF	4-103
LIMIT LINE 1	4-104
Limit Lines	4-104
LIMIT LINES	4-104
LIMITS -> DISK	4-105
LIMITS FIX REL	4-105
LIMITS FRQ TIME	4-106
LINE	4-107
LINEARITY	4-107
(LINEARITY CHECK)	4-107
LIN ON OFF	4-107
LIST -> DISK	4-108
LIST ON OFF	4-108
LMT DISP Y N AUTO	4-108
LMT TEST ON OFF	4-109
	4-109
2000000 000000000000000000000000000000	4-110
	4-111
	4-111
	4-111
MAIN COIL DR	4-112
	4-112
	4-112
MARGIN 1 ON OFF	4-113
MARGIN 2 ON OFF	4-113

MARK ALL DUPLICAT														4-113
MARK ALL SIGNALS .	ı													4-114
MARK LWR DUPLICAT														4-114
MARK SIGNAL														4-114
MARK TO END	,													4-114
MARKER	i													4-115
MARKER Δ	ı													4-115
MARKER ΔSPAN	ı													4-116
MARKER ->CF														4-116
MARKER ->CF STEP .	ı													4-116
MARKER-> MINIMUM .														4-117
MARKER ->PK-PK														4-117
MARKER ->REF LVL .	i													4-117
MARKER ->START		٠												4-118
MARKER ->STOP	,													4-118
MARKER 1 ON OFF .	,													4-118
MARKER 2 ON OFF .														4-118
MARKER 3 ON OFF .	,													4-119
MARKER 4 ON OFF .														4-119
MARKER ALL OFF														4-119
MARKER AMPTD														4-120
(MARKER FUNCTION)	į													4-120
MARKER NORMAL	,													4-120
MARKERS	,													4-121
MARKER TUNE SPN .	i													4-121
MAX HOLD A	i													4-122
MAX HOLD B	ı													4-122
MAX MXR LVL	i													4-122
MEAS SNG CONT	,													4-123
MEAS STEPPED	į													4-123
(MEAS/USER)					•									4-123
MEASURE AT MKR	,				•								•	4-124
Measure Detector .	ı									•	•		•	4-124
MEM LOCKED						•					٠	•	•	4-124
MIN HOLD C	ı	٠		•						•				4-125
MIXER BIAS DAC	,												•	4-125
MK COUNT ON OFF .	į					•						•		4-125
MK NOISE ON OFF .														4-126
MK PAUSE ON OFF .	,											•		4-126
MKR	ı	•	•	٠	•	•	•	•	•	٠	٠	•	•	4-126
(MKR ->)														4-127

MK READ F T I P									4-127
MK TRACE AUTO ABC									4-127
MK TRACK ON OFF									4-128
MNOPQR									4-128
(MODE)									4-129
MONO-CHROME									4-129
NEW EDIT									4-129
(NEXT)									4-130
NEXT PAGE							•	•	4-130
NEXT PEAK									4-130
NEXT PK LEFT									4-130
NEXT PK RIGHT .									4-131
NO CONVERSN									4-131
No User Menus .									4-131
NORMLIZE ON OFF									4-132
NORMLIZE POSITION									4-132
(ON/OFF)									4-132
OPTICAL FILTER .									4-133
OTHER -> DISK .									4-133
Other Factors .									4-133
OTHER ON OFF									4-134
(<u>OUTPUT</u>)									4-134
OUTPUT REPORT .								•	4-134
OVLD ON OFF									4-134
PAINTJET									4-135
PALETTE BARS									4-135
PEAK EXCURSN									4-135
Peak Menu									4-136
(PEAK SEARCH)									4-136
PK DWELL TIME .									4-136
PK-PK MEAS									4-137
Plot Config									4-137
PLOTTER ADDRESS									4-137
PLT MENU ON OFF									4-138
PLTS/PG 1 2 4 .									4-138
POINT									4-138
POWER ON IP LAST									4-139
(PREAMP)									4-140
PREAMP ON OFF .									4-140
PRESEL DAC									4-141
PRESEL DEFAULT .									4-141
PRESEL PEAK									4-141

(<u>PRESET</u>)													4-142
PRESET RECEIVER													4-145
PRESET SPECTRUM													4-146
Print Config													4-148
Print Options .													4-148
PRINTER ADDRESS													4-148
PRINTER SETUP .													4-148
Printer Type							•						4-149
PROTECT ON OFF .													4-149
PRN/PG 1 2							•						4-149
PRT MENU ON OFF	•												4-150
pTesla													4-150
PURGE LIMITS	•												4-150
PWR SWP ON OFF .	•												4-151
QP/AVG 10X OFF .							•						4-152
QP DET ON OFF .							•						4-152
QP DWELL TIME .							•						4-152
QP GAIN ON OFF .													4-153
QPD OFFSET													4-153
QPD RST ON OFF .													4-153
(QUASI-PEAK)													4-154
QUIETJET				•							•		4-154
(RECALL)			٠	•		٠				٠	•		4-154
RECALL ANTENNA .		•	•	•				•	•		•	•	4-154
RECALL CABLE													4-155
RECALL COLORS .													4-155
Recall Disk													4-155
Recall Internal													4-156
RECALL LIMITS .													4-156
RECALL LIST													4-156
RECALL OTHER							•						4-157
RECALL SETUP													4-157
RECALL TRACE													4-157
RECEIVER ADDRESS													4-158
RED	•												4-158
RED FILL							•						4-158
REF LVL													4-158
REF LVL OFFSET .													4-159
REMEAS ALL SIGS							•						4-159
REMEAS MARKED .													4-160
REMEAS SIGNAL .													4-160

Re-measure									4-160
RESOLUTN LOW HIGH									4-161
RESTART									4-161
SATUR-ATION									4-161
(SAVE)									4-162
SAVE ANTENNA									4-162
SAVE CABLE	•								4-162
SAVE COLORS								•	4-163
Save Disk									4-163
SAVE EDIT									4-163
Save Internal									4-164
SAVE LIMITS									4-164
SAVE LIN GRAPH									4-164
SAVE LIST									4-165
SAVE LOG GRAPH									4-165
SAVE OTHER									4-166
Save/Rcl List									4-166
SAVE SETUP									4-166
SAV LOCK ON OFF .									4-167
SCALE LOG LIN									4-167
(SELECT)	•								4-168
SELECT 1 2 3 4								•	4-168
SELECT AMPLITUD .									4-168
Select Axis									4-169
SELECT DELT AMP .									4-169
SELECT FREQ									4-170
SELECT FRM LIST .									4-171
SELECT LWR AMPL .									4-171
SELECT MID AMPL .								•	4-171
SELECT POINT									4-172
SELECT PREFIX									4-172
SELECT SEGMENT									4-173
Select Type									4-174
SELECT UPR AMPL .									4-175
Selectv Mark									4-175
Service Cal									4-176
Service Diag									4-176
SET ATTN ERROR									4-176
SET DATE									4-176
SET TIME									4-177
SETTINGS ON OFF .									4-177

(affilia)																	4 177
SETUP -> DISK .	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	•	4-177 4-178
SHOW Δ1 PK QP AV	•	•	•	•	•		•	•	•	•		•	•	•	•	•	4-178
SHOW A2 PK QP AV	•	•	•	•	•		•	•	•	•		•	•	•	•	•	4-178
SHOW COR ON OFF	•	•	•	•	•		•	•	•	•		•	•	•	•	•	4-179
SHOW DET PK QP AV	•	•	•	•	•		•					•		•	•		4-179
SHOW MKR ON OFF																	4-179
SHOW SETUP																	4-180
SHW INST CONFIG																	4-180
SIG LIST ON OFF																	4-180
SIGNAL ANALYSIS																	4-181
Signal Marking .																	4-181
(SINGLE)																	4-181
SLOPE																	4-181
SOFTKEYS																	4-182
SORT BY AVG AMP																	4-182
SORT BY FREQ												٠					4-182
SORT BY DLTA LIM																	4-183
SORT BY PK AMP .																	4-183
SORT BY QP AMP .																	4-183
Sort Signals																	4-183
(SPAN) or SPAN																	4-184
SPAN ZOOM																	4-184
SPEAKER ON OFF .																	4-185
Special Colors .																	4-185
SQUELCH																	4-185
SRC ATN MAN AUTO																	4-186
SRC PWR OFFSET .																	4-186
SRC PWR ON OFF .																	4-186
SRC PWR STP SIZE																	4-187
START FREQ																	4-187
STATE -> INTRNL																	4-187
STATUS			•				•	•							•		4-188
STEP LOG LIN																	4-188
STOP			•				•	•							•		4-188
STOP FREQ																	4-188
STORE FLATNESS .			•				•	•							•		4-189
STOR PWR ON UNITS													•				4-189
STP GAIN ZERO .																•	4-189
STUVWX							•									•	4-190
(SWEEP)																	4-190

SWEEP CONT SGL .																	4-190
SWEEP LOG LIN .																	4-190
SWEEP RAMP																	4-191
SWEEP TIME DAC .																	4-191
SWP CPLG SR RECV																	4-191
SWP TIME AUTO MAN																	4-192
(TEST)																	4-192
Test Patterns .																	4-192
THINKJET																	4-193
THRESHLD ON OFF																	4-193
Time Date																	4-193
TIMEDATE ON OFF																	4-194
(TRACE)																•	4-194
TRACE A B C		•														•	4-194
TRACE A																•	4-195
TRACE B																	4-195
TRACE C																	4-196
Trace -> Disk .																	4-196
Trace -> Intrnl																	4-197
(TRACK GEN)																	4-197
TRACKING PEAK .																•	4-197
(TRIG)		•	•	•	•	•	•	٠	•	•	•	•	•	•	•	•	4-198
TUNE SLO FAST .	•	•	•	•	•	•	•	٠	•	•	•	•	•	•	•	•	4-198
UNDO	•	•	٠	•	٠	٠	•	•	٠	٠	٠	•	•	•	•	•	4-198
VERT LINES		•	٠	•	٠	٠	•	•	٠	٠	٠	•	•	•	•	•	4-199
User Menus		•	•		•	•	•	•	•	•	•	•	•		•	•	4-199
VID AVG ON OFF .									•			•	•		•		4-199
VIDEO									•								4-200
VIEW Δ OFF																•	4-200
VIEW A																	4-200
VIEW B																	4-201
VIEW C																	4-201
VIEW CAL ON OFF																	4-201
VIEW PK QP AV .																	4-202
VISION ENHANCE1																	4-202
VISION ENHANCE2																	4-202
Volts																	4-203
Watts																	4-203
WHITE DOTS																	4-203
WHITE FILL																	4-203
WINDOWS OFF																	4.004
		•	•	•	•	•	•	•	•	•	•	-	-	•	-	•	

	X FINE TUNE DAC	4-204
	YTF DRIVER	4-204
	YTF SPAN	4-205
	YTF TUNE COARSE	4-205
	YTF TUNE FINE	4-205
	YZ_# Spc Clear	4-206
	ZERO SPAN	4-206
	ZONE CENTER	4-206
	ZONE PK LEFT	4-207
	ZONE PK RIGHT	4-207
	ZONE SPAN	4-208
	(ZOOM)	4-208
5.	Error Messages Nonrecoverable System Errors	5-14
A.	SRQ	
	Service Requests	A-1 A-1
	Status Byte Definition	A-3
	Index	

Figures

	1-2. HP 85422E Receiver RF Section Dimensions
Tables	
	4-1. Center Frequency and Span Settings for Harmonic
	Bands
	4-2. Internal Memory Catalog Information*
	4-4. Functions Which Exit The Windows Display Format . 4-52
	4-5. Default Configuration Values
	4-6. Preset Conditions for Receiver Mode of Operation 4-143
	4-7. Preset Conditions for Signal Analysis Mode of Operation 4-144
	4-8. Preset Receiver Conditions 4-145
	4-9. Preset Spectrum Conditions
	4-10
	A-1. Status Byte Definition

1-1. HP 8542E EMI Receiver Dimensions

HP 8542E/HP 85422E Specifications and **Characteristics**

This chapter contains specifications and characteristics for the HP 8542E EMI receiver and HP 85422E receiver RF section.

The specifications in this chapter apply to all functions autocoupled over the environmental conditions specified. All specifications apply after two hours of storage at a constant temperature within the operating temperature range, after the instrument has been operating for 60 minutes, and after CAL ALL has been run.

Definitions of Terms

The distinction between specifications, characteristics, typical performance, and nominal values is described as follows:

- Specifications describe warranted performance.
- Characteristics provide useful, but nonwarranted information about the functions and performance of the instrument.
- Typical Performance, where listed, is not warranted, but indicates performance which most units will exhibit.
- Nominal Value is an expected, but not warranted, value of the parameter.

General Specifications: HP 8542E EMI Receiver

Temperature Range		
Operating*	0 °C to +55 °C	
Storage	−20 °C to +65 °C	
* Disk drive +5 °C to +45 °C		

EMI Compatibility

Receiver is in compliance with CISPR Pub. 16.

Receiver radiated and conducted emissions performance is in compliance with CISPR Pub. 11/1990 Group 1 Class B.

Receiver susceptibility performance is in compliance with CISPR Pub. 16 at 3 V/m field strength.

Inputs	
Low frequency	Type N, 50 Ω, 9 kHz to 50 MHz
High frequency	Type N, 50 Ω, 9 kHz to 2.9 GHz
Detectors	
Measurement	Peak, Quasi-Peak, and Average
	Quasi-Peak and Average time constants conform with CISPR
	Pub.16.
Overload	Broadband RF (band 1 and 2 only) and IF
IF Bandwidths	
Measurement	200 Hz, 9 kHz, and 120 kHz
	(6 dB bandwidths which conform to CISPR Pub.16)
Bandwidth Accuracy	1 MHz, 6 dB bandwidth $\pm 10\%$
Diagnostic	30 Hz to 300 kHz, 3 dB bandwidths in 1,3,10 steps ($\pm 20\%$
0	

Averaging Bandwidths	30 Hz to 1 MHz in 1,3,10 steps (±30% characteristic), and 3 MHz. Post-detection single pole low-pass filters.
	1.2.10 Hg digital filters with anti-aliceing

characteristic), also 3 MHz and 5 MHz. Four-pole $synchronously-tuned,\ approximately\ Gaussian\ shape.$

General Specifications: HP 8542E EMI Receiver (continued)

Input Attenuator	
Range	0 to 50 dB
Linearity Test Attenuator	4 dB
Preamplification	12 dB (Band 1 and 2)
	$27 \text{ dB} \pm 4 \text{ dB (Bypass)}$
Demodulation	AM and FM
Disk Drive	Internal 3.5 inch disk drive, compatible with 1.44 MByte
	DOS and LIF format disks

Input Filter Bandwidths	Frequency Range	Filter Type
(all 3 dB bandwidths are characteristics)	9 kHz to 74 kHz	fixed
	74 kHz to 198 kHz	fixed
	198 kHz to 525 kHz	fixed
	525 kHz to 1025 kHz	fixed
	1 MHz to 2 MHz	fixed
	2 MHz to 6 MHz	tunable (20%, 3 dB)
	6 MHz to 17 MHz	tunable (10%, 3 dB)
	17 MHz to 29 MHz	tunable (7%, 3 dB)
	29 MHz to 52 MHz	tunable (8%, 3 dB)
	52 MHz to 98 MHz	tunable (6%, 3 dB)
	98 MHz to 152 MHz	tunable (6%, 3 dB)
	152 MHz to 216 MHz	tunable (6%, 3 dB)
	216 MHz to 330 MHz	tunable (5%, 3 dB)
	330 MHz to 500 MHz	tunable (5%, 3 dB)
	0.5 GHz to 1 GHz	tunable (4%, 3 dB)
	1 GHz to 2.9 GHz	fixed

General Specifications: HP 8542E EMI Receiver (continued)

Sweep Time	
Range	20 ms to 100 s
Sweep Trigger	Free Run, Single, Line, Video, External

Audible Noise	<5.5 Bels power (ISODP 7779)
---------------	------------------------------

Power Requirements		
On	Receiver RF Section	90 to 132 V rms, 47 to 440 Hz
		198 to 264 V rms, 47 to 66 Hz
		Power consumption <500 VA; <180 W
	RF Filter Section	90 to 132 V rms, 47 to 440 Hz 198 to 264 V rms, 47 to 66 Hz Power consumption <115 VA; <85 W
Off	Receiver RF Section	Power consumption <5 W

Environmental Conditions	
Environment	Indoor Use
Altitude	Up to 15,000 feet (4,572 meters)
Maximum Relative Humidity	80% for temperatures up to 31 °C decreasing linearly to 50% relative humidity at 40 °C.
INSTALLATION CATEGORY II according to IEC 1010	
POLLUTION DEGREE 2 according to IEC 664	

Tuning Specifications

Tuning Range	
Band 1	9 kHz to 50 MHz
Band 2	20 MHz to 2.9 GHz
Bypass	9 kHz to 2.9 GHz

Frequency Reference	
Aging	\pm 1 x 10 ⁻⁷ /year
Settability	$\pm 1 \times 10^{-8}$
Temperature Stability	$\pm 1 \times 10^{-8}$

Frequency Readout Accuracy	± (frequency readout x frequency reference error * + span accuracy
	+ 1% of span + 20% of IF Bandwidth + 100 Hz) †

*Frequency reference error=(aging rate x period of time since last adjustment + initial achievable accuracy + temperature stability). See frequency characteristics.

†See "Drift" under "Stability" in frequency characteristics.

Calibrator	
Frequency	300 MHz fundamental
Accuracy	see frequency reference error*

*Frequency reference error=(aging rate x period of time since last adjustment + initial achievable accuracy + temperature stability). See frequency characteristics.

Swept Frequency Specifications

Frequency Span		
Range	Band 1	1 kHz to 50 MHz
	Band 2	1 kHz to 2.9 GHz
	Bypass	1 kHz to 2.9 GHz
Resolution	Four digits or 20 Hz, whichever is greater	
Accuracy*		
Span ≤ 10 MHz	±2% of Span + 10 Hz	
Span > 10 MHz	±3% of Span	
*Sweep time > 75 ms		

Stability	
Noise sidebands*	
>10 kHz offset from CW signal	≤-90 dBc/Hz
>30 kHz offset from CW signal	≤-105 dBc/Hz
Residual FM	
30 Hz IF BW, 30 Hz Averaging BW	≤30 Hz pk-pk in 300 ms
1 kHz IF BW, 1 kHz Averaging BW	≤250 Hz pk-pk in 100 ms
System Related Sidebands	≤-65 dBc
>30 kHz offset from CW signal	
* 1 kHz IF BW, 30 Hz averaging BW, sample detector.	

±(marker frequency x frequency reference error* + counter resolution + 100 Hz)
±(marker frequency x frequency reference error* + counter resolution + 1 kHz)
Selectable from 10 Hz to 100 kHz
Selectable from 100 Hz to 100 kHz

^{*}Frequency reference error = (aging rate x period of time since last adjustment + initial achievable accuracy + temperature stability). See frequency characteristics.

[‡]Marker level to displayed noise level >25 dB, IF Bandwidth/Span ≥0.01, Span ≤300 MHz.

Amplitude Specifications

Amplitude specifications do not apply for negative peak detector mode except as noted in "Amplitude Characteristics."


Amplitude Range	-146 dBm to +30 dBm
	$-39~\mathrm{dB}\mu\mathrm{V}$ to $+~137~\mathrm{dB}\mu\mathrm{V}$

Displayed Average Noise Level	Band 1	Band 2	Bypass
$f_{o} > 400 \text{ kHz}$	9 kHz to	20 MHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$2.9~\mathrm{GHz}$
(input terminated, 0 dB attenuation, 30 Hz IF BW,			
30 Hz Averaging BW, sample detection)			
Preamplifier On	< ≤-39 dl	BμV>	
-	(-146		
Preamplifier Off	< ≤-31 d	BμV>	
-	(-138		
Characteristic Noise Figure			
Preamplifier On	< 10 d < 14 d	B>	
Preamplifier Off	14.4	D \	

Displayed Average Noise Level

 $f_o < 400 \text{ kHz}$

(input terminated, 0 dB attenuation, 30 Hz IF BW, 30 Hz Averaging BW, sample detection)

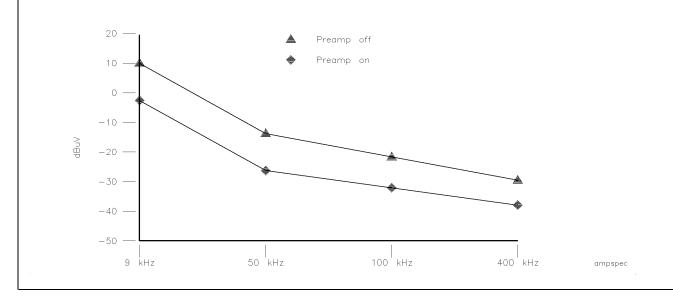

Noise Indication in CISPR Bandwidths			
(Characteristic)			
0 dB input attenuation, 50Ω input termination	Peak	Quasi-Peak	Average
200 Hz (6 dB), 9 kHz to 150 kHz			
Preamplifier On	$2 \text{ dB}\mu\text{V to } -28 \text{ dB}\mu\text{V}$	$-7~\mathrm{dB}\mu\mathrm{V}$ to $-29~\mathrm{dB}\mu\mathrm{V}$	-9 dB μ V to -31 dB μ V
	(-105 dBm to -135 dBm)	(-114 dBm to -136 dBm)	(-116 dBm to -138 dBm)
Preamplifier Off	15 dBμV to –15 dBμV	6 dB μ V to -25 dB μ V	$3~\mathrm{dB}\mu\mathrm{V}$ to $-27~\mathrm{dB}\mu\mathrm{V}$
	(-92 dBm to -122 dBm)	(-101 dBm to -132 dBm)	(-104 dBm to -134 dBm)
9 kHz (6 dB), 150 kHz to 30 MHz			
Preamplifier On	−8 dBµV	$-15 \mathrm{dB}\mu\mathrm{V}$	$-21 \mathrm{dB}\mu\mathrm{V}$
	(-115 dBm)	(-122 dBm)	(-128 dBm)
Preamplifier Off	−3 dBµV	$-11~\mathrm{dB}\mu\mathrm{V}$	$-18~\mathrm{dB}\mu\mathrm{V}$
	(-110 dBm)	(-118 dBm)	(-125 dBm)
120 kHz (6 dB), 30 MHz to 1 GHz			
Preamplifier On	$4~\mathrm{dB}\mu\mathrm{V}$	$-2 dB\mu V$	$-10 \mathrm{dB}\mu\mathrm{V}$
	(-103 dBm)	(-109 dBm)	(-117 dBm)
Preamplifier Off	9 d Bμ V	$2~\mathrm{dB}\mu\mathrm{V}$	$-5~\mathrm{dB}\mu\mathrm{V}$
	(-98 dBm)	(-105 dBm)	(-112 dBm)

	Band 1	Band 2	Bypass
	9 kHz to	20 MHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$2.9~\mathrm{GHz}$
System Amplitude Accuracy			
Specification [†]	< ±2 d	B>	
Characteristic‡	< ±1 d	B>	

^{† &}gt;(-10 dBµV + attenuation + (12 - preamplifier gain)) reference level. Use Measure at Marker or linear mode, top 4 graticules. If using the Measure at Marker function to measure a pulsed signal with a repetition frequency of less than 5 Hz, set the sweep time to greater than or equal to the inverse of the pulse repetition frequency. (For example, to measure a 1 Hz CISPR pulse, set the sweep time to 1 second or greater prior to using the Measure at Marker function.) If IFBW ≤ 300 Hz and signal separation ≤ 4 kHz, also use Linearity Check. ‡ 20 °C to 30 °C plus the above.

	Band 1	Band 2	Bypass
	9 kHz to	20 MHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$2.9~\mathrm{GHz}$
Gain Compression*			
Specification			
f _o ≥10 MHz	< <0.5	dB>	
200 kHz <f<sub>o<10 MHz</f<sub>	<<0.75		
Characteristic 1 dB Compression Point	,	•	
$f_o \ge 10 \text{ MHz}$			
Preamplifier On	< 77 dE	BμV>	
	(-30 c		
	(33)		
Preamplifier Off	< 89 dE	BμV>	
-	(-18 c		
$9 \text{ kHz} < f_o < 10 \text{ MHz}$, ,	,	
Preamplifier On	$72~\mathrm{dB}\mu\mathrm{V}$		
•	(-35 dBm)		
Preamplifier Off	$85~\mathrm{dB}\mu\mathrm{V}$		
•	(-22 dBm)		
Third Harmonic Intercept Point**			
Specification			
$f_o > 200 \text{ kHz}$			
Preamplifier On	< 85 dBμ	V>	<- 85 dBμV>
	(-22 c	dBm)	(-22 dBm)
Preamplifier Off	< 97 dBμ	V>	$<-112 \text{ dB}\mu\text{V}>$
	(-10 dBi	m)	(+5 dBm)
Characteristic			
f _o ≥10 MHz			
Preamplifier On	$<$ ———— 92 dB μ	V>	
	(-15 dBi	m)	
Preamplifier Off	< 101 dB	μV>	
	(-6 dBn	n)	
$9 \text{ kHz} < f_{\circ} < 10 \text{ MHz}$			
Preamplifier On	< 89 dBμ	V>	
	(-18 dBi		
Preamplifier Off	< 100 dB	μV———>	
	(-7 dBn		

^{*}Indicated specification is derived from measured distortion with a total power at the input mixer of -10 dBm. Bands 1 and $2:\ Power\ at\ the\ input\ mixer=input\ power\ -\ input\ attenuation\ +\ 15\ dB\ +\ preamplifier\ gain.\ Bypass:\ Power\ at\ the\ input\ power\ at\ power\ at\ the\ input\ power\ at\ power\ power\ power\ power\ power\ power\ at\ power\ po$ mixer=input power - input attenuation + preamplifier gain. If the IFBW is ≤ 300 Hz, this applies only if signal separation is ≥ 4 kHz and signal amplitudes \leq Ref. Level + 10 dB.

^{**} Signal separation > 50 kHz. Indicated specification derived from measured distortion products for two -30 dBm CW signals at the input.

	Band 1	Band 2	Bypass
	9 kHz to	20 MHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$2.9~\mathrm{GHz}$
econd Harmonic Intercept Point*			
Specification†			
$100 \text{ kHz} \leq \text{ f} \leq 1.8 \text{ GHz}$			
Preamplifier On	<110 dl	$B\mu V>$	
	(+3 6	dBm)	
Preamplifier Off	<122 dl	BμV>	
	(+15	dBm)	
$1.8~\mathrm{GHz} < \mathrm{f} \le 2.9~\mathrm{GHz}$			
Preamplifier On		$105~\mathrm{dB}\mu\mathrm{V}$	
		(-2 dBm)	
Preamplifier Off		$105~\mathrm{dB}\mu\mathrm{V}$	
		(-2 dBm)	
Characteristic			
$9 \text{ kHz} \leq f \leq 1.8 \text{ GHz}$			
Preamplifier On	<127 dl	$B\mu V>$	
	(+20	dBm)	
Preamplifier Off	<137 dl	3μ V———>	
	(+30	dBm)	
$1.8~\mathrm{GHz} < \mathrm{f} \le 2.9~\mathrm{GHz}$			
Preamplifier On		$114~\mathrm{dB}\mu\mathrm{V}$	
		(+7 dBm)	
Preamplifier Off		$112~\mathrm{dB}\mu\mathrm{V}$	
		(+5 dBm)	

† Indicated specification level was derived from measured harmonic levels for a -40 dBm input signal.

	Band 1	Band 2	Bypass
	9 kHz to	20 MHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$2.9~\mathrm{GHz}$
Other Input Related Spurious†			
other input Related Spurious	< - 68	5 dBc>	
Residual Responses			
Input terminated, 0 dB attenuation (preamplifier on)			
>30 kHz	<	$-$ < $-10 \text{ dB}\mu\text{ V}$ $$	>
		(-117 dBm)	
<30 kHz	<	< -2 dBμV	>
		(-109 dBm)	
Maximum Safe Input Level			
Average Continuous Power	<+30 0	dBm>	<+30 dBm
			(Input atten ≥10 c
Peak Pulse Power	2000 W peak for 10 µs > 20 dB input attenuation	$100 \text{ W for} < 10 \ \mu \text{s}$ $\text{pulse width} < 1\%$ $\text{duty cycle and} >$ 30 dB input attenuation	
DC (Volts)	<	0 V>	
Input VSWR			
0 dB input attenuation			
≤1.0 GHz	< 2	: 1>	
_ 1.0 GHz <f<sub>o≤2.9 GHz</f<sub>		< 2.5 : 1>	
10 dB input attenuation		·	
≤1.0 GHz	< 1.2	: 1>	
_ 1.0 GHz <f<sub>o≤2.9 GHz</f<sub>		< 1.6 : 1>	

Marker Readout Resolution	0.05 dB for log scale
	0.05% of reference level for linear scale

Reference Level	
Range	
Log Scale	-146 dBm to +30 dBm
Linear Scale	-126 dBm to +30 dBm
Resolution	
Log Scale	±0.01 dB
Linear Scale	± 0.12 % of reference level

Linear to Log Switching	±0.25 dB at reference level
-------------------------	-----------------------------

Display Scale Fidelity	
Log Maximum Cumulative*	
3 kHz to 3 MHz IF Bandwidth	$\pm (0.3 \text{ dB} + 0.01 \text{ x dB from Reference level})$
≤ 1 kHz IF Bandwidth	$\pm (0.4 \text{ dB} + 0.01 \text{ x dB from Reference level})$
Log Incremental Accuracy 0 to -56 dB from Reference Level	±0.4 dB/4 dB
Linear Accuracy	$\pm 3\%$ of Reference Level
* 0 to -66 dB from reference level.	

Relative Quasi-Peak Response to a CISPR Pulse (dB)*		Frequency Bands	
Pulse Repetition Frequency	$120~\mathrm{kHz}$ 6 dB BW	9 kHz 6 dB BW	$200~\mathrm{Hz}~6~\mathrm{dB}~\mathrm{BW}$
(Hz)	$0.03~\mathrm{GHz}$ to $1~\mathrm{GHz}$	0.15 MHz to 30 MHz	9 kHz to 150 kHz
1000	$+8.0 \pm 1.0$	$+4.5\pm1.0$	
100	0 dB (reference)†	0 dB (reference)†	$+\ 4.0\ \pm1.0$
60		<u></u>	$+3.0 \pm 1.0$
25			0 dB (reference)†
20	-9.0 ± 1.0	-6.5 ± 1.0	
10	-14.0 ± 1.5	-10.0 ± 1.5	-4.0 ± 1.0
5		<u></u>	-7.5 ± 1.5
2	-26.0 ± 2.0	-20.5 ± 2.0	-13.0 ± 2.0
1	-28.5 ± 2.0	-22.5 ± 2.0	-17.0 ± 2.0
Isolated Pulse	-31.5 ± 2.0	-23.5 ± 2.0	-19.0 ± 2.0

^{*} Specification applies to a pulsed RF signal with equivalent spectral intensity as called out in CISPR Pub.16, Part 1. (CISPR pulse measurements require either an HP 8542E or HP 8546A EMI receiver and do not apply to either an HP 8542E or HP 85462A receiver RF section.)

 $[\]dagger$ Reference pulse amplitude accuracy relative to the CW signal is <1.5 dB as specified in CISPR pub. 16. CISPR reference pulse: $0.044~\mu Vs$ for .03 GHz to 1 GHz, $0.316~\mu Vs$ for .15 MHz to 30 MHz, $13.5~\pm 1.5~\mu Vs$ for 9 kHz to 150 kHz.

Tracking Generator Specifications

All Specifications apply over 0° C to 55° C. The receiver/tracking generator combination will meet its specification after 2 hours of storage at a constant temperature within the operating temperature range, 30 minutes after the combination is turned on, and after CAL ALL, CAL TRK GEN, and TRACKING PEAK have been run.

Output Frequency Range	9 kHz to 2.9 GHz		
output 11 equency mange	V KIZ to 2.0 GHZ		
Warm-up time	30 minutes		
Output Power Level			
Range	-1 dBm to -66 dBm		
Resolution	0.1 dB		
Vernier	1		
Range	9 dB		
Accuracy			
(25 °C ±10 °C)			
(-20 dBm at 300 MHz, 16 dB attenuation)	$\pm 0.2 \text{ dB/dB}$		
Incremental Cumulative	$\pm 0.5~\mathrm{dB}$ Total		
Output Attenuator Range	0 to 56 dB in 8 dB steps		
Output Power Sweep			
Range	(−10 dBm to −1 dBm) − (source attenuator setting)		
Resolution	0.1 dB		
Tracking Generator Feedthrough			
400 kHz to 2.9 GHz	≤ -110 dBm		
Spurious Output (-1 dBm output)			
Harmonic Spurs from 300 kHz to 2.9 GHz			
TG output 300 kHz to 2.9 GHz	$\leq -25 \text{ dBc}$		
Non-harmonic Spurs from 300 kHz to 2.9 GHz			
Non-narmonic Spurs from 300 kHz to 2.9 GHz TG output 300 kHz to 2.0 GHz	< −27 dBc		
TG output 2.0 GHz to 2.9 GHz	$\leq -27 \text{ dBc}$ < -23 dBc		
13 Suspending Gills to Bio Gills	2 25 450		
LO Feedthrough			
LO frequency 3.9214 GHz to 6.8214 GHz	≤ -16 dBm		

Frequency Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Frequency Reference	
Aging	$5 \times 10^{-10}/\mathrm{day}, 7 \mathrm{day}$ average after being powered on for seven days
Warm-up	1×10^{-8} after 30 minutes on
Initial Achievable Accuracy	$\pm 2.2 \times 10^{-8}$ after being powered on for 24 hours

ninute of sweep time
_

Drift occurs only while receiver is sweeping frequency. Additional drift occurs when using Line, Video, or External trigger while waiting for the appropriate trigger.

Amplitude Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Input Attenuator Uncertainty	
Attenuator Setting (Bypass)	
0 dB	$\pm~0.2~\mathrm{dB}$
10 dB	Reference
20 dB	$\pm~0.4~\mathrm{dB}$
30 dB	$\pm~0.5~\mathrm{dB}$
40 dB	$\pm 0.7 \text{ dB}$
50 dB	\pm 0.8 dB
10 dB Step Uncertainty (attenuator setting 10 to 50 dB)	\pm 0.8 dB/dB
Repeatability	$\pm 0.05~\mathrm{dB}$

FM Demodulation	
Input Level	
- Preamplifier Off	>(-75 dBm + attenuator setting)
Signal Level	0 to -30 dB below reference level
FM Offset	400 Hz nominal
FM Deviation (FM GAIN)	
Resolution	1 kHz/volt nominal
Range	10 kHz/volt to 1 MHz/volt
Bandwidth	FM Deviation ÷ 2
FM Linearity	≤ 1% of FM deviation + 290 Hz

Tracking Generator Characteristics

Output Flatness		
(referenced to 300 MHz, -20 dBm)		
Frequency > 10 MHz	$\pm 2 \text{ dB}$	
Frequency ≤10 MHz	±3 dB	
Output Power Level		
Absolute Accuracy	±0.75 dB	
(-20 dBm at 300 MHz)		
(25 °C ±10 °C)		
	<u>I</u>	
Tracking Drift		
Usable in a 1 kHz IF Bandwidth after a 5 minute warm-up	1.5 kHz/5 minutes	
RF Power Off Residuals		
9 kHz to 2.9 GHz	< -120 dBm	
Dynamic Range		
(Difference between maximum power out and tracking generator feedthrough)	> 109 dB	
Output Attenuator Repeatability		
300 kHz to 300 MHz	±0.1 dB	
300 MHz to 2.0 GHz	$\pm 0.2 \text{ dB}$	
2.0 GHz to 2.9 GHz	±0.3 dB	
Output VSWR		
0 dB attenuation	<3.0:1	
8 dB attenuation	<1.5:1	

Physical Characteristics

Front Panel Inputs and Outputs	
Low Frequency Input	Type N female, 50 Ω nominal
High Frequency Input	Type N female, 50 Ω nominal
Tracking Generator Output	Type N female, 50 Ω nominal
Probe Power*	
Voltage / Current	$+15~{ m Vdc}~{\pm}7\%$ at $150~{ m mA}$ maximum
	$-12.6~{ m Vdc}~{\pm}10\%$ at $150~{ m mA}$ maximum
Earphone Jack	1/8 inch monaural jack

 $^{^*}$ Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE connectors cannot exceed 150 mA. Total current drawn from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE cannot exceed

Rear Panel Inputs and Outputs			
10 MHz REF OUTPUT			
Connector	BNC female		
Impedance	50 Ω		
Output Amplitude	> 0 dBm		
EXT REF IN			
Connector	BNC female		
Input Amplitude Range	-2 dBm to +10 dBm		
Frequency	10 MHz		
Trequency	10 3333		
AUX IF OUT			
Connector	BNC female		
Frequency	21.4 MHz		
Amplitude Range	-10 dBm to -60 dBm		
Impedance	50 Ω		
AUX VIDEO OUT			
Connector	BNC female		
Amplitude Range	0 V to 1 V (uncorrected)		
EXT KEYBOARD	Interface compatible with HP part number C1405 Option		
	ABA and most IBM/AT non auto-switching keyboards.		
EXT TRIG INPUT			
Connector	BNC female		
Trigger Level	Positive edge initiates sweep in EXT TRIG mode (TTL)		
LO OUTPUT			
Connector	SMA female (must be terminated in 50 Ω when not used)		
Impedance	50 Ω		
Frequency Range	3.0 GHz to 6.8214 GHz		

Physical Characteristics (continued)

Rear Panel Inputs and Outputs (continued)			
HI-SWEEP IN/OUT			
Receiver RF Section Input/Output			
Connector	SMA female		
Output	High=sweep, Low=retrace (TTL)		
Input	Open collector, Low stops sweep		
RF Filter Section Output	High=sweep, Low=retrace (TTL)		
SWEEP INPUT / OUTPUT			
Receiver RF Section Output			
Connector	SMA female		
Output	0 V to +10 V ramp		
RF Filter Section Input			
Connector	SMA female		
Input	0 V to +10 V		
REMOTE INTERFACE			
Receiver RF Section	HP-IB (RS-232 optional)		
RF Filter Section	HP-IB compatible service port		
MONITOR OUTPUT	R, G, B (composite video on G)		
	25 kHz horizontal rate		
	60 Hz vertical rate		

AUX INTERFACE Connector Type: 9-pin s	ubminiature D			
Connector Pinout:				
Pin #	Function	Current	Logic Mode	Serial Bit Mode
1	Control A		TTL Output Hi/Lo	TTL Output Hi/Lo
2	Control B		TTL Output Hi/Lo	TTL Output Hi/Lo
3	Control C		TTL Output Hi/Lo	Strobe
4	Control D		TTL Output Hi/Lo	Serial Data
5	Control I		TTL Input Hi/Lo	TTL Input Hi/Lo
6	Gnd		Gnd	Gnd
7*	$-15~\mathrm{Vdc}~\pm7\%$	150 ma		
8*	$+5~\mathrm{Vdc}~\pm5\%$	150 ma		
9*	$+$ 15 Vdc $\pm 5\%$	150 ma		

^{*} Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE cannot exceed 150 mA. Total current drawn from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE cannot exceed 150 mA.

WEIGHT	
Receiver RF Section	62.5 lb.
RF Filter Section	46 lb.

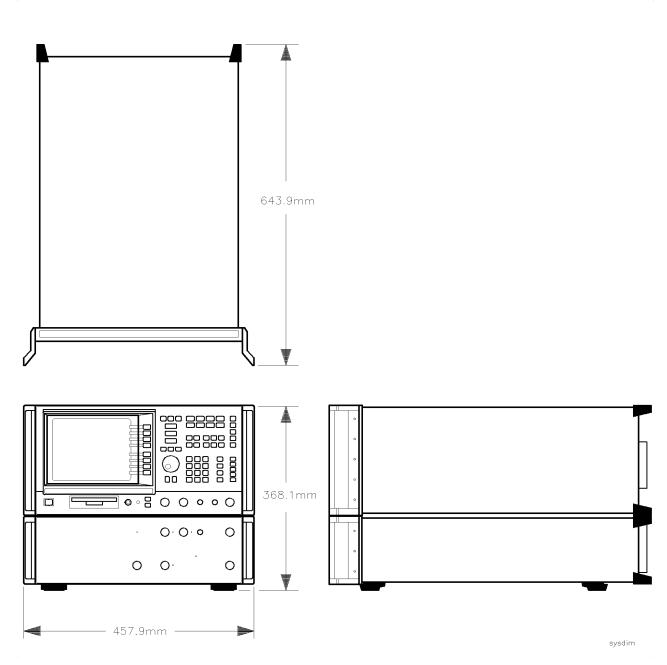


Figure 1-1. HP 8542E EMI Receiver Dimensions

General Specifications: HP 85422E Receiver RF Section

The specifications in this section apply to all functions autocoupled over the environmental conditions specified. All specifications apply after two hours of storage at a constant temperature within the operating temperature range, after the instrument has been operating for 60 minutes, and after CAL ALL has been run.

Temperature Range		
Operating*	0 °C to +55 °C	
Storage	-20 °C to +65 °C	
* Disk drive +5 °C to +45 °C		

EMI Compatibility

Receiver RF section radiated and conducted emissions performance is in compliance with CISPR Pub. 11/1990 Group 1 Class B. Receiver RF section susceptibility is in compliance with CISPR Pub. 16 at 3 V/m.

Inputs	Type N, 50 Ω, 9 kHz to 2.9 GHz
Detectors	
Measurement	Peak, Quasi-Peak, and Average.
	Quasi-Peak and Average time constants conform with CISPR Pub.16.
Overload	IF
IF Bandwidths	
Measurement	200 Hz, 9 kHz, and 120 kHz
	(6 dB bandwidths which conform to CISPR Pub.16)
Bandwidth Accuracy	1 MHz, 6 dB bandwidth $\pm 10\%$
Diagnostic	30 Hz to 300 kHz, 3 dB bandwidths in 1,3,10 steps ($\pm 20\%$ characteristic), also 3 MHz and 5 MHz. Four-pole synchronously-tuned, approximately Gaussian shape.
Averaging Bandwidths	30 Hz to 1 MHz in 1,3,10 steps ($\pm 30\%$ characteristic), and 3 MHz. Post-detection single pole low-pass filters.
	1,3,10 Hz digital filters with anti-aliasing
Input Attenuator	
Range	0 to 70 dB in 10 dB steps
Preamplification	$27 \text{ dB} \pm 1.5 \text{ dB} \le 500 \text{ MHz}, \pm 4 \text{ dB} > 500 \text{ MHz}$
Demodulation	AM and FM

General Specifications: HP 85422E Receiver RF Section (continued)

Sweep Time	
Range	20 ms to 100 s
Accuracy	±3%
Sweep Trigger	Free Run, Single, Line, Video, External
Sweep 1118801	Tree with origin, time, video, fixernal
Disk Drive	Internal 3.5 inch disk drive, compatible with 1.44 MByte
DISK DIIVC	DOS and LIF format disks
	DOS and Eri Tornat disks
Audible Noise	(E. F. D. L
Audible Noise	< 5.5 Bels power (ISODP 7779)
Power Requirements	
On	90 to 132 V rms, 47 to 440 Hz
	198 to 264 V rms, 47 to 66 Hz
	Power consumption <500 VA; <180 W
Off	Power consumption <5 W
Environmental Conditions	
Environment	Indoor Use
Altitude	Up to 15,000 feet (4,572 meters)
Maximum Relative Humidity	80% for temperatures up to 31 °C decreasing linearly to $50%$ relative humidity at 40 °C.
INSTALLATION CATEGORY II according to IEC 1010	
POLLUTION DEGREE 2 according to IEC 664	

Tuning Specifications

Tuning Range	
DC Coupled	9 kHz to 2.9 GHz
AC Coupled	100 kHz to 2.9 GHz

Frequency Reference	
Aging	$\pm 1 \times 10^{-7}$ /year
Settability	$\pm 1 \times 10^{-8}$
Temperature Stability	$\pm 1 \times 10^{-8}$

	± (frequency readout x frequency reference error * + span accuracy + 1% of span + 20% of IF Bandwidth + 100 Hz) †
*Frequency reference error=(aging rate x period of time	since last adjustment + initial achievable accuracy + temperature

stability). See frequency characteristics.

†See "Drift" under "Stability" in frequency characteristics.

Calibrator	
Frequency	300 MHz fundamental
Accuracy	see frequency reference error*
*Frequency reference error=(aging rate v period of time	since last adjustment + initial achievable accuracy + temperature

Frequency reference error=(aging rate x period of time since last adjustment +initial achievable accuracy + temperature stability). See frequency characteristics.

Swept Frequency Specifications

Frequency Span	
Range	1 kHz to 2.9 GHz
Resolution	Four digits or 20 Hz, whichever is greater
Accuracy	
Span ≤ 10 MHz	$\pm 2\%$ of span + 10 Hz
Span > 10 MHz	±3% of span

Stability	
Noise sidebands*	
>10 kHz offset from CW signal	≤-90 dBc/Hz
>30 kHz offset from CW signal	≤-105 dBc/Hz
Residual FM	
30 Hz IF BW, 30 Hz Averaging BW	≤30 Hz pk-pk in 300 ms
1 kHz IF BW, 1 kHz Averaging BW	≤250 Hz pk-pk in 100 ms
System Related Sidebands	≤-65 dBc
>30 kHz offset from CW signal	
* 1 kHz IF BW, 30 Hz averaging BW, sample detector.	

Marker Count Accuracy;	
Frequency Spans ≤ 10 MHz	±(marker frequency x frequency reference error* + counter resolution + 100 Hz)
Frequency Spans > 10 MHz	±(marker frequency x frequency reference error* + counter resolution + 1 kHz)
Counter Resolution	
Frequency Spans ≤10 MHz	Selectable from 10 Hz to 100 kHz
Frequency Spans > 10 MHz	Selectable from 100 Hz to 100 kHz
*Frequency reference error = (aging rate x period of time since	last adjustment + initial achievable accuracy + temperature


stability). See frequency characteristics.

[‡]Marker level to displayed noise level >25 dB, IF Bandwidth/Span \geq 0.01, Span \leq 300 MHz.

Amplitude Specifications

Amplitude specifications do not apply for negative peak detector mode except as noted in "Amplitude Characteristics."


Amplitude Range	-146 dBm to +30 dBm
	$-39 \text{ dB}\mu\text{V to} + 137 \text{ dB}\mu\text{V}$

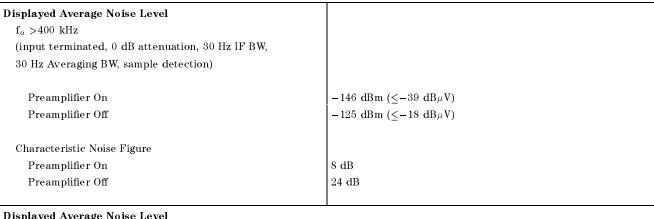

Displayed Average Noise Level

 $f_{\circ} < 400 \text{ kHz}$

(input terminated, 0 dB attenuation, 30 Hz IF BW, 30 Hz Averaging BW, sample detection)

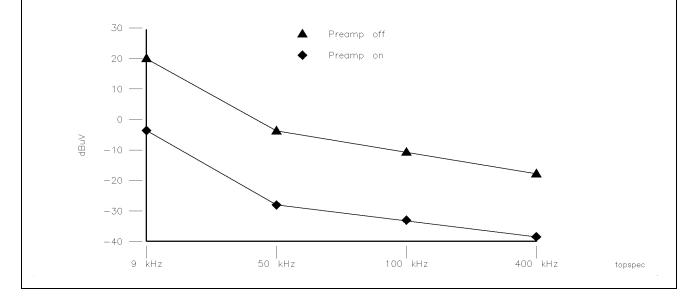

Gain Compression*	
Specification	
$f_o > 10 \text{ MHz}$	<0.5 dB
$200 \text{ kHz} \leq f_{\circ} \leq 10 \text{ MHz}$	<0.75 dB
Characteristic 1 dB Compression Point	
$f_o > 10 \text{ MHz}$	
Preamplifier On	$75 \text{ dB}\mu\text{V} \text{ (}-32 \text{ dBm)}$
Preamplifier Off	$102 \text{ dB}\mu\text{V} (-5 \text{ dBm})$
$9 \text{ kHz} \leq f_o \leq 10 \text{ MHz}$	
Preamplifier On	$68 \text{ dB}\mu\text{V} (-39 \text{ dBm})$
Preamplifier Off	$95 \text{ dB}\mu\text{V} (-12 \text{ dBm})$

^{*} Specifications derived from distortion measurements using a two-tone compression test with frequency offset of 30 MHz and -10 dBm total signal power at the input mixer. Total power at first mixer = input power input atten + preamp gain. IF BW \(\le 300\) Hz, this applies only if signal separation \(\ge 4\) kHz and signal amplitudes ≤ Reference Level + 10 dB.

hird Order Intercept Point†		
Specification		
$f_{\circ} > 200 \text{ kHz}$		
Preamplifier On	$85 \text{ dB}\mu\text{V} (-22 \text{ dBm})$	
Preamplifier Off	112 dB μ V (+ 5 dBm)	
Characteristic Third Order Intercept		
$f_{o} > 10 \text{ MHz}$		
Preamplifier On	89 dB _μ V (-18 dBm)	
Preamplifier Off	118 dB μ V (+11 dBm)	
$9 \text{ kHz} \le f_{\circ} \le 10 \text{ MHz}$		
Preamplifier On	$87 \text{ dB}\mu\text{V} (-20 \text{ dBm})$	
Preamplifier Off	115 $dB\mu V (+8 dBm)$	

signals at the first mixer and 50 kHz separation. Input mixer power = input power - input attenuation + preamp gain.

econd Harmonic Intercept*		
$f_o > 200 \text{ kHz}$		
Preamplifier On	$100 \text{ dB}\mu\text{V } (-9 \text{ dBm})$	
Preamplifier Off	$134~\mathrm{dB}\mu\mathrm{V}~(+27~\mathrm{dBm})$	
Characteristic Second Order Intercept		
Preamplifier On		
$f_o > 500 \text{ MHz}$	115 $dB\mu V (+8 dBm)$	
$9 \text{ kHz} \le f_o \le 500 \text{ MHz}$	$108 \mathrm{dB}\mu\mathrm{V} (+1 \mathrm{dBm})$	
Preamplifier Off	$144 dB\mu V (+37 dBm)$	

^{*} The indicated specification level was derived from a measured harmonic level of <-67 dBc and a -40 dBm CW signal at the input mixer. Input mixer power = input power = input attenuation + preamp gain.

Other Input Related Spurious	-65 dBc	
30 kHz offset for -20 dBm tone at the mixer ≤2.9 GHz, f _o >10 MHz. Input mixer power = input power - input attenuation + preamp gain.		

Residual Responses	
Input terminated, 0 dB attenuation, preamplifier on	
150 kHz to 2.9 GHz	$-8 \text{ dB}\mu\text{V} (-115 \text{ dBm})$
9 kHz to 150 kHz	$+2 \text{ dB}\mu\text{V} (-105 \text{ dBm})$

Maximum Safe Input Level	
Average Continuous Power	
9 kHz to 2.9 GHz	+30 dBm (with 10 dB input attenuation)
Peak Pulse Power Preamplifier Off	+50 dBm (100 W) for 10 μs pulse width and, 1% duty cycle, input atten ≥30 dB.
DC	0 V (dc coupled) 50 V (ac coupled)

Calibrator Output	
Amplitude	$-20~\mathrm{dBm}\pm0.4~\mathrm{dB}$

Calibration Repeatability*	±0.15 dB

*Repeatability in the measured absolute amplitude of the CAL OUT signal at the reference settings after CAL FREQ and CAL AMPTD self-calibration. Absolute amplitude reference settings are: -20 dB reference level; 10 dB input attenuation; 300 MHz center frequency; 3 kHz IF BW; 300 Hz averaging BW; linear scale; 50 kHz span; coupled sweep time; reference level positioned at the top graticule; corrections on; and sample detection.

Display Range	
Log Scale	0 to -66 dB from Reference Level is calibrated
	0.1, 0.2, 0.5 dB/division and 1 to 20 dB/division in 1dB steps; eight divisions displayed
Linear Scale	Eight divisions
Scale Units	dBm, dBmV, dB μ V, V, W

Marker Readout Resolution	0.05 dB for log scale	
	0.05% of reference level for linear scale	

Reference Level	
Range	
Log Scale	-146 dBm to $+30$ dBm
Linear Scale	-126 dBm to +30 dBm
Resolution	
Log Scale	$\pm 0.01~\mathrm{dB}$
Linear Scale	$\pm 0.12\%$ of Reference Level
Accuracy*	
0 dBm to -59.9 dBm	$\pm (0.3 \text{ dB} + 0.01 \text{ x dB from } -20 \text{ dBm})$
-60 dBm and below	
1 kHz to 3 MHz IF BW	$\pm (0.6 \text{ dB} + 0.01 \text{ x dB from } -20 \text{ dBm})$
30 Hz to 300 Hz IF BW	$\pm (0.7 \text{ dB} + 0.01 \text{ x dB from } -20 \text{ dBm})$

^{*} Referenced to -20 dBm reference level, 10 dB input attenuation, at a single frequency, in a fixed IF BW with preamplifier off. With preamplifier on, subtract preamplifier gain from all reference levels.

Linear to Log Switching ±0.25 dB at reference level	
Display Scale Fidelity	
Log Maximum Cumulative	
(0 to -66 dB from Reference Level)	
3 kHz to 3 MHz IF Bandwidth	$\pm (0.3 \text{ dB} + 0.01 \text{ x dB from Reference Level})$
≤ 1 kHz IF Bandwidth	$\pm (0.4 \text{ dB} + 0.01 \text{ x dB from Reference Level})$
Log Incremental Accuracy	$\pm 0.4 \text{ dB/4 dB}$
(0 to -56 dB from Reference Level)	
Linear Accuracy	$\pm 3\%$ of Reference Level

IF Bandwidth Switching Uncertainty	
(at Reference Level, referenced to 3 kHz IF BW)	
3 kHz to 3 MHz	±0.4 dB
1 kHz	$\pm 0.5~\mathrm{dB}$
30 Hz to 300 Hz	±0.6 dB

Flatness		
(dc coupled, 10 dB input attenuation)	Absolute*	${\bf Relative}\dagger$
9 kHz to 2.9 GHz		
Preamplifier On	±3.0 dB	$\pm 2.0~\mathrm{dB}$
Preamplifier Off	±1.5 dB	$\pm 1.0~\mathrm{dB}$
* Referenced to 300 MHz Calibrator.		

[†] Referenced to midpoint between highest and lowest frequency response deviations.

Tracking Generator Specifications

All Specifications apply over 0° C to 55° C. The receiver/tracking generator combination will meet its specification after 2 hours of storage at a constant temperature within the operating temperature range, 30 minutes after the combination is turned on, and after CAL ALL, CAL TRK GEN, and TRACKING PEAK have been run.

Output Frequency Range	9 kHz to 2.9 GHz
Warm-up time	30 minutes
Output Power Level	
Range	-1 dBm to -66 dBm
Resolution	0.1 dB
Absolute Accuracy	$\pm 0.75~\mathrm{dB}$
(-20 dBm at 300 MHz)	
(25 °C ±10 °C)	
Vernier	
Range	9 dB
Accuracy	
(25 °C ±10 °C)	
(-20 dBm at 300 MHz, 16 dB attenuation)	$\pm 0.2 \text{ dB/dB}$
Incremental Cumulative	±0.5 dB Total
Output Attenuator Range	0 to 56 dB in 8 dB steps
Output Power Sweep	
Range	(−10 dBm to −1 dBm) − (source attenuator setting)
Resolution	0.1 dB
Output Flatness	
(referenced to 300 MHz, - 20 dBm)	
Frequency > 10 MHz	±2 dB
Frequency ≤10 MHz	±3 dB
The sking Comments of Fredding &	
Tracking Generator Feedthrough 400 kHz to 2.9 GHz	≤ -110 dBm

Tracking Generator Specifications (continued)

Spurious Output (-1 dBm output)	
Harmonic Spurs from 300 kHz to 2.9 GHz TG output 300 kHz to 2.9 GHz	≤ −25 dBc
Non-harmonic Spurs from 300 kHz to 2.9 GHz TG output 300 kHz to 2.0 GHz TG output 2.0 GHz to 2.9 GHz	≤ −27 dBc ≤ −23 dBc
LO Feedthrough LO frequency 3.9214 GHz to 6.8214 GHz	≤ −16 dBm

Frequency Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Frequency Reference	
Aging	$5 \times 10^{-10}/{\rm day}, 7 {\rm day}$ average after being powered on for seven days
Warm-up	1×10^{-8} after 30 minutes on
Initial Achievable Accuracy	$\pm 2.2 \times 10^{-8}$ after being powered on for 24 hours

Stability	
Drift (after warm-up at stabilized temperature)	<2 kHz/minute of sweep time
Frequency spans ≤ 10 MHz, free run trigger	
TO 10: 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	11'0 1 ' . I ' I' I' I I . I

Drift occurs only while receiver is sweeping frequency. Additional drift occurs when using Line, Video, or External trigger while waiting for the appropriate trigger.

Amplitude Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Input Attenuator Uncertainty		
Attenuator Setting		
0 d B	$\pm~0.2~\mathrm{dB}$	
10 dB	Reference	
20 dB	$\pm~0.4~\mathrm{dB}$	
30 dB	$\pm~0.5~\mathrm{dB}$	
40 dB	$\pm 0.7 \text{ dB}$	
50 dB	$\pm~0.8~\mathrm{dB}$	
60 dB	± 1.0 dB	
70 dB	\pm 1.0 dB	
10 dB Step Uncertainty	$\pm~0.8~\mathrm{dB}$	
(attenuator setting 10 to 70 dB)		
Repeatability	±0.05 dB	

AC Coupled Insertion Loss*		
100 kHz to 300 kHz	$0.7~\mathrm{dB}$	
300 kHz to 1 MHz	$0.2~\mathrm{dB}$	
1 MHz to 100 MHz	0.07 dB	
100 MHz to 2.9 GHz	$0.05 \text{ dB} + (0.06 \times \text{F}) \dagger \text{dB}$	
* Referenced to dc coupled mode.		
† F=frequency in GHz.		

Marker Readout Resolution	
(digitizing resolution)	
Log Scale	$\pm 0.31~\mathrm{dB}$
Linear Scale	
Frequency ≤1 GHz	±0.59 % of Reference Level
Frequency ≥1 GHz	± 1.03 % of Reference Level

Amplitude Characteristics (continued)

FM Demodulation	
Input Level	>(-60 dBm + attenuator setting)
Signal Level	0 to -30 dB below reference level
FM Offset	400 Hz nominal
FM Deviation (FM GAIN)	
Resolution	1 kHz/volt nominal
Range	10 kHz/volt to 1 MHz/volt
Bandwidth (6 dB)	FM Deviation ÷ 2
FM Linearity	≤ 1% of FM deviation + 290 Hz

Tracking Generator Characteristics

Tracking Drift Usable in a 1 kHz IF Bandwidth after a 5 minute warm-up	1.5 kHz/5 minutes
RF Power Off Residuals 9 kHz to 2.9 GHz	< -120 dBm
Dynamic Range (Difference between maximum power out and tracking generator feedthrough)	> 109 dB
Output Attenuator Repeatability	
300 kHz to 300 MHz 300 MHz to 2.0 GHz	$\pm 0.1 \text{ dB}$ $\pm 0.2 \text{ dB}$
2.0 GHz to 2.9 GHz	±0.3 dB
Output VSWR	
0 dB attenuation 8 dB attenuation	<3.0:1 <1.5:1

Physical Characteristics

Front Panel Inputs and Outputs	
Input	Type N female, 50 Ω nominal
Calibrator Output	Type N female, 50 Ω nominal
Tracking Generator Output	Type N female, 50 Ω nominal
Probe Power* Voltage / Current	+ 15 Vdc ±7% at 150 mA max. -12.6 Vdc ±10% at 150 mA max.
Earphone Jack	1/8 inch monaural jack
External ALC	Negative Detector

 $^{^*}$ Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE connectors cannot exceed 150 mA. Total current draw from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE connectors cannot exceed 150 mA.

BNC female
50 Ω
>0 dBm
BNC female
-2 dBm to +10 dBm
10 MHz
BNC female
21.4 MHz
-10 dBm to -60 dBm
50 Ω
BNC female
0 to 1 V (uncorrected)

Physical Characteristics (continued)

Rear Panel Inputs and Outputs (continued)	
EXT KEYBOARD	Interface compatible with HP part number C1405 Option ABA and most IBM/AT non auto-switching keyboards.
EXT TRIG INPUT	
Connector	BNC female
Trigger Level	Positive edge initiates sweep in EXT TRIG mode (TTL)
LO OUTPUT	
Connector	SMA female (must be terminated in 50 Ω when not used)
Impedance	50 Ω
Frequency Range	3.0 to 6.8214 GHz
HI-SWEEP IN/OUT (input/output 85422E)	
Connector	SMA female
Output	High=sweep, Low=retrace (TTL)
Input	Open collector, low stops sweep
SWEEP INPUT / OUTPUT (output 85422E)	
Connector	SMA female
Output	0 to +10 V ramp
REMOTE INTERFACE (85422E)	HP-IB (RS-232 optional)
MONITOR OUTPUT	R, G, B (composite video on G)
	25 kHz horizontal rate
	60 Hz vertical rate

AUX INTERFACE				
Connector Type: 9-pin	subminiature D			
Connector Pinout:				
Pin #	Function	Current	Logic Mode	Serial Bit Mode
1	Control A		TTL Output Hi/Lo	TTL Output Hi/Lo
2	Control B		TTL Output Hi/Lo	TTL Output Hi/Lo
3	Control C		TTL Output Hi/Lo	Strobe
4	Control D		TTL Output Hi/Lo	Serial Data
5	Control I		TTL Input Hi/Lo	TTL Input Hi/Lo
6	Gnd		Gnd	$\overline{\mathrm{Gnd}}$
7 *	$-15~\mathrm{Vdc}~\pm7\%$	150 ma		
8*	$+5$ Vdc $\pm 5\%$	150 ma		
9*	$+$ 15 Vdc $\pm5\%$	150 ma		

 $^{^{*}}$ Total current drawn from the + 15 Vdc on the PROBE POWER and the AUX INTERFACE cannot exceed 150 mA. Total current drawn from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE cannot exceed 150 mA.

WEIGHT	
Receiver RF Section	62.5 lb.

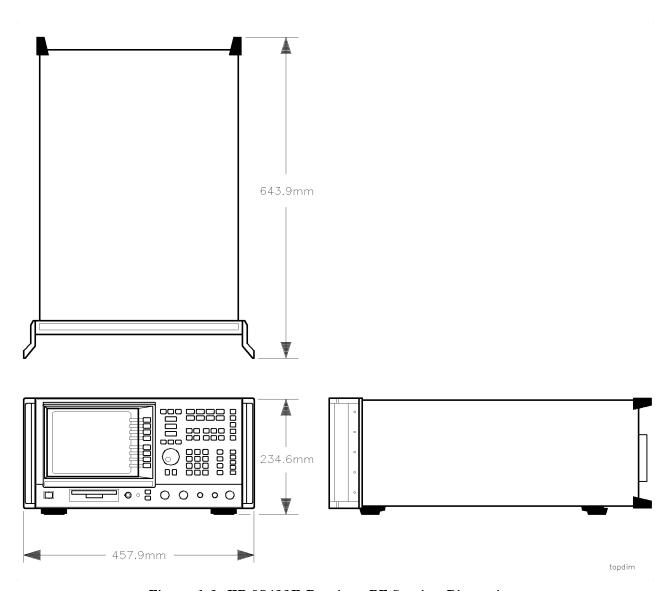


Figure 1-2. HP 85422E Receiver RF Section Dimensions

Regulatory Information

The information on the following page applies to the HP $8542E\ EMI$ receiver and HP 85422E receiver RF section.

DECLARATION OF CONFORMITY

according to ISO/IEC Guide 22 and EN 45014

Hewlett-Packard Co. Manufacturer's Name:

Manufacturer's Address: Santa Rosa Systems Division

1400 Fountaingrove Parkway

Santa Rosa, CA 95403-1799

USA

declares that the product

EMI Receiver **Product Name:**

HP 8542E, HP 85420E, HP 85422E, **Model Number:**

HP 8546A, HP 85460A, HP 85462A

Product Options: This declaration covers all options of the

above product.

conforms to the following Product specifications:

Safety: IEC 1010-1:1990+A1 / EN 61010-1:1993

CAN/CSA-C22.2 No. 1010.1-92

EMC: CISPR 11:1990/EN 55011:1991 Group 1, Class B

IEC 801-2:1984/EN 50082-1:1992 4 kV CD, 8 kV AD IEC 801-3:1984/EN 50082-1:1992 3 V/m, 27-500 MHz

IEC 801-4:1988/EN 50082-1:1992 0.5 kV Sig. Lines, 1 kV Power Lines

Supplementary Information:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC.

Santa Rosa, California, USA 11 Sept 1995

Dixon Browder/Quality Manager

European Contact: Your local Hewlett-Packard Sales and Service Office or Hewlett-Packard GmbH, Department ZQ/Standards Europe, Herrenberger Strasse 130, D-71034 Böblinger, Germany (FAX +49-7031-14-3143)

Notice for Germany: Noise Declaration

 $\mathrm{LpA} < 70~\mathrm{dB}$ am Arbeitsplatz (operator position) normaler Betrieb (normal position) nach DIN 45635 T. 19 (per ISO 7779)

HP 8546A/HP 85462A Specifications and **Characteristics**

This chapter contains specifications and characteristics for the HP 8546A EMI receiver and HP 85462A receiver RF section.

The specifications in this chapter apply to all functions autocoupled over the environmental conditions specified. All specifications apply after two hours of storage at a constant temperature within the operating temperature range, after the instrument has been operating for 60 minutes, and after CAL ALL and CAL YTF have been run.

Definitions of Terms

The distinction between specifications, characteristics, typical performance, and nominal values is described as follows:

- Specifications describe warranted performance.
- Characteristics provide useful, but nonwarranted information about the functions and performance of the instrument.
- Typical Performance, where listed, is not warranted, but indicates performance which most units will exhibit.
- Nominal Value is an expected, but not warranted, value of the parameter.

General Specifications: HP 8546A EMI Receiver

Temperature Range	
Operating*	0 °C to +55 °C
Storage	-20 °C to +65 °C
* Disk drive +5 °C to +45 °C	

EMI Compatibility

Receiver is in compliance with CISPR Pub. 16.

Receiver radiated and conducted emissions performance is in compliance with CISPR Pub. 11/1990 Group 1 Class B.

Receiver susceptibility performance is in compliance with CISPR Pub. 16 at 3 V/m field strength.

Inputs	
Low frequency	Type N, 50 Ω, 9 kHz to 50 MHz
High frequency	Type N, 50 Ω, 9 kHz to 6.5 GHz

Detectors	
Measurement	Peak, Quasi-Peak, and Average
	Quasi-Peak and Average time constants conform with CISPR Pub.16.
Overload	Broadband RF (band 1 and 2 only) and IF

IF Bandwidths		
Measurement	200 Hz, 9 kHz, and 120 kHz	
	(6 dB bandwidths which conform to CISPR Pub.16)	
Bandwidth Accuracy	1 MHz, 6 dB bandwidth $\pm 10\%$	
Diagnostic	30 Hz to 300 kHz, 3 dB bandwidths in 1,3,10 steps (±20% characteristic), also 3 MHz and 5 MHz. Four-pole synchronously-tuned, approximately Gaussian shape.	

9 9	30 Hz to 1 MHz in 1,3,10 steps (±30% characteristic), and 3 MHz. Post-detection single pole low-pass filters.
	1,3,10 Hz digital filters with anti-aliasing

General Specifications: HP 8546A EMI Receiver (continued)

Input Attenuator	
Range	0 to 50 dB
Linearity Test Attenuator	4 dB
Preamplification	12 dB (Band 1 and 2)
	$27 \text{ dB} \pm 4 \text{ dB (Bypass)}$
Demodulation	AM and FM

DOS and LIF format disks

Input Filter Bandwidths	Frequency Range	Filter Type
(all 3 dB bandwidths are characteristics)	9 kHz to 74 kHz	fixed
	74 kHz to 198 kHz	fixed
	198 kHz to 525 kHz	fixed
	525 kHz to 1025 kHz	fixed
	1 MHz to 2 MHz	fixed
	2 MHz to 6 MHz	tunable (20%, 3 dB)
	6 MHz to 17 MHz	tunable (10%, 3 dB)
	17 MHz to 29 MHz	tunable (7%, 3 dB)
	29 MHz to 52 MHz	tunable (8%, 3 dB)
	52 MHz to 98 MHz	tunable (6%, 3 dB)
	98 MHz to 152 MHz	tunable (6%, 3 dB)
	152 MHz to 216 MHz	tunable (6%, 3 dB)
	216 MHz to 330 MHz	tunable (5%, 3 dB)
	330 MHz to 500 MHz	tunable (5%, 3 dB)
	0.5 GHz to 1 GHz	tunable (4%, 3 dB)
	1 GHz to 2.9 GHz	fixed
	1 GHz to 6.5 GHz	fixed

General Specifications: HP 8546A EMI Receiver (continued)

Sweep Time	
Range	20 ms to 100 s
Sweep Trigger	Free Run, Single, Line, Video, External

Audible Noise	<5.5 Bels power (ISODP 7779)
---------------	------------------------------

Power Requirements		
On	Receiver RF Section	90 to 132 V rms, 47 to 440 Hz
		198 to 264 V rms, 47 to 66 Hz
		Power consumption <500 VA; <180 W
	RF Filter Section	90 to 132 V rms, 47 to 440 Hz 198 to 264 V rms, 47 to 66 Hz Power consumption <115 VA; <85 W
Off	Receiver RF Section	Power consumption <5 W

Environmental Conditions	
Environment	Indoor Use
Altitude	Up to 15,000 feet (4,572 meters)
Maximum Relative Humidity	80% for temperatures up to 31 °C decreasing linearly to 50% relative humidity at 40 °C.
INSTALLATION CATEGORY II according to IEC 1010	
POLLUTION DEGREE 2 according to IEC 664	

Tuning Specifications

Tuning Range		
Band 1	9 kHz to 50 MHz	
Band 2	20 MHz to 2.9 GHz	
Band 3	1 GHz to 6.5 GHz	
Bypass	9 kHz to 6.5 GHz	

Frequency Reference	
Aging	\pm 1 x 10^{-7} /year
Settability	$\pm 1 \times 10^{-8}$
Temperature Stability	$\pm 1 \times 10^{-8}$

Frequency Readout Accuracy	± (frequency readout x frequency reference error * + span accuracy		
	+ 1% of span + 20% of IF Bandwidth + 100 Hz) †		

 $^{{\}rm *Frequency\ reference\ error = (aging\ rate\ x\ period\ of\ time\ since\ last\ adjustment\ +\ initial\ achievable\ accuracy\ +\ temperature}$ stability). See frequency characteristics.

†See "Drift" under "Stability" in frequency characteristics.

Frequency 300 MHz fundamental	Calibrator	
Accuracy son fraquency reference error*	Frequency	300 MHz fundamental
Accuracy see frequency reference effor	Accuracy	see frequency reference error*

 $^{{\}rm *Frequency\ reference\ error = (aging\ rate\ x\ period\ of\ time\ since\ last\ adjustment\ + initial\ achievable\ accuracy\ +\ temperature}$ stability). See frequency characteristics.

Swept Frequency Specifications

Frequency Span		
Range	Band 1	1 kHz to 50 MHz
	Band 2	1 kHz to 2.9 GHz
	Band 3	1 kHz to 5.5 GHz
	Bypass	1 kHz to 6.5 GHz
Resolution	Four digits or 20 Hz, whichever	er is greater
Accuracy*	Bands 1 and 2	Band 3 and Bypass
Span ≤ 10 MHz	±2% of Span + 10 Hz	$\pm 4\%$ of Span
Span > 10 MHz	±3% of Span	$\pm 6\%$ of Span
*Sweep time > 75 ms		

Stability	
Noise sidebands*	
>10 kHz offset from CW signal	≤-90 dBc/Hz
>30 kHz offset from CW signal	\leq -105 dBe/Hz
Residual FM	
30 Hz IF BW, 30 Hz Averaging BW	≤30 Hz pk-pk in 300 ms
1 kHz IF BW, 1 kHz Averaging BW	<pre> ≤250 Hz pk-pk in 100 ms</pre>
System Related Sidebands	≤-65 dBc
>30 kHz offset from CW signal	
* 1 kHz IF BW, 30 Hz averaging BW, sample detector.	

Marker Count Accuracy‡			
Frequency Spans ≤ 10 MHz	±(marker frequency x frequency reference error* + counter resolution + 100 Hz)		
Frequency Spans > 10 MHz	±(marker frequency x frequency reference error* + counter resolution + 1 kHz)		
Counter Resolution			
Frequency Spans ≤10 MHz	Selectable from 10 Hz to 100 kHz		
Frequency Spans > 10 MHz Selectable from 100 Hz to 100 kHz			
	d of time since last adjustment + initial achievable accuracy + temperature		
stability). See frequency characteristics. Marker level to displayed noise level >25 dB, IF	Randwidth/Span >0.01 Span < 300 MHz		

Amplitude Specifications

Amplitude specifications do not apply for negative peak detector mode except as noted in "Amplitude Characteristics."


Amplitude Range	-146 dBm to +30 dBm
	$-39 \text{ dB}\mu\text{V to} + 137 \text{ dB}\mu\text{V}$

Displayed Average Noise Level	Band 1	Band 2	Band 3	Bypass
$f_{o} > 400 \text{ kHz}$	9 kHz to	20 MHz to	1 GHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$6.5~\mathrm{GHz}$	$6.5~\mathrm{GHz}$
(input terminated, 0 dB attenuation, 30 Hz IF BW,				
30 Hz Averaging BW, sample detection)				
Preamplifier On	< ≤-39 d	BμV>	$\leq -37 \mathrm{dB}\mu\mathrm{V}$	
	(-146	BμV> dBm)	(-144 dBm)	
Preamplifier Off	< ≤-31 d	BμV>	≤−16 dBµV	
	(-138	BμV> dBm)	(-123 dBm)	
Characteristic Noise Figure				
Preamplifier On	< 10	dB>	8 dB	
Preamplifier Off	< 14	dB>	24 dB	

Displayed Average Noise Level

 $f_o < 400 \text{ kHz}$

(input terminated, 0 dB attenuation, 30 Hz IF BW, 30 Hz Averaging BW, sample detection)

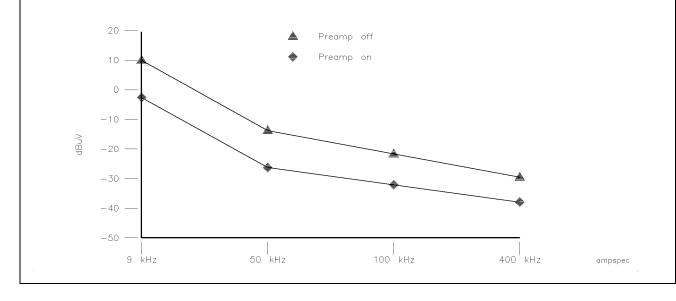

Noise Indication in CISPR Bandwidths			
(Characteristic)			
0 dB input attenuation, 50Ω input termination	Peak ————	Quasi-Peak	Average
200 Hz (6 dB), 9 kHz to 150 kHz			
Preamplifier On	$2 \text{ dB}\mu\text{V to } -28 \text{ dB}\mu\text{V}$	$-7~\mathrm{dB}\mu\mathrm{V}$ to $-29~\mathrm{dB}\mu\mathrm{V}$	-9 dB μ V to -31 dB μ V
	(-105 dBm to -135 dBm)	(-114 dBm to -136 dBm)	(-116 dBm to -138 dBm)
Preamplifier Off	15 dBμV to –15 dBμV	6 dB μ V to -25 dB μ V	$3~\mathrm{dB}\mu\mathrm{V}$ to $-27~\mathrm{dB}\mu\mathrm{V}$
	(-92 dBm to -122 dBm)	(-101 dBm to -132 dBm)	(-104 dBm to -134 dBm)
9 kHz (6 dB), 150 kHz to 30 MHz			
Preamplifier On	−8 dBµV	$-15 \mathrm{dB}\mu\mathrm{V}$	$-21 \mathrm{dB}\mu\mathrm{V}$
	(-115 dBm)	(-122 dBm)	(-128 dBm)
Preamplifier Off	$-3 \mathrm{dB}\mu \mathrm{V}$	$-11~\mathrm{dB}\mu\mathrm{V}$	$-18~\mathrm{dB}\mu\mathrm{V}$
	(-110 dBm)	(-118 dBm)	(-125 dBm)
120 kHz (6 dB), 30 MHz to 1 GHz			
Preamplifier On	$4~\mathrm{dB}\mu\mathrm{V}$	$-2 dB\mu V$	$-10 \mathrm{dB}\mu\mathrm{V}$
-	(-103 dBm)	(-109 dBm)	(-117 dBm)
Preamplifier Off	9 dBμV	$2~\mathrm{dB}\mu\mathrm{V}$	$-5~\mathrm{dB}\mu\mathrm{V}$
	(-98 dBm)	(-105 dBm)	(-112 dBm)

	Band 1 9 kHz to 50 MHz	Band 2 20 MHz to 2.9 GHz	Band 3 1 GHz to 6.5 GHz	Bypass 9 kHz to 6.5 GHz	
em Amplitude Accuracy					
ication†	<±2 dI	<±2 dB> <±1 dB> ±3 dB			
teristic‡	<±1 dI	<> ±3 dB			

^{† &}gt;(-10 dBμV + attenuation +(12 - preamplifier gain)) reference level. Use Measure at Marker or linear mode, top 4 graticules. If using the Measure at Marker function to measure a pulsed signal with a repetition frequency of less than 5 Hz, set the sweep time to be greater than or equal to the inverse of the pulse repetition frequency. (For example, to measure a 1 Hz CISPR pulse, set the sweep time to 1 second or greater prior to using the Measure at Marker function.) If IFBW ≤ 300 Hz and signal separation ≤ 4 kHz, also use Linearity Check. ‡ 20 °C to 30 °C plus the above. (Plus YIG filter peaked, Band 3 only.)

	Band 1 Band 2 Band 3 Bypass
	9 kHz to 20 MHz to 1 GHz to 9 kHz to
	50 MHz 2.9 GHz 6.5 GHz 6.5 GHz
Gain Compression*	
Specification	
$f_o \ge 10 \text{ MHz}$	<>
200 kHz≤f₀<10 MHz	<>
Characteristic 1 dB Compression Point	
$f_o \ge 10 \text{ MHz}$	
Preamplifier On	<> (-30 dBm)
Preamplifier Off	$<> 89 \text{ dB}\mu\text{V}> 102 \text{ dB}\mu\text{V} $ $(-18 \text{ dBm}) (-5 \text{ dBm})$
9 kHz <f<sub>o<10 MHz</f<sub>	
Preamplifier On	$72~\mathrm{dB}\mu\mathrm{V}$
	(-35 dBm)
Preamplifier Off	$85~\mathrm{dB}\mu\mathrm{V}$
-	(-22 dBm)
Third Harmonic Intercept Point**	
Specification	
$f_o > 200 \text{ kHz}$	
Preamplifier On	$<> 85 dB\mu V> < 85 dB\mu V> (-22 dBm) (-22 dBm)$
Preamplifier Off	$<>$ 97 dB μ V $> < 112 dB\muV> (-10 \text{ dBm}) (+5 \text{ dBm})$
Characteristic	
$f_{o} \ge 10 \text{ MHz}$	
Preamplifier On	<> 92 dBμV>
-	(-15 dBm)
Preamplifier Off	$<>$ 101 dB μ V $>$
	(-6 dBm)
9 kHz < f _o < 10 MHz	
Preamplifier On	< 89 dBuV>
	<> (-18 dBm)
Preamplifier Off	<> 100 dBμV>
	(-7 dBm)
*Indicated specification is derived from measured dis	stortion with a total power at the input mixer of -10 dBm. Bands 1

^{*}Indicated specification is derived from measured distortion with a total power at the input mixer of -10 dBm. Bands 1 and 2: Power at the input mixer=input power - input attenuation + 15 dB + preamplifier gain. Band 3 and Bypass: Power at the input mixer=input power - input attenuation + preamplifier gain. If the IFBW is ≤ 300 Hz, this applies only if signal separation is ≥ 4 kHz and signal amplitudes \leq Ref. Level + 10 dB.

^{**} Signal separation > 50 kHz. Indicated specification derived from measured distortion products for two −30 dBm CW signals at the input.

	Band 1 Band 2 9 kHz to 20 MHz to 50 MHz 2.9 GHz	Band 3 1 GHz to 6.5 GHz	Bypass 9 kHz to 6.5 GHz
Second Harmonic Intercept Point*			
Specification†			
$100~\mathrm{kHz} \leq \mathrm{f} \leq 1.8~\mathrm{GHz}, >2.9~\mathrm{GHz}$			
Preamplifier On	<> (+3 dBm)	$100 \mathrm{dB}\mu\mathrm{V}$ $(-7 \mathrm{dBm})$	
Preamplifier Off	<> (+ 15 dBm)	$134~\mathrm{dB}\mu\mathrm{V}$ (+27 dBm)	
$1.8~\mathrm{GHz} < \mathrm{f} \le 2.9~\mathrm{GHz}$			
– Preamplifier On	$105~\mathrm{dB}\mu\mathrm{V}$		
	(-2 dBm)		
Preamplifier Off	105 dB _μ V (-2 dBm)		
Characteristic			
9 kHz \leq f \leq 1.8 GHz			
Preamplifier On	<> (+20 dBm)		
Preamplifier Off	<> (+30 dBm)		
$1.8~\mathrm{GHz} < \mathrm{f} \le 2.9~\mathrm{GHz}$			
Preamplifier On	$114 dB\mu V $ (+7 dBm)		
Preamplifier Off	$112~\mathrm{dB}\mu\mathrm{V}$ (+5 dBm)		

^{*} f is the receiver tune frequency (second harmonic frequency).
† Indicated specification level was derived from measured harmonic levels for a -40 dBm input signal.

	Band 1	Band 2	Band 3	Bypass
	9 kHz to	20 MHz to	1 GHz to	9 kHz to
	50 MHz	$2.9~\mathrm{GHz}$	$6.5~\mathrm{GHz}$	6.5 GHz
Other Input Related Spurious†				
	<	65 dBc	>	
Residual Responses				
Input terminated, 0 dB attenuation (preamplifier on)				
>30 kHz	<	< - 10	dBμ V————	>
		(-117 d	Bm)	
<30 kHz	<	< - 2 ·	dΒμV	>
		(-109 d	Bm)	
Maximum Safe Input Level				
Average Continuous Power	<+30	dBm>	<+30	dBm
			(Input atte	n ≥10 dB)
Peak Pulse Power	2000 W peak	100 W for <		
	for 10 μs >	$10~\mu \mathrm{s}$ pulse		
	20 dB input	width <1%		
	attenuation	duty cycle and >30 dB input		
		attenuation		
DC (Volts)	<	0 V	>	
Input VSWR				
0 dB input attenuation			3:1*	
≤1.0 GHz	< 2	: 1>		
_ 1.0 GHz <f<sub>o≤2.9 GHz</f<sub>		<- 2.5 : 1 ->		
10 dB input attenuation			2:1*	
≤1.0 GHz	< 1.2	: 1>		
$1.0 \text{ GHz} < f_{\circ} \le 2.9 \text{ GHz}$		<- 1.6 : 1 ->		

Marker Readout Resolution	0.05 dB for log scale
	0.05% of reference level for linear scale

Reference Level	
Range	
Log Scale	-146 dBm to +30 dBm
Linear Scale	-126 dBm to +30 dBm
Resolution	
Log Scale	$\pm 0.01 \text{ dB}$
Linear Scale	± 0.12 % of reference level

Linear to Log Switching	± 0.25 dB at reference level

Display Scale Fidelity	
Log Maximum Cumulative*	
3 kHz to 3 MHz IF Bandwidth	±(0.3 dB + 0.01 x dB from Reference level)
≤ 1 kHz IF Bandwidth	$\pm (0.4 \text{ dB} + 0.01 \text{ x dB from Reference level})$
Log Incremental Accuracy 0 to -56 dB from Reference Level (0 to -54 dB, Band 3 only)	±0.4 dB/4 dB
Linear Accuracy	±3% of Reference Level
* 0 to -66 dB from reference level. 0 to -64 dB Band 3 only.	

Relative Quasi-Peak Response to a CISPR Pulse (dB)*		Frequency Bands	
Pulse Repetition Frequency	$120~\mathrm{kHz}~6~\mathrm{dB}~\mathrm{BW}$	9 kHz 6 dB BW	$200~\mathrm{Hz}~6~\mathrm{dB}~\mathrm{BW}$
(Hz)	$0.03~\mathrm{GHz}$ to $1~\mathrm{GHz}$	0.15 MHz to 30 MHz	9 kHz to 150 kHz
1000	$+8.0 \pm 1.0$	$+\ 4.5\ \pm1.0$	
100	0 dB (reference)†	0 dB (reference)†	$+\ 4.0\ \pm1.0$
60			$+3.0 \pm 1.0$
25			0 dB (reference)†
20	-9.0 ± 1.0	-6.5 ± 1.0	
10	-14.0 ± 1.5	-10.0 ± 1.5	-4.0 ± 1.0
5			-7.5 ± 1.5
2	-26.0 ± 2.0	-20.5 ± 2.0	-13.0 ± 2.0
1	-28.5 ± 2.0	-22.5 ± 2.0	-17.0 ± 2.0
Isolated Pulse	-31.5 ± 2.0	-23.5 ± 2.0	-19.0 ± 2.0

^{*} Specification applies to a pulsed RF signal with equivalent spectral intensity as called out in CISPR Pub.16, Part 1. (CISPR pulse measurements require either an HP 8542E or HP 8546A EMI receiver and do not apply to either an HP 85422E or HP 85462A receiver RF section.)

 $[\]dagger$ Reference pulse amplitude accuracy relative to the CW signal is <1.5 dB as specified in CISPR pub. 16. CISPR reference pulse: $0.044~\mu Vs$ for .03 GHz to 1 GHz, $0.316~\mu Vs$ for .15 MHz to 30 MHz, $13.5~\pm 1.5~\mu Vs$ for 9 kHz to 150 kHz.

Tracking Generator Specifications

All Specifications apply over 0° C to 55° C. The receiver/tracking generator combination will meet its specification after 2 hours of storage at a constant temperature within the operating temperature range, 30 minutes after the combination is turned on, and after CAL ALL, CAL TRK GEN, and TRACKING PEAK have been run.

Output Frequency Range	9 kHz to 2.9 GHz
output 11 equency mange	V KIIZ TO 2.0 CIIZ
Warm-up time	30 minutes
Output Power Level	
Range	-1 dBm to -66 dBm
Resolution	0.1 dB
Vernier	1
Range	9 dB
Accuracy	
(25 °C ±10 °C)	
(-20 dBm at 300 MHz, 16 dB attenuation)	$\pm 0.2 \text{ dB/dB}$
Incremental Cumulative	$\pm 0.5~\mathrm{dB}$ Total
Output Attenuator Range	0 to 56 dB in 8 dB steps
Output Power Sweep	
Range	(−10 dBm to −1 dBm) − (source attenuator setting)
Resolution	0.1 dB
Tracking Generator Feedthrough	
400 kHz to 2.9 GHz	≤ -110 dBm
Spurious Output (-1 dBm output)	
Harmonic Spurs from 300 kHz to 2.9 GHz	
TG output 300 kHz to 2.9 GHz	$\leq -25 \text{ dBc}$
Non-harmonic Spurs from 300 kHz to 2.9 GHz	
Non-narmonic Spurs from 300 kHz to 2.9 GHz TG output 300 kHz to 2.0 GHz	≤ −27 dBc
TG output 2.0 GHz to 2.9 GHz	≤ −27 dBc < −23 dBc
13 Suspending Gills to Bio Gills	2 25 450
LO Feedthrough	
LO frequency 3.9214 GHz to 6.8214 GHz	≤ -16 dBm

Frequency Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Frequency Reference	
Aging	$5 \times 10^{-10}/{\rm day}, 7 {\rm day}$ average after being powered on for seven days
Warm-up	1×10^{-8} after 30 minutes on
Initial Achievable Accuracy	$\pm 2.2 \times 10^{-8}$ after being powered on for 24 hours

ninute of sweep time
_

Drift occurs only while receiver is sweeping frequency. Additional drift occurs when using Line, Video, or External trigger while waiting for the appropriate trigger.

Amplitude Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Input Attenuator Uncertainty	
Attenuator Setting (Band 3 and Bypass)	
0 dB	$\pm~0.2~\mathrm{dB}$
10 dB	Reference
20 dB	$\pm~0.4~\mathrm{dB}$
30 dB	$\pm~0.5~\mathrm{dB}$
40 dB	$\pm~0.7~\mathrm{dB}$
50 dB	\pm 0.8 dB
10 dB Step Uncertainty (attenuator setting 10 to 50 dB)	\pm 0.8 dB/dB
Repeatability	±0.05 dB

Relative†
±1 dB
±1 dB

FM Demodulation	
Input Level	
Preamplifier Off	>(-75 dBm + attenuator setting)
Signal Level	0 to -30 dB below reference level
FM Offset	400 Hz nominal
FM Deviation (FM GAIN)	
Resolution	1 kHz/volt nominal
Range	10 kHz/volt to 1 MHz/volt
Bandwidth	FM Deviation ÷ 2
FM Linearity	≤ 1% of FM deviation + 290 Hz

Tracking Generator Characteristics

Output Flatness	
(referenced to 300 MHz, -20 dBm)	
Frequency > 10 MHz	$\pm 2 \text{ dB}$
Frequency ≤10 MHz	±3 dB
Output Power Level	
Absolute Accuracy	±0.75 dB
(-20 dBm at 300 MHz)	
(25 °C ±10 °C)	
	<u>I</u>
Tracking Drift	
Usable in a 1 kHz IF Bandwidth after a 5 minute warm-up	1.5 kHz/5 minutes
RF Power Off Residuals	
9 kHz to 2.9 GHz	< -120 dBm
Dynamic Range	
(Difference between maximum power out and tracking generator feedthrough)	> 109 dB
Output Attenuator Repeatability	
300 kHz to 300 MHz	±0.1 dB
300 MHz to 2.0 GHz	±0.2 dB
2.0 GHz to 2.9 GHz	±0.3 dB
Output VSWR	
0 dB attenuation	<3.0:1
8 dB attenuation	<1.5:1

Physical Characteristics

Front Panel Inputs and Outputs	
Low Frequency Input	Type N female, 50 Ω nominal
High Frequency Input	Type N female, 50 Ω nominal
Tracking Generator Output	Type N female, 50 Ω nominal
Probe Power*	
Voltage / Current	$+15~{ m Vdc}~{\pm}7\%$ at $150~{ m mA}$ maximum
	$-12.6~{ m Vdc}~{\pm}10\%$ at $150~{ m mA}$ maximum
Earphone Jack	1/8 inch monaural jack

 $^{^*}$ Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE connectors cannot exceed 150 mA. Total current drawn from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE cannot exceed

Rear Panel Inputs and Outputs	
10 MHz REF OUTPUT	
Connector	BNC female
Impedance	50 Ω
Output Amplitude	> 0 dBm
EXT REF IN	
Connector	BNC female
Input Amplitude Range	-2 dBm to +10 dBm
Frequency	10 MHz
Trequency	10 3333
AUX IF OUT	
Connector	BNC female
Frequency	21.4 MHz
Amplitude Range	-10 dBm to -60 dBm
Impedance	50 Ω
AUX VIDEO OUT	
Connector	BNC female
Amplitude Range	0 V to 1 V (uncorrected)
EXT KEYBOARD	Interface compatible with HP part number C1405 Option
	ABA and most IBM/AT non auto-switching keyboards.
EXT TRIG INPUT	
Connector	BNC female
Trigger Level	Positive edge initiates sweep in EXT TRIG mode (TTL)
LO OUTPUT	
Connector	SMA female (must be terminated in 50 Ω when not used)
Impedance	50 Ω
Frequency Range	3.0 GHz to 6.8214 GHz

Physical Characteristics (continued)

Rear Panel Inputs and Outputs (continued)	
HI-SWEEP IN/OUT	
Receiver RF Section Input/Output	
Connector	SMA female
Output	High = sweep, Low = retrace (TTL)
Input	Open collector, Low stops sweep
RF Filter Section Output	High = sweep, Low = retrace (TTL)
SWEEP INPUT / OUTPUT	
Receiver RF Section Output	
Connector	SMA female
Output	0 V to + 10 V ramp
RF Filter Section Input	
Connector	SMA female
Input	0 V to +10 V
REMOTE INTERFACE	
Receiver RF Section	HP-IB (RS-232 optional)
RF Filter Section	HP-IB compatible service port
MONITOR OUTPUT	R, G, B (composite video on G)
	25 kHz horizontal rate
	60 Hz vertical rate

AUX INTERFACE Connector Type: 9-pin s	ubminiature D			
Connector Pinout:				
Pin #	Function	Current	Logic Mode	Serial Bit Mode
1	Control A		TTL Output Hi/Lo	TTL Output Hi/Lo
2	Control B		TTL Output Hi/Lo	TTL Output Hi/Lo
3	Control C		TTL Output Hi/Lo	Strobe
4	Control D		TTL Output Hi/Lo	Serial Data
5	Control I		TTL Input Hi/Lo	TTL Input Hi/Lo
6	Gnd		Gnd	Gnd
7*	$-15~\mathrm{Vdc}~\pm7\%$	150 ma		
8*	$+5~\mathrm{Vdc}~\pm5\%$	150 ma		
9*	$+$ 15 Vdc $\pm 5\%$	150 ma		

^{*} Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE cannot exceed 150 mA. Total current drawn from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE cannot exceed 150 mA.

WEIGHT	
Receiver RF Section	62.5 lb.
RF Filter Section	46 lb.

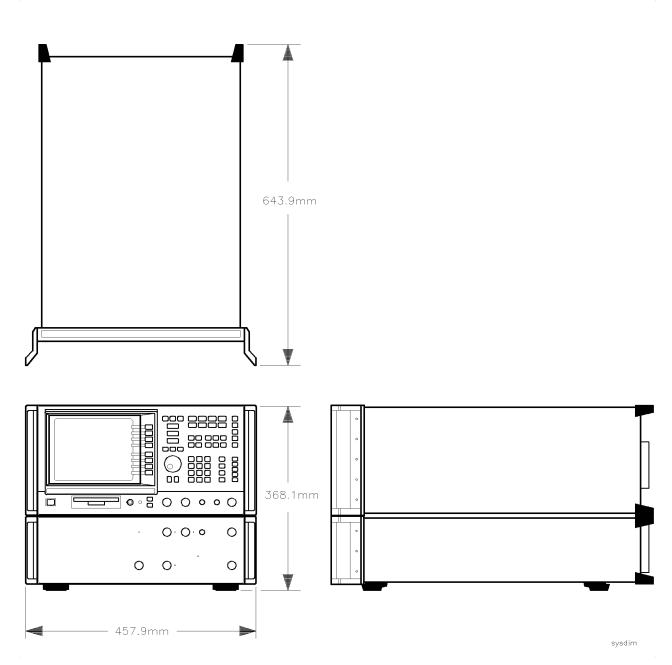


Figure 2-1. HP 8546A EMI Receiver Dimensions

General Specifications: HP 85462A Receiver RF Section

The specifications in this section apply to all functions autocoupled over the environmental conditions specified. All specifications apply after two hours of storage at a constant temperature within the operating temperature range, after the instrument has been operating for 60 minutes, and after CAL ALL and CAL YTF have been run.

Temperature Range	
Operating*	0 °C to +55 °C
Storage	-20 °C to +65 °C
* Disk drive +5 °C to +45 °C	

EMI Compatibility

Receiver RF section radiated and conducted emissions performance is in compliance with CISPR Pub. 11/1990 Group 1 Class B. Receiver RF section susceptibility is in compliance with CISPR Pub. 16 at 3 V/m.

Inputs	Type N, 50 Ω, 9 kHz to 6.5 GHz
Detectors	
Measurement	Peak, Quasi-Peak, and Average.
	Quasi-Peak and Average time constants conform with CISPR Pub.16.
Overload	IF
IF Bandwidths	
Measurement	200 Hz, 9 kHz, and 120 kHz
	(6 dB bandwidths which conform to CISPR Pub.16)
Bandwidth Accuracy	1 MHz, 6 dB bandwidth $\pm 10\%$
Diagnostic	30 Hz to 300 kHz, 3 dB bandwidths in 1,3,10 steps (±20% characteristic), also 3 MHz and 5 MHz. Four-pole synchronously-tuned, approximately Gaussian shape.
Averaging Bandwidths	30 Hz to 1 MHz in 1,3,10 steps ($\pm 30\%$ characteristic), and 3 MHz. Post-detection single pole low-pass filters.
	1,3,10 Hz digital filters with anti-aliasing
Input Attenuator	
Range	0 to 70 dB in 10 dB steps
Preamplification	27 dB ±1.5 dB ≤500 MHz, ±4 dB >500 MHz
Demodulation	AM and FM

General Specifications: HP 85462A Receiver RF Section (continued)

Sweep Time		
Range	20 ms to 100 s	
Accuracy	±3%	
Sweep Trigger	Free Run, Single, Line, Video, External	
Sweep 1118801	Tree with origin, time, video, fixernal	
Disk Drive	Internal 3.5 inch disk drive, compatible with 1.44 MByte	
DISK DIIVC	DOS and LIF format disks	
	DOS and Eri Tornat disks	
Audible Noise	(5.5 Pl	
Audible Noise	< 5.5 Bels power (ISODP 7779)	
Power Requirements		
On	90 to 132 V rms, 47 to 440 Hz	
	198 to 264 V rms, 47 to 66 Hz	
	Power consumption <500 VA; <180 W	
Off	Power consumption <5 W	
Environmental Conditions		
Environment	Indoor Use	
Altitude	Up to 15,000 feet (4,572 meters)	
Maximum Relative Humidity	80% for temperatures up to 31 °C decreasing linearly to $50%$ relative humidity at 40 °C.	
INSTALLATION CATEGORY II according to IEC 1010		
POLLUTION DEGREE 2 according to IEC 664		

Tuning Specifications

Tuning Range	
DC Coupled	9 kHz to 6.5 GHz
AC Coupled	100 kHz to 6.5 GHz

Frequency Reference	
Aging	$\pm 1 \times 10^{-7}$ /year
Settability	$\pm 1 \times 10^{-8}$
Temperature Stability	$\pm 1 \times 10^{-8}$

- ·	\pm (frequency readout x frequency reference error * + span accuracy + 1% of span + 20% of IF Bandwidth + 100 Hz) †
*Frequency reference error=(aging rate x period of time since last adjustment + initial achievable accuracy + temperature	

stability). See frequency characteristics.

†See "Drift" under "Stability" in frequency characteristics.

Calibrator	
Frequency	300 MHz fundamental
Accuracy	see frequency reference error*

 ${}^*Frequency\ reference\ error = (aging\ rate\ x\ period\ of\ time\ since\ last\ adjustment\ + initial\ achievable\ accuracy\ +\ temperature$ stability). See frequency characteristics.

Swept Frequency Specifications

Frequency Span	
Range	1 kHz to 6.5 GHz
Resolution	Four digits or 20 Hz, whichever is greater
Accuracy (single mixing band spans)	
Span ≤ 10 MHz	±2% of span + 10 Hz
Span > 10 MHz	±3% of span


Stability	
Noise sidebands*	
>10 kHz offset from CW signal	≤-90 dBc/Hz
>30 kHz offset from CW signal	≤-105 dBc/Hz
Residual FM	
30 Hz IF BW, 30 Hz Averaging BW	≤30 Hz pk-pk in 300 ms
1 kHz IF BW, 1 kHz Averaging BW	≤250 Hz pk-pk in 100 ms
System Related Sidebands	≤-65 dBc
>30 kHz offset from CW signal	
* 1 kHz IF BW, 30 Hz averaging BW, sample detector.	

Marker Count Accuracy‡	
Frequency Spans ≤ 10 MHz	±(marker frequency x frequency reference error* + counter resolution + 100 Hz)
Frequency Spans > 10 MHz	±(marker frequency x frequency reference error* + counter resolution + 1 kHz)
Counter Resolution	
Frequency Spans ≤10 MHz	Selectable from 10 Hz to 100 kHz
Frequency Spans >10 MHz	Selectable from 100 Hz to 100 kHz
	e last adjustment + initial achievable accuracy + temperature
stability). See frequency characteristics. ‡Marker level to displayed noise level >25 dB, IF Bandwidth/	Span ≥0.01, Span ≤300 MHz.

Amplitude Specifications


Amplitude specifications do not apply for negative peak detector mode except as noted in "Amplitude Characteristics."

Amplitude Range	-146 dBm to +30 dBm
	$-39 \text{ dB}\mu\text{V to} + 137 \text{ dB}\mu\text{V}$

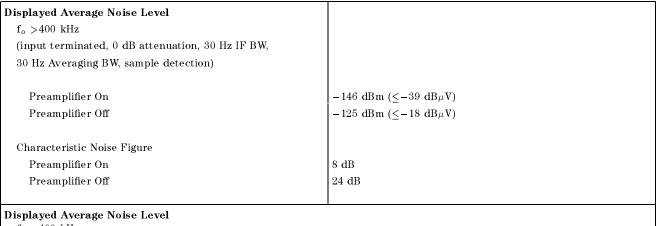

 $f_{\circ} < 400 \text{ kHz}$

(input terminated, 0 dB attenuation, 30 Hz IF BW, 30 Hz Averaging BW, sample detection)

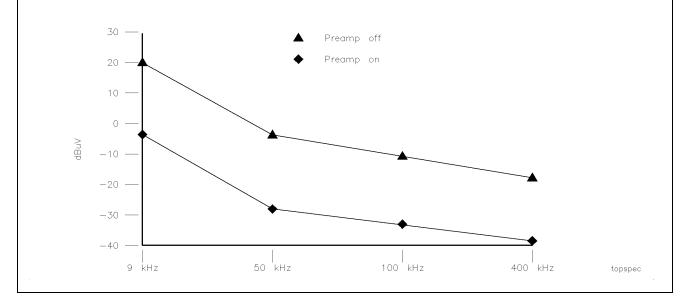

Gain Compression*	
Specification	
$f_o > 10 \text{ MHz}$	<0.5 dB
$200 \text{ kHz} \leq f_{\circ} \leq 10 \text{ MHz}$	<0.75 dB
Characteristic 1 dB Compression Point	
$f_o > 10 \text{ MHz}$	
Preamplifier On	$75 \text{ dB}\mu\text{V} \text{ (}-32 \text{ dBm)}$
Preamplifier Off	$102 \text{ dB}\mu\text{V} (-5 \text{ dBm})$
$9 \text{ kHz} \le f_o \le 10 \text{ MHz}$	
Preamplifier On	$68 \text{ dB}\mu\text{V} (-39 \text{ dBm})$
Preamplifier Off	$95 \text{ dB}\mu\text{V} (-12 \text{ dBm})$

^{*} Specifications derived from distortion measurements using a two-tone compression test with frequency offset of 30 MHz and -10 dBm total signal power at the input mixer. Total power at first mixer = input power input atten + preamp gain. IF BW \(\le 300\) Hz, this applies only if signal separation \(\ge 4\) kHz and signal amplitudes ≤ Reference Level + 10 dB.

hird Order Intercept Point†		
Specification		
$f_{\circ} > 200 \text{ kHz}$		
Preamplifier On	$85 \text{ dB}\mu\text{V} (-22 \text{ dBm})$	
Preamplifier Off	112 dB μ V (+ 5 dBm)	
Characteristic Third Order Intercept		
$f_{o} > 10 \text{ MHz}$		
Preamplifier On	89 dB _μ V (-18 dBm)	
Preamplifier Off	118 dB μ V (+11 dBm)	
$9 \text{ kHz} \le f_{\circ} \le 10 \text{ MHz}$		
Preamplifier On	$87 \text{ dB}\mu\text{V} (-20 \text{ dBm})$	
Preamplifier Off	115 $dB\mu V (+8 dBm)$	

signals at the first mixer and 50 kHz separation. Input mixer power = input power - input attenuation + preamp gain.

econd Harmonic Intercept*	
$f_o > 200 \text{ kHz}$	
Preamplifier On	$100 dB\mu V (-9 dBm)$
Preamplifier Off	$134~\mathrm{dB}\mu\mathrm{V}~(+27~\mathrm{dBm})$
Characteristic Second Order Intercept	
Preamplifier On	
$f_o > 500 \text{ MHz}$	$115 \mathrm{dB}\mu \mathrm{V} (+8 \mathrm{dBm})$
$9 \text{ kHz} \le f_o \le 500 \text{ MHz}$	$108 \mathrm{dB}\mu\mathrm{V} (+1 \mathrm{dBm})$
Preamplifier Off	$144 dB\mu V (+37 dBm)$

^{*} The indicated specification level was derived from a measured harmonic level of <-67 dBc and a -40 dBm CW signal at the input mixer. Input mixer power = input power = input attenuation + preamp gain.

Other Input Related Spurious	-65 dBc
30 kHz offset for -20 dBm tone at the mixer ≤2.9 GHz, f _o >10 MHz. Input mixer power = input power - input attenuation + preamp gain.	

Residual Responses	
Input terminated, 0 dB attenuation, preamplifier on	
150 kHz to 6.5 GHz	$-8 \text{ dB}\mu\text{V} \ (-115 \text{ dBm})$
9 kHz to 150 kHz	$+2 \text{ dB}\mu\text{V} (-105 \text{ dBm})$

Maximum Safe Input Level	
Average Continuous Power	
9 kHz to 2.9 GHz	+ 30 dBm
2.9 GHz to 6.5 GHz	+30 dBm (with 10 dB input attenuation)
Peak Pulse Power Preamplifier Off	$+50$ dBm (100 W) for 10 μs pulse width and, 1% duty cycle, input atten $\geq\!30$ dB.
DC	0 V (dc coupled)
	50 V (ac coupled)

Calibrator Output	
Amplitude	$-20 \text{ dBm} \pm 0.4 \text{ dB}$

Calibration Donastability*	±0.15 dB
Calibration Repeatability*	1 ±0.15 dB

*Repeatability in the measured absolute amplitude of the CAL OUT signal at the reference settings after CAL FREQ and CAL AMPTD self-calibration. Absolute amplitude reference settings are: -20 dB reference level; 10 dB input attenuation; 300 MHz center frequency; 3 kHz IF BW; 300 Hz averaging BW; linear scale; 50 kHz span; coupled sweep time; reference level positioned at the top graticule; corrections on; and sample detection.

Display Range	
Log Scale	0 to -66 dB from Reference Level is calibrated
	0.1, 0.2, 0.5 dB/division and 1 to 20 dB/division in 1dB steps; eight divisions displayed
Linear Scale	Eight divisions
Scale Units	dBm, dBmV, dB μ V, V, W

Marker Readout Resolution	0.05 dB for log scale
	0.05% of reference level for linear scale

Reference Level	
Range	
Log Scale	-146 dBm to +30 dBm
Linear Scale	-126 dBm to +30 dBm
Resolution	
Log Scale	$\pm 0.01 \text{ dB}$
Linear Scale	$\pm 0.12\%$ of Reference Level
Accuracy*	
0 dBm to -59.9 dBm	$\pm (0.3 \text{ dB} + 0.01 \text{ x dB from } -20 \text{ dBm})$
-60 dBm and below	
1 kHz to 3 MHz IF BW	$\pm (0.6 \text{ dB} + 0.01 \text{ x dB from } -20 \text{ dBm})$
30 Hz to 300 Hz IF BW	$\pm (0.7 \text{ dB} + 0.01 \text{ x dB from } -20 \text{ dBm})$

^{*} Referenced to -20 dBm reference level, 10 dB input attenuation, at a single frequency, in a fixed IF BW with preamplifier off. With preamplifier on, subtract preamplifier gain from all reference levels.

Linear to Log Switching	± 0.25 dB at reference level
Display Scale Fidelity	
Log Maximum Cumulative	
(0 to -66 dB from Reference Level)	
3 kHz to 3 MHz IF Bandwidth	$\pm (0.3 \text{ dB} + 0.01 \text{ x dB from Reference Level})$
≤ 1 kHz IF Bandwidth	$\pm (0.4 \text{ dB} + 0.01 \text{ x dB from Reference Level})$
Log Incremental Accuracy	$\pm 0.4 \text{ dB/4 dB}$
(0 to -56 dB from Reference Level)	
Linear Accuracy	$\pm 3\%$ of Reference Level

IF Bandwidth Switching Uncertainty	
(at Reference Level, referenced to 3 kHz IF BW)	
3 kHz to 3 MHz	$\pm 0.4~\mathrm{dB}$
1 kHz	$\pm 0.5~\mathrm{dB}$
30 Hz to 300 Hz	±0.6 dB

HP 85462A Receiver RF Section

Flatness		
(dc coupled, 10 dB input attenuation)	Absolute*	${\bf Relative}\dagger$
9 kHz to 2.9 GHz		
Preamplifier On	±3.0 dB	$\pm 2.0~\mathrm{dB}$
Preamplifier Off	±1.5 dB	$\pm 1.0~\mathrm{dB}$
2.9 GHz to 6.5 GHz (preselector peaked)		
Preamplifier On	±2.5 dB	$\pm 1.5~\mathrm{dB}$
Preamplifier Off	±2.0 dB	$\pm 1.5~\mathrm{dB}$
* Referenced to 300 MHz Calibrator		

[†] Referenced to midpoint between highest and lowest frequency response deviations.

Tracking Generator Specifications

All Specifications apply over 0° C to 55° C. The receiver/tracking generator combination will meet its specification after 2 hours of storage at a constant temperature within the operating temperature range, 30 minutes after the combination is turned on, and after CAL ALL, CAL TRK GEN, and TRACKING PEAK have been run.

Output Frequency Range	9 kHz to 2.9 GHz
Output Frequency nange	8 KHZ to 2.8 GHZ
Warm-up time	30 minutes
Output Power Level	
Range	-1 dBm to -66 dBm
Resolution	0.1 dB
Absolute Accuracy	±0.75 dB
(-20 dBm at 300 MHz)	
(25 °C ±10 °C)	
Vernier	
Range	9 dB
Accuracy	
(25 °C ±10 °C)	
(-20 dBm at 300 MHz, 16 dB attenuation)	$\pm 0.2 \text{ dB/dB}$
Incremental Cumulative	±0.5 dB Total
Output Attenuator Range	0 to 56 dB in 8 dB steps
Output Power Sweep	
Range	(-10 dBm to -1 dBm) - (source attenuator setting)
Resolution	0.1 dB
Output Flatness	
(referenced to 300 MHz, - 20 dBm)	
Frequency > 10 MHz	±2 dB
Frequency ≤10 MHz	±3 dB
<u> </u>	
Tracking Generator Feedthrough	
400 kHz to 2.9 GHz	≤ -110 dBm

Tracking Generator Specifications (continued)

Spurious Output (-1 dBm output)	
Harmonic Spurs from 300 kHz to 2.9 GHz TG output 300 kHz to 2.9 GHz	≤ −25 dBc
Non-harmonic Spurs from 300 kHz to 2.9 GHz TG output 300 kHz to 2.0 GHz TG output 2.0 GHz to 2.9 GHz	≤ -27 dBe ≤ -23 dBc
LO Feedthrough LO frequency 3.9214 GHz to 6.8214 GHz	≤ -16 dBm

Frequency Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Frequency Reference	
Aging	$5 \times 10^{-10}/\mathrm{day},7$ day average after being powered on for seven days
Warm-up	1 x 10 $^{-8}$ after 30 minutes on
Initial Achievable Accuracy	± 2.2 x 10 $^{-8}$ after being powered on for 24 hours

Stability	
Drift (after warm-up at stabilized temperature)	< 2 kHz/minute of sweep time
Frequency spans ≤ 10 MHz, free run trigger	

Drift occurs only while receiver is sweeping frequency. Additional drift occurs when using Line, Video, or External trigger while waiting for the appropriate trigger.

Amplitude Characteristics

These are not specifications. Characteristics provide useful but nonwarranted information about instrument performance.

Input Attenuator Uncertainty		
Attenuator Setting		
0 dB	$\pm~0.2~\mathrm{dB}$	
10 dB	Reference	
20 dB	\pm 0.4 dB	
30 d B	$\pm~0.5~\mathrm{dB}$	
40 dB	\pm 0.7 dB	
50 d B	± 0.8 dB	
60 d B	± 1.0 dB	
70 dB	± 1.0 dB	
10 dB Step Uncertainty	± 0.8 dB	
(attenuator setting 10 to 70 dB)		
Repeatability	±0.05 dB	

Unpeaked Frequency Response (dc coupled) (without preselector peaking, span ≤50 MHz, 10 dB input attenuation)	${ m Absolute}^*$	Relative†
2.75 to 6.5 GHz		
Preamplifier On	±3 dB	±1 dB
Preamplifier Off	±2 dB	±1 dB
* Referenced to 300 MHz CAL OUT. † Referenced to midpoint between highest and lowest frequency response deviations.		

AC Coupled Insertion Loss‡		
100 kHz to 300 kHz	0.7 dB	
300 kHz to 1 MHz	0.2 dB	
1 MHz to 100 MHz	0.07 dB	
100 MHz to 2.9 GHz	$0.05 \text{ dB} + (0.06 \times \text{F})^{**} \text{ dB}$	
2.9 GHz to 6.5 GHz	$0.05 \text{ dB} + (0.13 \times \text{F})^{**} \text{ dB}$	
‡ Referenced to dc coupled mode. ** F = frequency in GHz.		

Marker Readout Resolution	
(digitizing resolution)	
(digitizing resolution)	
Log Scale	$\pm 0.31~\mathrm{dB}$
Linear Scale	
Frequency ≤1 GHz	± 0.59 % of Reference Level
Frequency >1 GHz	$\pm 1.03~\%$ of Reference Level

Amplitude Characteristics (continued)

FM Demodulation		
Input Level	>(-60 dBm + attenuator setting)	
Signal Level	0 to -30 dB below reference level	
FM Offset	400 Hz nominal	
FM Deviation (FM GAIN)		
Resolution	1 kHz/volt nominal	
Range	10 kHz/volt to 1 MHz/volt	
Bandwidth (6 dB)	FM Deviation ÷ 2	
FM Linearity	≤ 1% of FM deviation + 290 Hz	

Tracking Generator Characteristics

Tracking Drift Usable in a 1 kHz IF Bandwidth after a 5 minute warm-up	1.5 kHz/5 minutes
RF Power Off Residuals	
9 kHz to 2.9 GHz	< -120 dBm
Dynamic Range	
(Difference between maximum power out and tracking generator feedthrough)	> 109 dB
Output Attenuator Repeatability	
300 kHz to 300 MHz	±0.1 dB
300 MHz to 2.0 GHz	$\pm 0.2~\mathrm{dB}$
2.0 GHz to 2.9 GHz	±0.3 dB
	1
Output VSWR	
0 dB attenuation	<3.0:1
8 dB attenuation	<1.5:1

Physical Characteristics

Front Panel Inputs and Outputs	
Input	Type N female, 50 Ω nominal
Calibrator Output	Type N female, 50 Ω nominal
Tracking Generator Output	Type N female, 50 Ω nominal
Probe Power*	
Voltage / Current	+ 15 Vdc ±7% at 150 mA max.
	-12.6 Vdc ±10% at 150 mA max.
Earphone Jack	1/8 inch monaural jack
External ALC	Negative Detector

 $^{^*}$ Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE connectors cannot exceed 150 mA. Total current draw from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE connectors cannot exceed 150 mA.

Rear Panel Inputs and Outputs	
10 MHz REF OUTPUT	
Connector	BNC female
Impedance	50 Ω
Output Amplitude	>0 dBm
EXT REF IN	
Connector	BNC female
Input Amplitude Range	-2 dBm to +10 dBm
Frequency	10 MHz
AUX IF OUT	
Connector	BNC female
Frequency	21.4 MHz
Amplitude Range	-10 dBm to -60 dBm
Impedance	50 Ω
AUX VIDEO OUT	
Connector	BNC female
Amplitude Range	0 to 1 V (uncorrected)

Physical Characteristics (continued)

Rear Panel Inputs and Outputs (continued)		
EXT KEYBOARD	Interface compatible with HP part number C1405 Option ABA and most IBM/AT non auto-switching keyboards.	
EXT TRIG INPUT		
Connector	BNC female	
Trigger Level	Positive edge initiates sweep in EXT TRIG mode (TTL)	
LO OUTPUT		
Connector	SMA female (must be terminated in 50 Ω when not used)	
Impedance	50 Ω	
Frequency Range	3.0 to 6.8214 GHz	
HI-SWEEP IN/OUT (input/output 85462A)		
Connector	SMA female	
Output	High-sweep, Low-retrace (TTL)	
Input	Open collector, low stops sweep	
SWEEP INPUT / OUTPUT (output 85462A)		
Connector	SMA female	
Output	0 to +10 V ramp	
REMOTE INTERFACE (85462A)	HP-IB (RS-232 optional)	
MONITOR OUTPUT	R, G, B (composite video on G)	
	25 kHz horizontal rate	
	60 Hz vertical rate	

AUX INTERFACE				
Connector Type: 9-pin :	subminiature D			
Connector Pinout:				
Pin #	Function	Current	Logic Mode	Serial Bit Mode
1	Control A		TTL Output Hi/Lo	TTL Output Hi/Lo
2	Control B		TTL Output Hi/Lo	TTL Output Hi/Lo
3	Control C		TTL Output Hi/Lo	\mathbf{Strobe}
4	Control D		TTL Output Hi/Lo	Serial Data
5	Control I		TTL Input Hi/Lo	TTL Input Hi/Lo
6	Gnd		Gnd	Gnd
7*	−15 Vdc ±7%	150 ma		
8*	$+5~\mathrm{Vdc}~\pm5\%$	150 ma		
9*	+ 15 Vdc ±5%	150 ma		

 $^{^{*}}$ Total current drawn from the +15 Vdc on the PROBE POWER and the AUX INTERFACE cannot exceed 150 mA. Total current drawn from the -12.6 Vdc on the PROBE POWER and the -15 Vdc on the AUX INTERFACE cannot exceed

WEIGHT	
Receiver RF Section	62.5 lb.

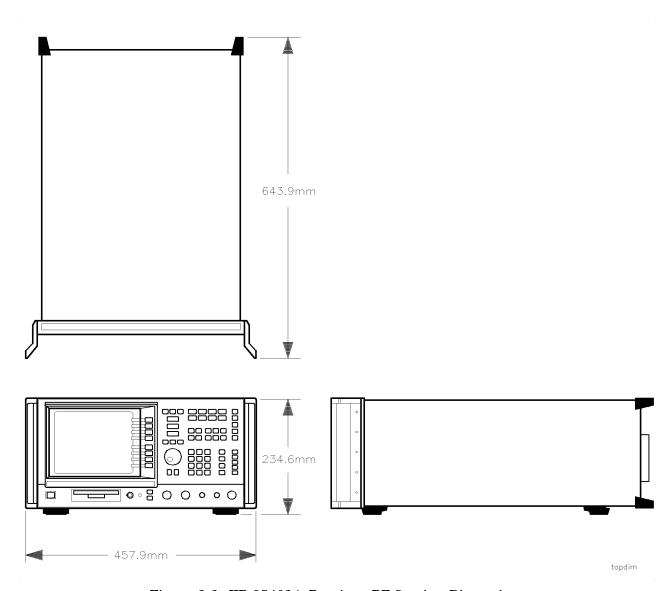


Figure 2-2. HP 85462A Receiver RF Section Dimensions

Regulatory Information

The information on the following page applies to the HP 8546A EMI receiver and HP 85462A receiver RF section.

DECLARATION OF CONFORMITY

according to ISO/IEC Guide 22 and EN 45014

Manufacturer's Name: Hewlett-Packard Co.

Manufacturer's Address: Santa Rosa Systems Division

> 1400 Fountaingrove Parkway Santa Rosa, CA 95403-1799

USA

declares that the product

Product Name: EMI Receiver

HP 8542E, HP 85420E, HP 85422E, **Model Number:**

HP 8546A, HP 85460A, HP 85462A

Product Options: This declaration covers all options of the

above product.

conforms to the following Product specifications:

Safety: IEC 1010-1:1990+A1 / EN 61010-1:1993

CAN/CSA-C22.2 No. 1010.1-92

EMC: CISPR 11:1990/EN 55011:1991 Group 1, Class B

IEC 801-2:1984/EN 50082-1:1992 4 kV CD, 8 kV AD IEC 801-3:1984/EN 50082-1:1992 3 V/m, 27-500 MHz

IEC 801-4:1988/EN 50082-1:1992 0.5 kV Sig. Lines, 1 kV Power Lines

Supplementary Information:

The product herewith complies with the requirements of the Low Voltage Directive 73/23/EEC and the EMC Directive 89/336/EEC.

Santa Rosa, California, USA 11 Sept 1995

Dixon Browder/Quality Manager

European Contact: Your local Hewlett-Packard Sales and Service Office or Hewlett-Packard GmbH, Department ZQ/Standards Europe, Herrenberger Strasse 130, D-71034 Böblinger, Germany (FAX +49-7031-14-3143)

Notice for Germany: Noise Declaration

LpA < 70 dBam Arbeitsplatz (operator position) normaler Betrieb (normal position) nach DIN 45635 T. 19 (per ISO 7779)

Key Menus


This chapter contains the key menu diagrams for the EMI receiver and receiver RF section. Each diagram is arranged alphabetically according to the front-panel key name.

User Defined Keys

The top two softkeys are user-definable keys that remain the same regardless of the key menu selected. The default softkey definitions are:


- Last Hrd Key Menu toggles between the lowest level accessed on the last two hardkey menus selected. (toggles between the lowest level menu accessed by the last two hardkeys previously selected?)
- SPAN duplicates the SPAN softkey located under the (SPAN) key.

To define a user-definable softkey, use the DEFINE USER KEY on the third page of the SETUP menus. For more information on the user-defined keys, refer to Chapter 12, "User-Definable Softkeys," of the *EMI Receiver Series User's Guide*.

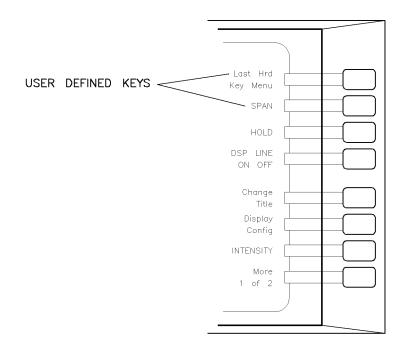

userdef

AMPLITUDE

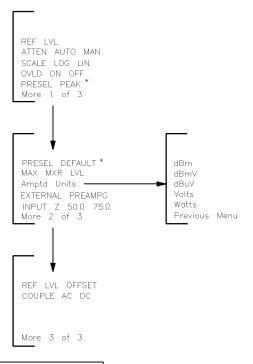

* Available only for an HP 8546A or an HP 85462A.

amplitud


AUTO COUPLE

AUTO ALL
IF BW AUTO MAN
AVG BW AUTO MAN
ATTEN AUTO MAN
SWP TIME AUTO MAN
CF STEP AUTO MAN

autocoup

AUTO RANGE

autorang




* Available only for a standalone receiver RF section.

auxctrl

AVERAGE

average



bw


CALIBRATE SET TIME CAL ALL Cal At Time CORRECT ON OFF AUTO CAL ON OFF EXIT LAST CAL CAL FETCH CAL STORE Previous Menu More 1 of 3CAL 85462 ① STOR PWR ON UNITS * CAL INPUT 1 + EXECUTE TITLE Flatness Data CAL INPUT 2 ‡ Last Cal ** CAL TIMEBASE CAL MXR 2 SET ATTN ERROR EDIT FLATNESS EDIT PA FLATNESS STORE FLATNESS * II More 2 of 3 INIT FLT * IDNUM * INPUT 1 INPUT 1 PREAMP INPUT 2 INPUT 2 PREAMP EXIT More Service Cal DISPLAY CAL DATA Display Sys Data § = STP GAIN ZERO Service Diag DEFAULT CAL DATA CAL TRK GEN CAL YTF 2 IF GAINS More 3 of 3 More 1 2v REF DETECTOR MAIN SPAN FINE TUNE DAC GND REF DETECTOR MAIN COIL DR SWEEP RAMP SWEEP TIME DAC X FINE TUNE DAC +10V REF DETECTOR COARSE TUNE DAC YTF SPAN 2 FM COIL DRIVE -10V REF DETECTOR FM SPAN DROOP More 2 More 3 More 4 * For service use only. † Softkey changes to CAL FREQ for a standalone receiver RF section. ‡ Softkey changes to CAL AMP for a standalone receiver RF section. YTF TUNE COARSE² YTF TUNE FINE² YTF DRIVER² FREQ DIAG QP DET ON OFF \$LOCK ON OFF QP GAIN ON OFF § Softkey changes to DACS for a standalone receiver RF section. QPD RST ON OFF FRQ DISC NORM OFF MIXER BIAS DAC@ PRESEL DAC@ More 6 FM GAIN FM OFFSET QPD OFFSET II Only appears when EDIT FLATNESS or EDIT PA FLATNESS are pressed. DACS More 7 More 5 -** Available only for an EMI receiver. ① Softkey changes to CAL 85422 for an HP 85422E. 2 Available only for an HP 8546A or an HP 85462A.



calcheck

calbrate

CONFIG

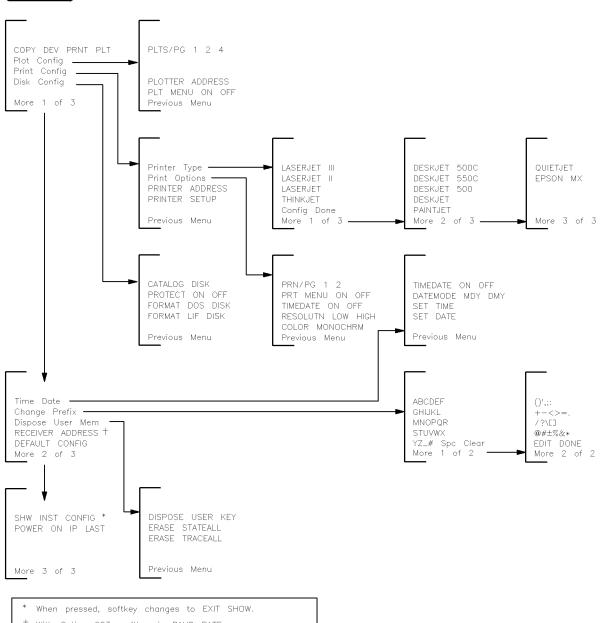

† With Option 023, softkey is BAUD RATE.

COPY

copymenu

DEMOD

ON/OFF


SELECT

DEMOD ON OFF DEMOD AM FM SPEAKER ON OFF SQUELCH FM GAIN DWELL TIME

demod


DISPLAY hardkey-in RECEIVER mode only

The DISPLAY hardkey has different Limit Lines softkey menus between the receiver and signal analysis modes.

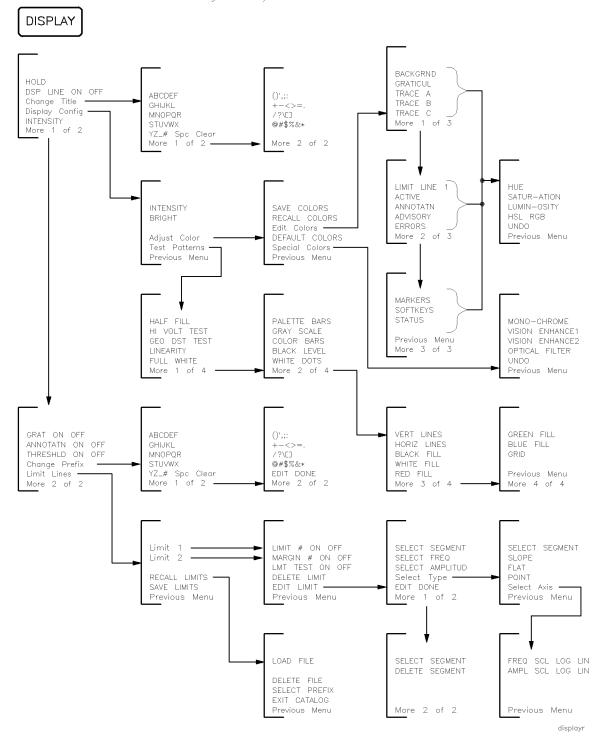

DISPLAY hardkey-in SIGNAL ANALYSIS mode only

The DISPLAY hardkey has different Limit Lines softkey menus between the receiver and signal analysis modes.

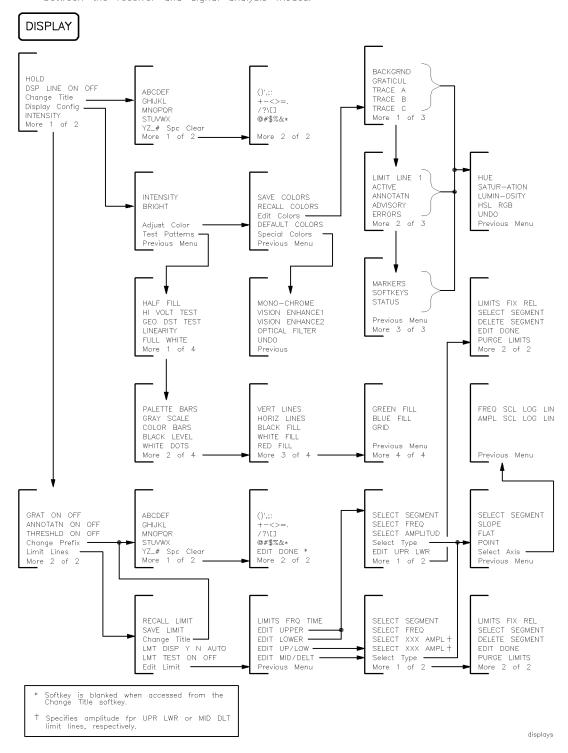

FREQUENCY

```
CENTER FREQ
START FREQ
STOP FREQ
CF STEP AUTO MAN
SWEEP LOG LIN
More 1 of 2

FREQ OFFSET
Band Lock†

LOGF SPD STD FAST
INPT LCK ON OFF*
More 2 of 2

CENTER FREQ
O-2.9 Gz BAND 0†
2.75-6.5 BAND 1†

BND LOCK ON OFF†
Previous Menu
```

* Available only for an EMI receiver. + Available only for an HP 8546A or an HP 85462A.

frequenc

INPUT

INPUT 1 9k-50M*
INPUT 2 20M-2.9G*
INPUT 2 1-6.5G †
INPUT 2 BYPASS *
VIEW CAL ON OFF


* Available only for an EMI receiver. + Available only for an HP 8546A.

inputm

LINEARITY CHECK

linechk


MEAS/ USER



* Available only when LIN is selected for the SWEEP LOG LIN softkey.

measuser





mkr


MKR->

```
MARKER -> CF
MARKER -> REF LVL
MARKER -> CF STEP
MARKER -> CF STEP
MARKER -> CF STEP
MARKER -> MARKER -> PK-PK
Peak Menu
More 1 of 2


MARKER -> PK-PK
PEAK
SEARCH
```

mkrright

MARKER FUNCTION



mkrfctn




- * Only occurs when switching from signal analysis mode to receiver mode. † When EMI RECEIVER mode is active, pressing the MODE hardkey twice displays the softkey PRESET RECEIVER.
- $\mbox{$\frac{1}{2}$}$ When SIGNAL ANALYSIS mode is active, pressing the MODE hardkey twice displays the softkey PRESET SPECTRUM.

mode

COPY SCREEN OUTPUT REPORT Define Report Define List EDIT ANNOTATN ON OFF LIST ON OFF SETTINGS ON OFF Previous Menu SHOW DET PK QP AV SHOW Δ 1 PK QP AV SHOW Δ 2 PK QP AV SHOW COR ON OFF SHOW MRK ON OFF SHOW MRK ON OFF SHOW MRK ON OFF Previous Menu CLEAR ANNOTATN

output




EXIT EDIT

peaksrch

PREAMP


preamp




preset



quasipk

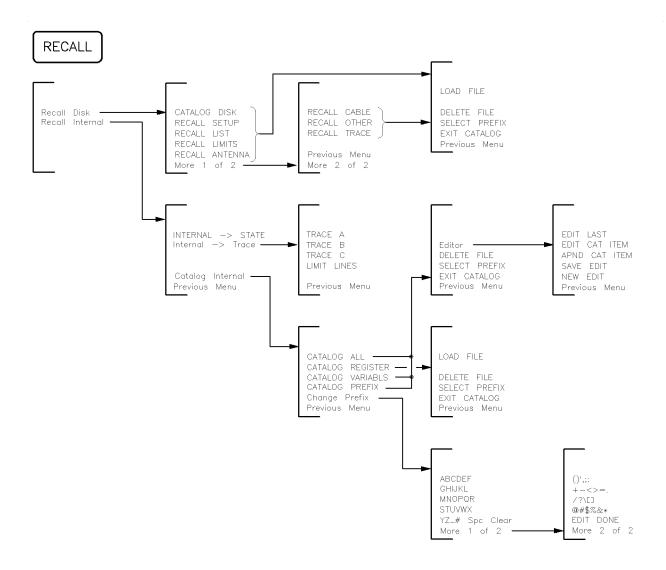


recall

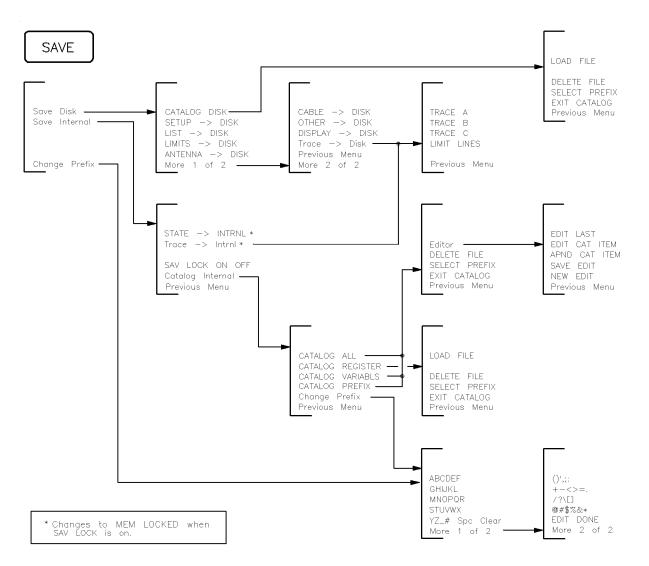


savemenu

SETUP hardkey-in RECEIVER mode only

The SETUP hardkey has different Limit Lines softkey menus between the receiver and signal analysis modes.

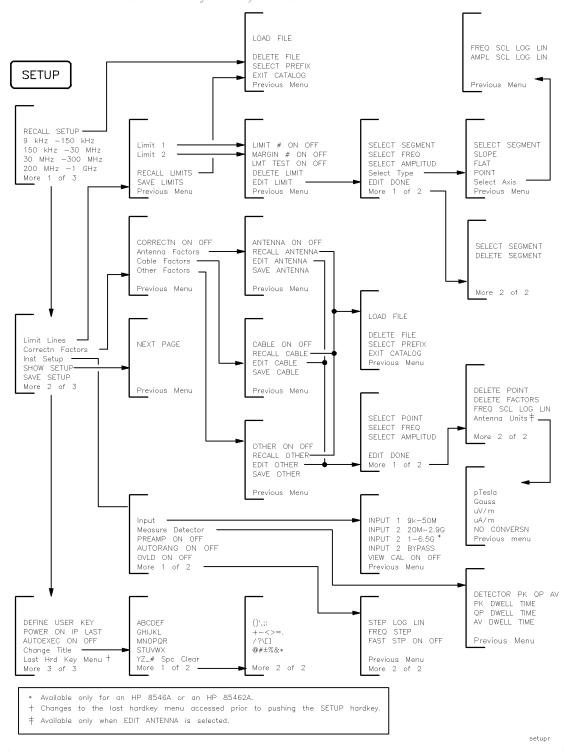

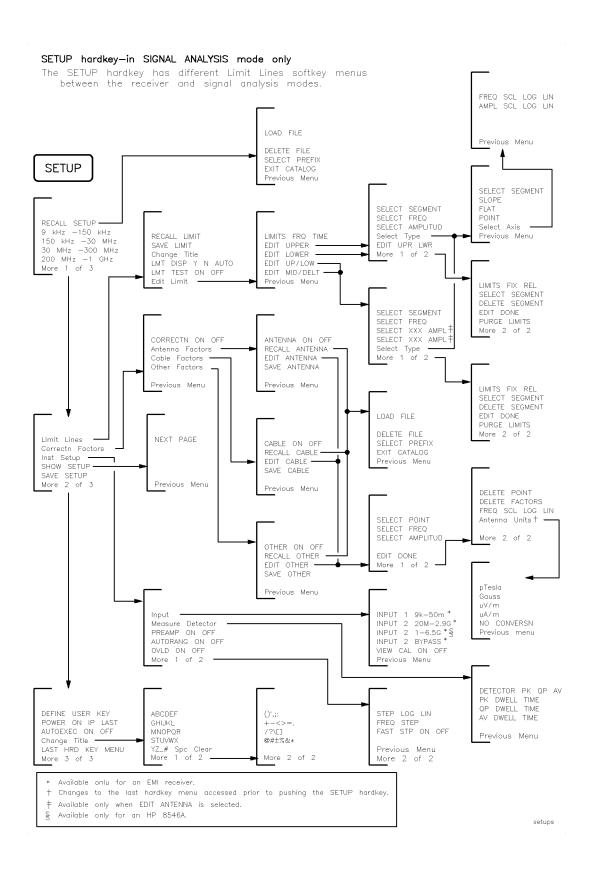

SINGLE

single

SPAN

SPAN ZOOM FULL SPAN ZERO SPAN LAST SPAN

spanmenu

SWEEP

SWP TIME AUTO MAN SWEEP CONT SGL


SWEEP LOG LIN LOGF SPD STD FAST*

 * Available only when LOG is selected for the SWEEP LOG LIN softkey.

sweep


TEST hardkey-in RECEIVER mode only

TEST

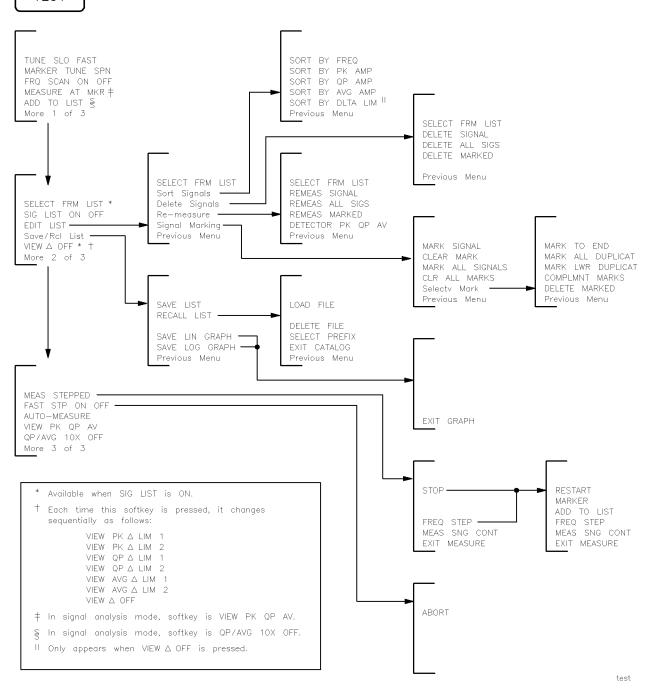

(with Trace A selected)

TRACE



* With Trace C selected, softkey changes to MIN HOLD C.

tracem

TRACK GEN

SCR PWR ON OFF
TRACKING PEAK
MAN TRK ADJUST
PWR SWP ON OFF*
SRC ATN MAN AUTO
More 1 of 2

SCR PWR STP SIZE
SCR PWR OFFSET
ALC INT EXT
SWP CPLG SR RECV
More 2 of 2

* Available only when LIN is selected for the SWEEP LOG LIN softkey.

trackgen

TRIG

SWEEP CONT SGL FREE RUN VIDEO LINE EXTERNAL

trig

WINDOWS

CTRL

ZONE CENTER
ZONE SPAN
ZONE PK RIGHT
ZONE PK LEFT
PEAK EXCURSN
WINDOWS OFF

NEXT

(If windows are on, activates alternate windows.)

ZOOM

(Toggles between split—screen and full—size display, if windows are on.)

windows

Key Dictionary Reference

This chapter describes functions and controls of the instrument. The front-panel keys and softkey functions are listed alphabetically followed by a complete and detailed description.

Brief descriptions for service functions have also been included in this chapter. However, for more detailed descriptions and information about the use of each function, refer to the respective service guide for your instrument. A listing of all service calibration and service diagnostic functions has been provided in the following "Service Functions" section.

All softkeys and their relationship to the front-panel keys are shown in Chapter 3.

Service Functions

Two types of functions are available for service use only:

- Service calibration functions.
- Service diagnostic functions.

These service functions are designed for service use only. However, brief descriptions for each function are provided in this chapter.

Service Calibration Functions

Service Cal accesses the following service calibration softkeys:

CAL MXR
CAL TIMEBASE
EDIT FLATNESS
EDIT PA FLATNESS
EXECUTE TITLE
EXIT
Flatness Data
IDNUM
INIT FLT
SET ATTN ERROR
STOR PWR ON UNITS
STORE FLATNESS

Service Diagnostic Functions

Service Diag accesses the following diagnostic softkeys:

 ϕ LOCK ON OFF +10V REF DETECTOR -10V REF DETECTOR 2v REF DETECTOR COARSE TUNE DAC DACS DISPLAY CAL DATA Display Sys Data DROOP FINE TUNE DAC FM COIL DRIVE FM GAIN FM OFFSET FM SPAN FREQ DIAG FRQ DISC NORM OFF GND REF DETECTOR IF GAINS MAIN COIL DR MAIN SPAN MIXER BIAS DAC

PRESEL DAC QP DET ON OFF QP GAIN ON OFF QPD OFFSET QPD RST ON OFF STP GAIN ZERO SWEEP RAMP SWEEP TIME DAC X FINE TUNE DAC YTF DRIVER YTF SPAN YTF TUNE COARSE YTF TUNE FINE

Key Functions

% AM

Softkey that determines the percent of amplitude modulation of the largest displayed signal and its two sidebands. The sidebands are assumed to be entirely from amplitude modulation. If there are differences in the sideband amplitude, the larger value is used. The measurement runs continuously, reexecuting at the end of each sweep.

All three signal must be displayed. The frequency spacing of the sideband signals must be the same within the span accuracy of the measurement. All of the signals must be greater than the peak excursion above the threshold. The amplitude scale may be either linear or logarithmic.

Key Path


Related Programming Command

none

ϕ LOCK ON OFF

Softkey that turns off phase locking on the instrument. The counter is turned off so frequency correction is no longer done at the start of each sweep. Turning the phase locking off increases measurement speed, but it decreases frequency accuracy. This is a service diagnostic function and is for service use.

Key Path




Related Programming Command

none

 $\mu A/m$

Softkey that selects $\mu A/m$ as the transducer conversion units for the antenna amplitude-correction factors.

Key Path




Related Programming Command

XUNITS

 μ V/m

Softkey that selects $\mu V/m$ as the transducer conversion units for the antenna amplitude-correction factors.

Key Path



Related Programming Command

XUNITS

0-2.9 Gz BAND 0

For an HP 8546A/HP 85462A only.

Softkey that locks onto harmonic Band 0. Once 0-2.9Gz BAND 0 has been pressed only frequencies and spans that fall within this frequency band may be entered. The span is reduced automatically to accommodate a center frequency specified near the end of the band range.

If a start frequency is entered that is outside of the current band boundaries, it will be set to the nearest band edge instead. If a start frequency that is greater than the current stop frequency is entered, the (possibly modified) start frequency is used for both the start and the stop frequency; therefore, the span will be set to zero. If the start and stop frequencies specify too large a span, they will be modified.

If a stop frequency is entered that is outside of the current band boundaries, it will be set to the nearest band edge instead. If a stop frequency that is less than the current start frequency is entered, the (possibly modified) stop frequency will be used for both the start and stop frequency; therefore, the span will be set to zero.

The span will be modified if necessary to get the center frequency specified without crossing the band edges. The span will be limited as necessary to keep the start and stop frequencies within the band

edges without changing the center frequency. The maximum span allowed is 2.904 GHz.

Note

For this softkey function to work properly, the corresponding (INPUT) must first be selected.

Key Path

More Band 0-2.9 Gz (FREQUENCY) 1 of 2 Lock BAND 0

Related Programming Command

HNLOCK

2v REF DETECTOR

Softkey that displays the output of the 2 V reference produced on the A16 processor/video assembly as a horizontal line at the top graticule. This is a service diagnostic function and is for service use only.

Key Path

More More Service 2v REF

(CALIBRATE) 1 of 3 2 of 3 Diag More 1 DETECTOR

Related Programming Command

none

2.75-6.5 BAND 1

For an HP 8546A/HP 85462A only.

Softkey that locks onto harmonic Band 1. Once 2.75-6.5 BAND 1 has been pressed only frequencies and spans that fall within this frequency band may be entered. The span is reduced automatically to accommodate a center frequency specified near the end of the band range.

If a start frequency is entered that is outside of the current band boundaries, it will be set to the nearest band edge instead. If a start frequency that is greater than the current stop frequency is entered, the (possibly modified) start frequency is used for both the start and the stop frequency; therefore, the span will be set to zero. If the start and stop frequencies specify too large a span, they will be modified.

If a stop frequency is entered that is outside of the current band boundaries, it will be set to the nearest band edge instead. If a stop frequency that is less than the current start frequency is entered, the (possibly modified) stop frequency will be used for both the start and stop frequency; therefore, the span will be set to zero.

The span will be modified if necessary to get the center frequency specified without crossing the band edges. The span will be limited as necessary to keep the start and stop frequencies within the band edges without changing the center frequency. The maximum span allowed is 3.6 GHz.

Note

For this softkey function to work properly, the corresponding (INPUT) must first be selected.

Key Path

	More	Band	2.75-6.5
(FREQUENCY)	1 of 2	Lock	BAND 1

Related Programming Command

HNLOCK

3 dB POINTS

Softkey that initiates an automatic 3 dB bandwidth measurement on the highest peak displayed on screen.

Key Path

3 dB POINTS (MEAS/USER)

Related Programming Command

none

3rd ORD MEAS

Softkey that initiates an automatic frequency and amplitude measurement on a third-order product. At least one of the fundamental tones and the third-order product must be displayed on the screen.

Key Path

More 3rd ORD 1 of 2 MEAS (MEAS/USER)

Related Programming Command

none

6 dB POINTS

Softkey that initiates an automatic 6 dB bandwidth measurement on the highest peak displayed on the screen.

Key Path

6 dB (MEAS/USER) POINTS

Related Programming Command

none

9 kHz -150 kHz

Softkey that presets the instrument to the predefined settings:

9 kHzStart frequency: $150~\mathrm{kHz}$ Stop frequency: I.F. bandwidth: $200~\mathrm{Hz}$ Reference level: $70~\mathrm{dB}\mu\mathrm{V}$ Attenuation: 10 dB

Key Path

9 kHz -(SETUP) 150 kHz

Related Programming Command

none

9 kHz EMI BW

Softkey that allows a 6 dB intermediate frequency bandwidth of 9 kHz. This bandwidth is useful when performing electromagnetic interference (EMI) measurements.

Key Path

9 kHz EMI BW (BW)


Related Programming Command

none

+10V REF DETECTOR

Softkey that displays the output of the +10 V reference from the analog interface circuit board as a horizontal line at the top of the graticule. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

none

-10V REF DETECTOR

Softkey that displays the output of the -10 V reference from the analog circuit board as a horizontal line at the bottom graticule. This is a service diagnostic function and is for service use only.

Key Path

(CALIBRATE)	More 1 of 3	No.e	Service Diag	More 1	 More 3
-10V REF DETECTOR					

Related Programming Command

none

30 MHz -300 MHz

Softkey that presets the receiver to the predefined settings:

Start frequency: $30~\mathrm{MHz}$ 300 MHz Stop frequency: I.F. bandwidth: $120~\mathrm{kHz}$ $80 \text{ dB}\mu\text{V}$ Reference level: 10 dB Attenuation:

Key Path

30 MHz -(SETUP) 300 MHz

Related Programming Command

none

99% PWR BW

Softkey that initiates an automatic measurement of the 99% power bandwidth of the largest signal displayed on the screen.

Key Path

99% PWR More (MEAS/USER) 1 of 2

Related Programming Command

none

120 kHz EMI BW

Softkey that allows a 6 dB intermeditate frequency bandwidth of 120 kHz. This bandwidth is useful when performing electromagnetic interference (EMI) measurements.

Key Path

120 kHz (BW)EMI BW

Related Programming Command

none

150 kHz -30 MHz

Softkey that presets the instrument to the predefined settings:

 $150~\mathrm{kHz}$ Start frequency: Stop frequency: 30 MHzI.F. bandwidth: 9 kHzReference level: $75 \text{ dB}\mu\text{V}$ Attenuation: 10 dB

Key Path

150 kHz -(SETUP) 30 MHz

Related Programming Command

none

200 Hz EMI BW

Softkey that allows a 6 dB intermeditate frequency bandwidth of 200 Hz. This bandwidth is useful when performing electromagnetic interference (EMI) measurements.

Key Path

200 Hz (BW) EMI BW

Related Programming Command

none

200 MHz 1 GHz

Softkey that presets the instrument to the predefined settings:

200 MHz Start frequency: 1 GHz Stop frequency: I.F. bandwidth: $120~\mathrm{kHz}$ Reference level: $80 \text{ dB}\mu\text{V}$ 10 dB Attenuation:

Key Path

200 MHz -(SETUP) 1 GHz

Related Programming Command

none

A<-->B

Softkey that exchanges the contents of the trace A register with the trace B register and puts trace A in view mode.

Key Path

More 1 of 3 A<-->B

Related Programming Command

AXB

 $A-B \rightarrow A$ ON OFF

Softkey that when ON is underlined, subtracts the data in trace B from the measured data in trace A. A minus sign (-) appears between the trace A status and the trace B status in the screen annotation while the function is active.

To deactivate this function, press $A - B \rightarrow A$ ON OFF so that OFF is underlined. The A-B -> A and B-DL -> B functions are math functions. Unlike operations on dBm units, math functions operate on measurement units. Measurement units are used to format trace data for data within the graticule limits. The displayed amplitude of each element falls on one of 8000 vertical points with the value of 8000 being equal to the reference level. For log scale data, each point is equal to 0.01 dB. The peak of a signal equal to -10 dBm, or one division below the reference level, is equal to 7000 measurement units (8000 - 1000 = 7000). In linear mode, each point has a resolution of [reference level in volts/8000].

For example, if trace A contains amplitude values of -10 dBm and trace B contains amplitude values of -40 dBm, the result of the $A - B \rightarrow A$ function would be -10.004 dBm if dBm units were used. Since measurement units are used for the $A - B \rightarrow A$ function, the result of $A - B \rightarrow A$ is -50 dBm (-10 dBm = 7000 measurement units, -40 dBm = 4000 measurement units; the result is 3000 measurement units, which is equal to -50 dBm).

Key Path

	MATA	

Related Programming Command

AMB

A -> C

Softkey that copies trace A into trace C.

Key Path

More More 2 of 3 A -> C TRACE 1 of 3

Related Programming Command

none

ABCDEF

Softkey that accesses the softkey menu for selecting screen title characters A through F.

Key Access

(CONFIG), (DISPLAY), (RECALL), (SAVE), or (SETUP)

Related Programming Command

none

ABORT

Softkey that exits the Auto Measure function.

Key Path

AUTO-More More (TEST) 1 of 3 2 of 3 MEASURE ABORT

Related Programming Command

none

ACTIVE

Softkey that displays the current settings of the display subsystem's color editor.

Key Path

Display Adjust Edit More (DISPLAY) Config Color Colors 1 of 3 ACTIVE

Related Programming Command

SETC

ADD TO LIST

Softkey that adds a signal to the internal signal list. The signal added is either for the last MEASURE AT MKR result or the measurement at the marker position after a stepped measurement.

Key Path

ADD TO (TEST) LIST More More MEAS ADD TO 1 of 3 2 of 3 LIST (TEST) STEPPED STOP More More MEAS ADD TO FREQ 1 of 3 2 of 3 STEPPED STEP LIST (TEST)

Related Programming Command

SIGADD

Adjust Color

Softkey that accesses a menu used to adjust the color editor display subsystem.

Key Path

Display Adjust (DISPLAY) Config Color

Related Programming Command

SETC

ADVISORY

Softkey that activates the advisory portion of the display screen for color editing.

Key Path

Display Adjust Edit More (DISPLAY) Config Color Colors 1 of 3 ADVISORY

Related Programming Command

SETC

ALC INT EXT

Softkey that activates internal (INT) leveling or external (EXT) leveling.

Key Path

More ALC (TRACK GEN) 1 of 2 INT EXT

Related Programming Command

SRCALC

AMPL SCL LOG LIN

Softkey that specifies whether the limit line is derived from a logarithmic or linear amplitude axis. Underline LIN to set the amplitude axis to linear or LOG to set the amplitude axis to logarithmic.

Key Path

Receiver mode

	More	Limit		EDIT	Select	Select
(DISPLAY	<u>)</u> 1 of 2	Lines	*	LIMIT	Туре	Axis
AMPL	SCL					
LOG I	IN.					
	1/f	Limit		EDTT	Select	Select
	More	LJ LILL L				
(SETUP)	more 1 of 3	Lines	*	LIMIT	Туре	Axis
(SETUP) AMPL	1 of 3		*			

Signal analysis mode

	More	Limit	Edit		Select	Select
DISPLAY) 1 of 2	Lines	Limit	†	Туре	Axis
AMPL S	SCL					
LOG L	IN					
	More	Limit	Edit		Select	Select
(SETUP)	1 of 3	Lines	Limit .	†	Туре	Axis
AMPL S	SCL					
LOG L	IN					

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Related Programming Command

LIMIAMPSCL

AMPLITUDE)

Hardkey that activates the reference level function and accesses the amplitude menu. The softkeys accessed when you press (AMPLITUDE) change reference level, input attenuation, vertical scale, mixer level, amplitude units, input impedance, and amplitude offset. Pressing (AMPLITUDE) accesses the preselector peaking and preselector default functions also.

Related Programming Command

none

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

Amptd Units

Softkey that accesses a menu to select the desired amplitude units. Amplitude units can be selected by pressing, dBm, dBmV, dBuV, Volts, or Watts.

Key Path

Amptd More 1 of 3 Units (AMPLITUDE)

Related Programming Command

AUNITS

ANNOTATN

Softkey that activates the annotation portion of the display screen for color editing.

Key Path

Display Adjust Edit More Color Colors DISPLAY Config 1 of 3 ANNOTATN

Related Programming Command

SETC

ANNOTATN ON OFF

As accessed from (DISPLAY).

Softkey that turns the screen annotation on or off. However, softkey annotation will remain on the screen. The screen annotation may not be required for prints or plots, or during remote operation. Refer to the HOLD softkey description regarding softkey annotation.

As accessed from (OUTPUT).

Softkey that turns on or off the generation of a tabular listing of the screen annotation. The listing will be sent to the printer when OUTPUT REPORT is executed.

Key Path

(DISPLAY)	More 1 of 2	ANNOTATN ON OFF
(OUTPUT)	Define Report	

Related Programming Command

ANNOT

ANTENNA -> DISK

Softkey that saves the current antenna amplitude-correction factors to a floppy disk. To save antenna data press, ANTENNA -> DISK. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The antenna data has now been saved to a disk.

Key Path

Save ANTENNA Disk -> DISK SAVE

Related Programming Command

none

Antenna Factors

Softkey that accesses a menu to turn on, recall, edit, or save antenna amplitude-correction factors. Antenna factors are conversion factors relating field strength to measured voltage.

Key Path

More Correctn Antenna (SETUP) 1 of 3 Factors Factors

Related Programming Command

AMPCOR

ANTENNA ON OFF

Softkey that turns on or off antenna amplitude-correction factors.

Key Path

More Correctn Antenna ANTENNA (SETUP) 1 of 3 Factors Factors ON OFF

Related Programming Command

AMPCOR

Antenna Units

Softkey that accesses a menu of the transducer conversion units for the antenna-correction factors. This specifies the units of the physical attribute to which an antenna actually responds and which will be indicated on the display for reference level, display line level, threshold level, and marker readouts.

Key Path

(SETUP)	More	Correctn	Antenna	EDIT	More
	1 of 3	Factors	Factors	ANTENNA	1 of 2
Anten Units	ina				

Related Programming Command

XUNITS

APND CAT ITEM

Softkey that starts the DLP editor function and allows the highlighted item from the catalog of instrument memory to be added to the end of the item that is currently in the DLP editor memory of the instrument. If the item to be added will not fit in the available memory space, it will not be appended.

Key Path

Recall Catalog RECALL Internal Internal	APND l * Editor CAT ITEM
Save Catalog (SAVE) Internal Internal	APND * Editor CAT ITEM

^{*} Any of the following can be used to complete the key path: CATALOG ALL, CATALOG PREFIX, or CATALOG VARIABLS.

Related Programming Command

none

ATTEN AUTO MAN

Softkey that sets the input attenuation in 10 dB increments. The instrument input attenuator, which is normally coupled (linked) to the reference level control, reduces the power level of the input signal at the input mixer. The attenuator is recoupled when AUTO is underlined.

Key Path

ATTEN (AMPLITUDE) AUTO MAN

ATTEN (AUTO COUPLE) AUTO MAN

CAUTION

- To prevent damage to the input mixer, the power level at the input mixer must not exceed +30 dBm. To prevent signal compression, power at the input to the input mixer must be kept below -10dBm.
- To protect the mixer from possible damage, 0 dB RF attenuation (no input power reduction to the mixer) can be selected only from the data keys.

Related Programming Command

ΑT

AUTO ALL

Softkey that couples the following functions:

- intermeditate frequency bandwidth
- average video bandwidth
- attenuation
- sweep time
- center-frequency step
- average video bandwidth
- average-video-bandwidth to intermediate-frequency-bandwidth ratio.

Key Path

AUTO (AUTO COUPLE) ALL

Related Programming Command

AUTO

AUTO CAL ON OFF

Softkey that turns the automatic calibration feature of the EMI receiver on or off.

Key Path

AUTO CAL Cal At Time ON OFF (CALIBRATE)

Related Programming Command

AUTOCAL

AUTO COUPLE

Hardkey that accesses the softkey menu of functions that can be coupled. (Coupled functions are functions that are linked: if one function is changed, the other function is changed.) The functions that can be auto-coupled are listed below:

- Intermediate frequency bandwidth couples to span.
- Average video bandwidth couples to intermeditate frequency bandwidth when the instrument has a average-video-bandwidth to intermediate-frequency-bandwidth ratio of 0.3.
- Sweep time couples to span, intermeditate frequency bandwidth, and average video bandwidth.
- RF attenuation couples to reference level.
- Center frequency step size couples to 10% of span.

During normal operation, the sweep time, intermeditate frequency bandwidth, and average video bandwidth are coupled to yield optimum performance. If any of these functions becomes uncoupled (that is, is manually set), a "#" will appear next to the screen annotation representing the function on the screen.

If one or more function(s) is manually set so that the amplitude or frequency becomes uncalibrated, MEAS UNCAL appears on the top right-side of the graticule.

Recouple a single function by pressing the function label (to activate the function), and pressing the function again so that AUTO is underlined.

Pressing (AUTO COUPLE), AUTO ALL couples all coupled functions listed.

Related Programming Command

none

AUTO-MEASURE

Softkey that finds all signals on the display and makes an EMI measurement using specified detectors. Each signal is tuned to in sequence, the span is reduced in steps to zero span, and a maximum of three detectors are measured. The detectors used are selected using DETECTOR PK QP AV. Measurement time is determined by selecting AV DWELL TIME, PK DWELL TIME, or QP DWELL TIME. After each signal is measured it is added to the signal list. If a limit margin is on, only signals above the margin are measured and added to the list.

Key Path

	 MEACHDE

Related Programming Command

MEASALLSIGS

AUTO RANGE

Hardkey that turns the current state of the auto-range function on or off. When on, the auto-range function automatically adjusts RF attenuation or reference level (IF step-gain) in response to either an IF or RF overload condition detected during the previous sweep.

Auto range requires overload detection capability. The RF filter section must be present (and not in a bypass state) for RF overload detection. IF overload detection does not require the RF filter section.

When on, auto range automatically enables overload detection. When disabled, auto range does not disable over load detection.

Related Programming Command

ARNG

AUTOEXEC ON OFF

Softkey that enables and disables the automatic loading and execution of the file named "AUTOEXEC.DLP" from a DOS disk ("dAUTOEXEC" from a LIF disk). When enabled, the instrument, upon a power-up sequence, will search the disk for an "AUTOEXEC" file and if found will load and execute it.

Key Path

	More	HOTE	AUTOEXEC
(SETUP)	1 of 3	2 of 3	ON OFF

Related Programming Command

none

AUTORANG ON OFF

Softkey that turns the current state of the auto-range function on or off. When on, the auto-range function automatically adjusts RF attenuation or reference level (IF step-gain) in response to either an IF or RF overload condition detected during the previous sweep,

Auto range requires overload detection capability. The RF filter section must be present (and not in a bypass state) for RF overload detection. IF overload detection does not require the RF filter section.

When on, auto range automatically enables overload detection. When disabled, auto range does not disable over load detection.

Key Path

		AUTORANG
More		
		ON OFF
	SATIIN	

Related Programming Command

none

Aux Conn Control

Available only for a standalone receiver RF section.

Softkey that accesses the menu used to control the auxiliary outputs and input. The auxiliary outputs are controlled by pressing CNTL A O 1, CNTL B O 1, CNTL C O 1, and CNTL D O 1. The status of the auxiliary input (control line I), can be displayed on the screen with DISPLAY CNTL I.

Key Path

Aux Conn (AUX CTRL) Control

Related Programming Command

none

AUX CTRL

Hardkey that accesses the softkey menu used for control of the auxiliary interface connector.

Related Programming Command

none

AV DWELL TTME.

Softkey that sets the measurement time when the average detector is measured. This key is used in conjunction with MEASURE AT MKR, RE-measure, AUTO-MEASURE, and MEAS STEPPED.

Key Path

Inst Measure AV DWELL More (SETUP) 1 of 3 Setup Detector TIME

Related Programming Command

MEASTIMEAVG

AVERAGE

Hardkey that toggles the average detector on and off. When on, the instrument is placed in linear amplitude detection, the average detector is turned on, and the system settings are optimized to accurately measure average amplitude.

Related Programming Command

none

AVG BW AUTO MAN

Softkey that specifies the averaging bandwidth, which is a post-detection, low-pass filter. The intermediate frequency bandwidth, average video bandwidth, and sweep time are normally coupled to the span. Selecting MAN uncouples the average video bandwidth from intermediate frequency bandwidth (it does nothing to the sweeptime and span coupling). Selecting AUTO recouples average video bandwidth to the intermediate frequency bandwidth.

Frequency values other than the values in the 1, 3, 10 sequence are rounded to the nearest permissible value.

Key Path

AVG BW (AUTO COUPLE) AUTO MAN

AVG BW (BW) AUTO MAN

Related Programming Command

AVBW, VB

AV/IF BW RATIO

Softkey that determines the automatic setting of average video bandwidth by multiplying the parameter by the intermeditate frequency bandwidth. Ratio values other than the values in the 1, 3, 10 sequence are rounded to the nearest permissible value.

Key Path

More AV/IF (BW) 1 of 2 BW RATIO

Related Programming Command

VBR

B -> C

Softkey that moves trace B into trace C, then stops updating trace C by placing it in the view mode. Trace B is unchanged by BTC. Trace B must contain a complete sweep of measurement information.

Key Path

More More

(TRACE) 1 of 3 2 of 3 $B \rightarrow C$

Related Programming Command

BTC

B <--> C

Softkey that exchanges the contents of trace B with trace C and puts trace B in view mode.

Key Path

More More

(TRACE) 1 of 3 2 of 3 B <--> C

Related Programming Command

BXC

B-DL -> B

Softkey that subtracts the display line from trace B and places the result in trace B. The B-DL-> B function is a math operation. See the A-B-> A ON OFF softkey description for information about math operations.

Key Path

More More (TRACE) 1 of 3 2 of 3 B-DL -> B

Related Programming Command

BML

BACKGRND

Softkey that activates the background of the display screen for color editing.

Key Path

Display Adjust Edit

(DISPLAY) Config Color Colors BACKGRND

Related Programming Command

SETC

Band Lock

For an HP 8546A/HP 85462A only.

Softkey that accesses the harmonic band menu and the band lock function. Selecting a harmonic band causes the instrument to lock onto the specified harmonic band and automatically select the settings shown in Table 4-1.

Table 4-1. Center Frequency and Span Settings for Harmonic Bands

Softkey	Center Frequency	Span	Description
0-2.9 Gz BAND 0	1.45 GHz	$2.865~\mathrm{GHz}$	Low-pass filtered, first harmonic mixing.
2.75-6.5 BAND 1	$4.638~\mathrm{GHz}$	$3.6~\mathrm{GHz}$	Preselected, first harmonic mixing.

BND LOCK ON OFF locks the instrument onto a selected frequency band (local oscillator harmonic number). When only one frequency band is being swept the corresponding softkey will be underlined, even if band lock is off.

Note

For this softkey function to work properly, the corresponding (INPUT) must first be selected.

Key Path

	More	Band
(EDECHENCY)	1 04 0	
(FREQUENCY)	1 01 2	LOCK

Related Programming Command

HNLOCK

BAUD RATE

Softkey that specifies the baud rate of an instrument with the RS-232 interface installed.

Note

The RS-232 interface is only available with Option 023.

Key Path

	More	BAUD
(CONFIG)	1 of 3	RATE

Related Programming Command

BAUDRATE

BLACK FILL

Softkey that replaces the standard display screen with a black box. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

Related Programming Command

none

BLACK LEVEL

Softkey that replaces the standard display screen with four color bars overlayed on a black background. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

	Display	lest	More	BLACK
(DISPLAY)	Config	Patterns	1 of 4	TEVET
(DIST LAT)	UUIII I S			

Related Programming Command

none

BLANK A

Softkey that stores the amplitude data for trace A and removes it from the screen. The trace A register will not be updated as the instrument sweeps.

Key Path

(TRACE) BLANK A

Related Programming Command

BLANK

BLANK B

Softkey that stores the amplitude data for trace B and removes it from the screen. The trace B register will not be updated as the instrument sweeps.

Key Path

(TRACE) BLANK B

Related Programming Command

BLANK

BLANK C

Softkey that stores the amplitude data for trace C and removes it from the screen. The trace C register will not be updated as the instrument sweeps.

Key Path

(TRACE) BLANK C

Related Programming Command

BLANK

BLUE

Softkey that changes the intensity of the blue portion of the primary light source output for the display annotation, traces, graticule, and so on.

Key Path

Related Programming Command

none

BLUE FILL

Softkey that replaces the standard display screen with a blue box. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

	Test.		
	Patterns		

Related Programming Command

none

BND LOCK ON OFF

For an HP 8546A/HP 85462A only.

Softkey that when ON is underlined, the instrument is locked to the lowest frequency band (local oscillator harmonic number) containing the correct center frequency. Start and stop frequencies will be changed if necessary. Executing a band lock limits the tuning range to the selected harmonic number. Selecting the softkeys for either band 0 or band 1 turns on the band lock function automatically.

If the start frequency is well within a lower band, turning band lock off will result in a multiband sweep. If a specific band had been selected prior to changing to a multiband sweep, the softkey label of the selected band will no longer be underlined indicating that it is not selected. Sweep of a single band is indicated if the softkey label of the selected band is underlined.

Note

Before changing the frequency range to another harmonic band, unlock the band by pressing BND LOCK ON OFF so that OFF is underlined.

Key Path

	More	Band	BND LOCK
(FREQUENCY)	1 of 2	Lock	ON OFF

Related Programming Command

HNLOCK, HNUNLK

BRIGHT

Softkey that changes the brightness or luminance of the display. The brightness level is shown on the top left-hand side of the screen. Use the knob or step keys to adjust the brightness level.

Key Path

	Display	
(DISPLAY)	Config	BRIGHT
<u></u>		

Related Programming Command

 $(\overline{\mathsf{BW}})$

Hardkey that activates the intermediate frequency bandwidth function and accesses the softkeys that control the bandwidth functions: 120 kHz EMI BW, 9 kHz EMI BW, 200 Hz EMI BW, IF BW AUTO MAN, AVG BW AUTO MAN, AV/IF BW RATIO, and VID AVG ON OFF. (Also see the IF BW AUTO MAN softkey description.)

Related Programming Command

none

CABLE -> DISK Softkey that saves cable amplitude-correction data to a floppy disk. To save cable data press, CABLE -> DISK. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The cable data has now been saved to a disk.

Key Path

			MADTE
			$C\Delta RIF$
	Save	More	
			_N DTCV
(CA\/E1			
		1 01 2	

Related Programming Command

none

Cable Factors

Softkey that accesses a menu to turn on, recall, edit, or save cable amplitude-correction factors. Cable factors are conversion factors used to correct for cable insertion loss.

Key Path

More	Correctn	
	Factors	Factors

Related Programming Command

AMPCOR

CABLE ON OFF Softkey that turns on or off cable amplitude correction factors.

Key Path

Correctn Cable CABLE More (SETUP) 1 of 3 Factors Factors ON OFF

Related Programming Command

AMPCOR

CAL 85422

Softkey that performs a calibration only on the HP 85422E receiver RF section when configured as an HP 8542E EMI receiver.

Key Path

More CAL (CALIBRATE) 1 of 3 85422

Related Programming Command

CAL

CAL 85462 Softkey that performs a calibration only on the HP 85462A receiver RF section when configured as an HP 8546A EMI receiver.

Key Path

More CAL (CALIBRATE) 1 of 3 85462

Related Programming Command

CAL

CAL ALL

Softkey that initiates frequency and amplitude correction routines.

Key Path

(CALIBRATE) CAL ALL

Related Programming Command

CAL AMP

Available only for a standalone receiver RF section.

Softkey that initiates the amplitude correction routine.

Key Path

CAL More

(CALIBRATE) 1 of 3 AMP

Related Programming Command

CAL

Cal At Time

Softkey that accesses a menu to set the time of an automatic calibration.

Key Path

Cal

(CALIBRATE) At Time

Related Programming Command

CAL

(CAL CHECK)

Hardkey that checks the calibration of the 300 MHz input.

Related Programming Command

CALCHECK

CAL FETCH

Softkey that retrieves stored self-calibration correction factors from the last calibration saved using CAL STORE.

Key Path

CAL

(CALIBRATE) FETCH

Related Programming Command

CAL FREQ Available only for a standalone receiver RF section.

Softkey that initiates the frequency correction routine.

Key Path

More CAL (CALIBRATE) 1 of 3 FREQ

Related Programming Command

CAL

(CALIBRATE)

Hardkey that accesses menus used for the self-calibration, service-diagnostics, and service-calibration functions.

Related Programming Command

none

CAL INPUT 1

Softkey that calibrates the conducted measurement band of the instrument, 9 kHz to 50 MHz, for amplitude flatness through each filter.

Key Path

More CAL 1 of 3 INPUT 1 (CALIBRATE)

Related Programming Command

CAL

CAL INPUT 2

Softkey that calibrates the radiated measurement band of the instrument, 20 MHz to 2.9 GHz, for amplitude flatness through each filter.

Key Path

More CAL 1 of 3 INPUT 2 (CALIBRATE)

Related Programming Command

CAL MXR

For an HP 8546A/HP 85462A only.

Softkey that adjusts the bias-current DAC setting for the optimum displayed-signal amplitude using the 300 MHz CAL OUT signal. This is a service calibration function and is for service use only.

Key Path

	More	More	Service	
CALIBRATE	1 1 Af 3	2 of 3	627	CAL MXR
CALIDITATE				OUT HUIF

Related Programming Command

none

CAL STORE

Softkey that stores the correction factors from the last calibration. The stored correction factors are automatically retrieved when the instrument is turned on. If correction factors are not stored, they will be retained only until the instrument is turned off. See the description for the CAL FETCH softkey.

Key Path

CAL (CALIBRATE) STORE

Related Programming Command

CAL

CAL TIMEBASE

Softkey that changes the setting of the 10 MHz reference (standard timebase) DAC that is located on the A25 counter lock assembly. This is a service calibration function and is for service use only,

Key Path

(CALLED ATE)	More	More	Service	CAL
(CALIBRATE)	1 01 3	2 01 3	Cal	IIMERASE

Related Programming Command

CAL TRK GEN

Softkey that performs absolute amplitude, and vernier self-calibration routines. The instrument should be amplitude calibrated by pressing CAL AMP prior to using the CAL TRK GEN function. Connect the tracking generator output to the instrument input before pressing CAL TRK GEN.

Key Path

	MOTA	

Related Programming Command

CAL

CAL YTF

For an HP 8546A/HP 85462A only.

Softkey that generates the best slope and offset adjustment to calibrate the YIG-tuned filter (YTF) for each harmonic band. The self-calibration routine, CAL ALL should be performed before running the CAL YTF routine.

Key Path

	More	More	CAT.
CALIBRATE	1 Af 3	2 of 3	VTF
CALIBITATE		2 01 0	

Related Programming Command

CAL

CATALOG ALL

Softkey that catalogs all the programs and variables stored in instrument memory. Press CATALOG REGISTER to catalog states, traces, and limit-line tables, saved in instrument memory.

Key Path

Recall Interna	Catalog CA Internal AL	TALOG L
Save (SAVE) Internal	Catalog CATA Internal ALL	LOG

Related Programming Command


CATALOG DISK

Softkey that catalogs the floppy disk. Existing data on the floppy disk will be displayed if the disk has been formatted. If the disk has not been formatted the following message will be displayed:

Cannot read disk drive. Please verify drive door is closed and that disk is formatted and error free.

When cataloging a floppy disk, you can specify the type of information to be cataloged, in either LIF or DOS format.

Key Path



Related Programming Command

CAT

Catalog Internal

Softkey that accesses a menu of cataloging functions for instrument memory: CATALOG ALL, CATALOG REGISTER,

CATALOG VARIABLS, and CATALOG PREFIX. Each catalog function displays catalog information. The catalog contains information about the data stored in internal memory. See Figure 4-1 and Table 4-2.

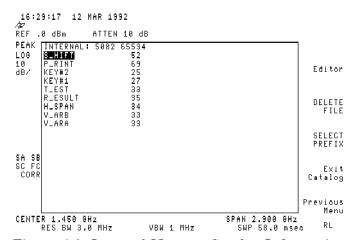


Figure 4-1. Internal Memory Catalog Information

Table 4-2. Internal Memory Catalog Information*

Callout Number	Description of Items in Figure 4-1		
1	Name of the catalog source.		
2	Bytes of internal memory used.		
3	Total bytes of internal memory available.		
4	Bytes used by item.		
5	Name of item.		
* This table is not applicable when using CATALOG REGISTER.			

Unlike saving to the floppy disk, data is saved as an item in internal memory.

Use the step keys or knob to view different sections of the directory, then press LOAD FILE to select a file. The selected file is highlighted in inverse video.

Each of the catalog softkey functions access the menu that has the DELETE FILE function. Use DELETE FILE to delete the item from internal memory.

Pressing CATALOG REGISTER allows access to the LOAD FILE function. Use LOAD FILE to load a state or trace from internal memory. Do not use LOAD FILE to load limit-line table and amplitude-correction factor items.

Also see the CATALOG ALL and CATALOG VARIABLS softkey descriptions.

Key Path

RECALL	Rec Int		Catalog Internal
(SAVE)	Save Inte	rnal I	Catalog Internal

Related Programming Command

CAT

CATALOG PREFIX

Softkey that catalogs all of the saved data, that has the specified prefix, that is either on the floppy disk or in internal memory. The entire prefix does not have to be specified. For example, if you want to catalog all the files beginning with the prefix S, specify S as the prefix, using the change prefix function, then select CATALOG PREFIX. Prefixed items can be saved in internal memory by either loading in from a floppy disk or using remote programming commands to define them.

Key Path

(RECALL)	Recall Internal	Catalog Internal	PREFIX
(SAVE)	Internal	Catalog Internal	CATALOG

Related Programming Command

none

CATALOG REGISTER

Softkey that displays the status of state and trace registers in internal memory. States 1 through 8 are displayed with the center frequency (denoted by CF) and span (denoted by SP). The status of trace registers 0 to the maximum number of traces is displayed also. If a trace, limit-line table, or amplitude correction factors have been saved in the trace register, the screen title (denoted by "TR:") is displayed, otherwise UNUSED is displayed. If the screen title length allows, or if no title is saved with the trace, the time and date are displayed. To load the contents of the state or trace register into internal memory, use the knob or step keys to select the register and press LOAD FILE. The DELETE FILE key can be used to delete a state or trace register from internal memory.

Note

Do not use LOAD FILE to load the contents of a trace register containing limit-line tables or amplitude-correction factors.

Key Path

RECAL	Recall Interna	Catalo	g CATALOG al REGISTER
(SAVE)	Save	Catalog	CATALUG
	Internal	Internal	REGISTER

Related Programming Commands

CATALOG VARIABLS

Softkey that catalogs all of the variables saved in internal memory. Variables can be saved in internal memory by loading in a downloadable program from the floppy disk or defining a function using remote programming commands (VARDEF or TRDEF).

Note

Variables beginning with an underscore are used by the instrument firmware. Modifying these is not recommended and may give unexpected results.

Key Path

(RECALL)	Recall Interna	1 Inte	log rnal	CATALOG VARIABLS
(SAVE)	lnternal	Catalo,	g (al V	CATALOG VARIABLS

Related Programming Command

none

CENTER FREQ

Softkey that activates the center-frequency function to allow the selection of frequency that will be at the center of the screen.

Key Path

CENTER FREQUENCY FREQ

Related Programming Command

CF

CF STEP AUTO MAN

Softkey that changes the step size for the center frequency function. Once a step size has been selected and the center frequency function is activated, the step keys change center frequency by the step-size value. The step size function is useful for finding harmonics and sidebands beyond the current frequency span of the instrument. When auto-coupled, the center frequency step size is set to one graticule (10 percent of the span).

Key Path

CF STEP (AUTO COUPLE) AUTO MAN CF STEP (FREQUENCY) AUTO MAN

Change Prefix

Softkey that allows you to enter a prefix that can be used for saving and recalling data to and from the floppy disk, and for cataloging by the prefix. The prefix can be from one to seven characters long. The longer the prefix, the shorter the register number must be. The total length of the prefix and register number cannot exceed eight characters. The prefix can be any character; however, the underscore should not be the first character of the prefix. Pressing Change Prefix accesses a menu containing the letters of the alphabet, the underscore symbol (_), the number symbol (#), a space, and the clear function. To select a character, press the softkey that displays the group of characters that contains the desired character. The softkey menu changes to allow you to select an individual character. If you make a mistake, press (BK SP) to space back over the incorrect character. Additional characters are available by pressing More 1 of 2. Numbers may be selected with the data keys.

A prefix can be cleared with the clear function. Press (CONFIG) or (DISPLAY), Change Prefix, YZ_# Spc Clear, Clear to clear the current prefix. The current prefix is blanked by pressing DEFAULT CONFIG.

Key Path

	More	Change	
(CONFIG)	1 of 3	Prefix	
	More	Change	
(DISPLAY)	1 of 2	Prefix	
	Recall	Catalog	Change
(RECALL)	Internal	Interna	l Prefix
(Change		
(SAVE) I	refix		
Ç.	Save	Catalog	Change
(SAVE)	Internal	Internal	Prefix

Related Programming Command

PREFX

Change Title

Softkey that allows you to write a 53-character screen title across the top of the screen. The marker readout may interfere with the last 26 characters. The markers can be turned off by pressing (MKR),


More 1 of 2, and MARKER ALL OFF. Pressing Change Title accesses the softkey menus that contain the available characters and symbols. A programming command can be entered in the screen title area. It can then be executed from the front panel by pressing EXECUTE TITLE.

The screen title will remain on the screen until either Change Title is pressed again or a trace is recalled that was saved with a screen title. A screen title can also be cleared by using the clear function. Press (DISPLAY), Change Title, YZ_# Spc Clear, Clear to clear the current screen title.

Pressing Change Title accesses a menu containing the letters of the alphabet, the underscore symbol (_), the number symbol (#), a space, and the Clear softkey. To select a character, press the softkey that displays the group of characters that contains the desired character. The softkey menu changes to allow you to select an individual character. If you make a mistake, press (BK SP) to space back over the incorrect character. Additional characters are available by pressing More 1 of 2. Numbers may be selected by using the data keys.

Key Path

Receiver Mode



Change

DISPLAY	J 1 01 2	: Lines	Title
(SETUP)	More	Limit	Change
	1 of 3	Lines	Title

Related Programming Command

TITLE

CLEAR ANNOTATN

Softkey that clears the annotation editor of all text.

Key Path

EDIT CLEAR (OUTPUT) ANNOTATN ANNOTATN

Related Programming Command

none

CLEAR MARK

Softkey that clears the mark from a signal on the signal list.

Key Path

M	COTT		CITAD
nore	LULL	STRIIGT	ULLAR
(TFCT) 1 of 2		Monteleine	MADV
LIESIJ I OI O		narking	MARA

Related Programming Command

SIGUNMARK

CLEAR WRITE A

Softkey that erases any data previously stored in trace A and continuously displays any signals during the sweep of the instrument. This function is activated at power on and by pressing (PRESET).

Changing the trace mode of trace C to clear write or minimum hold can change the trace mode of trace A. If trace A is in clear-write mode or maximum-hold mode when trace C is changed to clear write or minimum hold, the trace mode of trace A is changed to store blank. The following table shows the trace mode of trace A before and after changing trace C to clear-write or minimum-hold trace mode.

Trace Mode of Trace A Before	Trace Mode of Trace A After
Clear write	Store blank
Maximum hold	Store blank
View	View

Changing the trace mode of trace A to clear write or maximum hold can change the trace mode of trace C. If trace C is in clear-write mode when trace A is changed to clear write or minimum hold, the trace mode of trace C is changed to minimum hold.

Trace Mode of Trace C Before	Trace Mode of Trace C After
Clear write	Minimum hold
Minimum hold	Minimum hold
View	View

Key Path

CLEAR WRITE A TRACE

Related Programming Command

CLRW

CLEAR WRITE B

Softkey that erases any data previously stored in trace B and continuously displays any signals detected during the sweep of the instrument. This function is activated at power on and by pressing (PRESET).

Changing the trace mode of trace C to clear write or minimum hold can change the trace mode of trace B. If trace B is in clear-write mode or maximum-hold mode when trace C is changed to clear write or minimum hold, the trace mode of trace B is changed to store blank.

The following table shows the trace mode of trace B before and after changing trace C to clear-write or minimum-hold trace mode.

Trace Mode of Trace B Before	Trace Mode of Trace B After
Clear write	Store blank
Maximum hold	Store blank
View	View

Changing the trace mode of trace B to clear write or maximum hold can change the trace mode of trace C. If trace C is in clear-write mode when trace B is changed to clear write or minimum hold, the trace mode of trace C is changed to minimum hold.

Trace Mode of Trace C Before	Trace Mode of Trace C After
Clear write	Minimum hold
Minimum hold	Minimum hold
View	View

Key Path

CLEAR (TRACE) WRITE B

Related Programming Command

CLRW

CLEAR WRITE C

Softkey that erases any data previously stored in trace C and continuously displays any signals detected during the sweep of the instrument. This function is activated at power on and by pressing (PRESET).

Changing the trace mode of trace C to clear write or minimum hold can change the trace mode of trace A and trace B. If trace A or trace B is in clear-write mode or maximum-hold mode when trace C is changed to clear write or minimum hold, the trace mode of trace A or trace B is changed to store blank. The following table shows the trace mode of trace A or trace B before and after changing trace C to clear-write or minimum-hold trace mode.

Trace Mode of Trace A or B Before	Trace Mode of Trace A or B After
Clear write	Store blank
Maximum hold	Store blank
View	View

If you want to use trace A or trace B in the clear-write or maximum-hold mode and do not want trace C to blank it, use minimum-hold or view-trace mode for trace C.

Key Path

CLEAR WRITE C TRACE

Related Programming Command

CLRW

CLR ALL MARKS

Softkey that clears all signals in the signal list.

Key Path

More Signal EDIT CLR ALL (TEST) 1 of 3 LIST Marking MARKS

Related Programming Command

SIGUNMARK

CNTL A

Available only for a standalone receiver RF section.

Softkey that makes the auxiliary-interface control line A output high or low (TTL). This line can be used to control any external drive that takes a TTL input.

Key Path

	Aux Conn	CNTL A
(AUX CTRL)) Control	0 1

Related Programming Command

CNTLA

CNTL B 0 1

Available only for a standalone receiver RF section..

Softkey that makes the auxiliary-interface control line B output high or low (TTL). This line can be used to control any external drive that takes a TTL input.

Key Path

	Aux Conn	CNTL B
(AUX CTRL)	Control	0 1

Related Programming Command

CNTLB

CNTL C 0 1

Available only for a standalone receiver RF section.

Softkey that makes the auxiliary-interface control line C output high or low (TTL). This line can be used to control any external drive that takes a TTL input.

Key Path

	Aux Conn	CNTL C
(AUX CTRL)	Control	0 1

Related Programming Command

CNTLC

CNTL D 0

Available only for a standalone receiver RF section.

Softkey that makes the auxiliary-interface control line D output high or low (TTL). This line can be used to control any external drive that takes a TTL input.

Key Path

Aux Conn CNTL D (AUX CTRL) Control 0 1

Related Programming Command

CNTLD

COARSE TUNE DAC

Softkey that displays the analog output of the YTO coarse-tune DAC located on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path

More More Service (CALIBRATE) 1 of 3 2 of 3 Diag More 1 More 2 COARSE TUNE DAC

Related Programming Command

none

COLOR BARS

Softkey that replaces the standard display screen with a color bars. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

More COLOR Display Test (DISPLAY) Config Patterns 1 of 4 BARS

Related Programming Command

COLOR MONOCHRM

Softkey that specifies either a color print when COLOR is underlined or a black and white print when MONOCHRM is underlined. This function is used when a color printer is connected to the output port.

Key Path

		COLOR
		MONOCHRM
(CONFIG)	Ontions	

Related Programming Command

none

COMPLMNT MARKS

Softkey that complements all marked signals in the signal list. For example, if all the even numbered signals in the signal list are marked, pressing COMPLMNT MARKS, with mark all odd numbered signals instead.

Key Path

		COMDIMNT
	~ ~ ~ · · · · · · · · · · · · · · · · ·	
	Marking	MADIC

Related Programming Command

SIGMARK



Hardkey that accesses the menu used for printer and plotter configurations, time and date display functions, changing the current prefix, floppy disk configuration functions, disposing of user-defined variables and programs from internal memory, changing the instrument address or the baud rate, displaying the installed options on screen, and changing the format of the MONITOR output. Pressing (CONFIG) after the instrument has been placed in the remote mode places the instrument in the local mode and enables front-panel control. During remote operation, an R appears in the lower-right corner of the screen indicating remote mode. Pressing (CONFIG) removes the R annotation from the lower-right corner.

Related Programming Command

CONFIG DONE

Softkey that sets the specified printer type then exits the menu.

Key Path

		Printer	1,011119
LCONFIG 1	CONTIC	37 A A	Ilana

Related Programming Command

none



Hardkey that initiates an output of the screen data, without an external controller, to a previously specified graphics printer or plotter. Refer to the programmer's guide for detailed information about printing and plotting.

The printer or plotter must have already been selected using CONFIG and either Plot Config (for a plotter) or Print Config (for a printer). To obtain a print, press (CONFIG), COPY DEV PRNT PLT (so that PRNT is underlined), then Print Config.

If the instrument is connected to an HP PaintJet printer and you want a color printout, press Printer Type, More 1 of 3,

PAINTJET PRINTER. If the instrument is connected to an HP PaintJet printer and you want a black and white printout, press Print Options then, COLOR MONOCHRM so that MONOCHRM is underlined. The paintjet printer's mode switches must be set correctly for use with the instrument. The switch settings are indicated in Table 4-3. If the switch settings are changed, the printer must be turned off and then back on after they are changed. More Thinkjet printer information can be found in the programmer's guide.

Table 4-3. Setting of Thinkjet Printer Mode Switches

Switch Number	Setting	Comments
1	down	Printer performs a carriage return only.
2	down	Printer performs a line feed only.
3	up	Sets the printer to skip paper perforations
4	down	Sets the printer for a paper length of 11 inches.
5	down	Sets the printer to HP MODE.
6	up	
7	down	Sets the printer to USASCII.
8	down	

If you want the softkey labels to be printed with the instrument display printout when using (COPY), press PRT MENU ON OFF so that ON is underlined.

Press (COPY) and the process will begin. The screen remains frozen (no further sweeps taken) until the data transfer to the printer is complete. The instrument works with many Hewlett-Packard printers.

The plotting process is similar to the printing process. On the spectrum analyzer, press (CONFIG), Plot Config. For Option 023, use BAUD RATE to change the baud rate of the instrument, if necessary.

With PLTS/PG 1 2 4, you can choose a full-page, half-page, or quarter-page plot. Press PLTS/PG 1 2 4 to underline the number of plots per page desired. If two or four plots per page are chosen, a softkey function is displayed that allows you to select the location of the plotter output on the paper. If two plots per page are selected, PLT []LOC _ _ is displayed. If four plots per page are selected, PLT []_LOC _ _ is displayed. Press the softkey until the rectangular marker is in the desired section of the softkey label. The upper and lower sections of the softkey label graphically represent the position of the page where the plotter output will be located.

Note

The HP 7470A plotter does not support two plots per page output, you can select one or four plots per page, but not two plots per page.

For a multipen plotter, the pens of the plotter draw the different components of the screen as follows:

Pen Number	Description
1	Draws trace A, the active function, markers, display line, and softkeys.
2	Draws limit 2, status and error messages.
3	Draws limit 1 and the annotation.
4	Draws the graticule.
5	Draws trace C.
6	Draws trace B.

To plot, press Previous Menu, COPY DEV PRNT PLT (PLT should be underlined), and (COPY).

Printing is usually faster than plotting, but plotting provides higher resolution output. The instrument works with plotters such as the HP 7440A.

Figure 4-2 shows the rear view of a typical printer and instrument configuration.

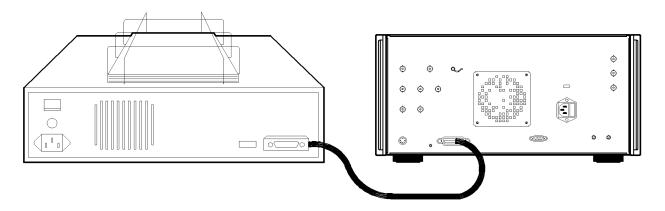


Figure 4-2. Connecting a Printer to the Instrument

Note

Printing and plotting require an optional interface. Generally, instruments with an HP-IB interface set the plotter address to 5 and the printer address to 1. Instruments with an RS-232 interface must have the baud rate set to match the baud rate of the printer or plotter being used. The programmer's guide that comes with the optional interfaces details the different interfaces. Refer to the programmers guide for more information about printing and plotting.

Related Programming Commands

PLOT, PRINT

COPY DEV PRNT PLT

Softkey that changes between a printer and plotter. For example, if you have been printing and want to do a plot, press COPY DEV PRNT PLT to underline PLT before pressing (COPY).

Key Path

COPY DEV (CONFIG) PRNT PLT

Related Programming Command

COPY SCREEN

Softkey that sends a copy of the current display to the printer specified by Printer Type.

Key Path

COPY (OUTPUT) SCREEN

Related Programming Command

none

CORRECT ON OFF

Softkey that controls use of some correction factors. When ON is underlined, correction factors are used and CORR appears on the left hand-side of the display. When OFF is underlined, correction factors are not used. Turning the correction factors off degrades amplitude accuracy.

Note

Correction factors must be on for the instrument to meet its specified performance.

Key Path

CORRECT ON OFF (CALIBRATE)

Related Programming Command

CAL

Correctn Factors

Softkey that accesses a menu of correction factors used to create, edit, and view antenna, cable, and other amplitude-correction factors.

Key Path

More Correctn (SETUP) 1 of 3 Factors

Related Programming Command

AMPCOR

CORRECTN ON OFF

Softkey that turns antenna, cable, or other amplitude-correction factors on or off.

Key Path

	More	Correctn	CORRECTN
	More	COLLECTI	COUVECTN
(
(SETUP)	1013	Factors	ON OFF

Related Programming Command

CORREK

COUPLE AC DC

Softkey that specifies alternating-current (AC) or direct-current (DC) coupling at the instrument input. Selecting ac coupling blocks any dc voltage at the instrument input; however, the ac coupling also decreases the frequency range of the instrument. The input coupling is set to ac by an instrument preset.

Amplitude specifications apply only when coupling is set to DC.

CAUTION

Do not use dc coupling if there is any dc voltage at the instrument input.

Key Path

	WATE A	
		AATA
AMPLITUDE		

Related Programming Command

COUPLE

CNT RES AUTO MAN

Softkey that sets the resolution of the marker frequency counter. When AUTO is underlined, the marker counter resolution is set to 6 kHz. When MAN is underlined, the marker counter resolution can be set manually from 1 Hz to 100 kHz.

Key Path

	More	CNT RES
(MARKER FUNCTION)	1 of 2	AUTO MAN

Related Programming Command

MKFCR

CTRL

Hardkey that activates the windows display mode and accesses the menu of window zone functions. The windows display function splits the screen into two separate displays. Only one of these displays is active at a time. The currently active window will have a highlighted line around the graticule. The WINDOWS (NEXT) key will switch the active display between the upper and lower windows. The instrument state of the active window can be changed without affecting the state of the inactive window. The complete annotation is not displayed for each window because of space limitations.

When the windows display mode is first turned on, the top window will contain an inactive copy of the previous full display. The lower window will be active and will display a subset of the frequency span of the upper window. The displayed span, or zone, of the lower window will be indicated on the upper window by two vertical lines called zone markers. The zone can be moved and changed using the zone keys which are accessed by pressing the WINDOWS (CTRL) key. Changing the span or center frequency of the lower window will change the corresponding zone markers on the upper window.

Most functions can be used from within the windows display mode. Some functions, like editing limit lines and showing the options, require a full-sized display. They will temporarily exit the windows display format. When the function is finished the instrument will return to a windows display. Other functions will permanently exit the windows display and it will be necessary to restart the windows display mode by pressing WINDOWS (CTRL). See Table 4-4.

Limit lines can be displayed and tested within the windows display mode. Viewing and testing must be turned on independently in each window. The current limit lines will be common to both windows.

(SAVE) and (RECALL) do not save the windows display mode. If the windows display mode is being used, the save state function saves the state of the currently active window. The recall state function recalls the stored state into the currently active window. See the STATE -> INTRNL softkey description for more information about saving the display.

Table 4-4. Functions Which Exit The Windows Display Format

Function	Description
Calibration Functions	self-calibration routines
Dispose User Memory	deletes user's items from instrument memory
Instrument Preset	returns instrument to preset state

Related Programming Command


WINON

DACS

Available only for a standalone receiver RF section.

Softkey that changes the DAC numbers of the span, DAC YTO coarse-tune, DAC YTO fine-tune, and YTO FM tune DAC located on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

none

DATEMODE MDY DMY

Softkey that changes the display of the date from a month-day-year format to a day-month-year format. It is set to a month-day-year format by pressing DEFAULT CONFIG.

Key Path

	More	Time	DATEMODE
(CONFIG)	1 of 3	date	MDY DMY

Related Programming Command

DATEMODE

dBm

Softkey that changes the amplitude units to dBm for the current setting (logarithmic or linear).

Key Path


	More	Amptd	
(AMPLITUDE)	1 of 3	Units	dBm

Related Programming Command

dBmV

Softkey that changes the amplitude units to dBmV for the current setting (logarithmic or linear).

Key Path



Related Programming Command

none

$dB_{\mu}V$

Softkey that changes the amplitude units to $dB\mu V$ for the current setting (logarithmic or linear).

Key Path

	More	Amptd	
		77 · .	15 77
(AMPLITUDE)	1 01 3	Units	dBµ∀

Related Programming Command

none

DEFAULT CAL DATA

Softkey that accesses the factory-default correction factors. A special pass code is required for use. If the message Self cal needed appears when DEFAULT CAL DATA is pressed, the CAL FREQ and CAL AMP routines need to be run. CAL ALL must be run to ensure specifications. (If the maximum frequency of interest is higher than 3 GHz, the CAL YTF routine must also be run.) The calibration results must then be saved by pressing CAL STORE.

Key Path

V ~~~	Mara	

Related Programming Command

DEFAULT COLORS

Softkey that sets all the display screen attributes to the factory-defined colors. To change the color elements, refer to Edit Colors.

Key Path

	Display	Admist	DEFAILT
(DISPLAY)	Config	Color	COLORS

Related Programming Command

SETC

DEFAULT CONFIG

Softkey that resets the instrument configuration to the state it was in when it was originally shipped from the factory then performs an instrument preset. See Table 4-5 for the default user-configuration values set by pressing DEFAULT CONFIG.

Table 4-5. Default Configuration Values

Configuration	Default Value
Analyzer address ¹	18
Copy device	printer
CRT position (Horizontal and Vertical)	10, 48
Printer address (Option 023)	1
Plotter address (Option 023)	5
Baud rate (Option 023)	1200
External preamp	0 dB
Save lock (internal states or traces)	Off
Printer	black and white printer
Print menu	on
Plots per page	1
Time/date display	on
Date mode	month-day-year format
Prefix	(blank)
Analyzer state at power on	instrument preset

¹ Signal analysis mode only.

Key Path

More DEFAULT 1 of 3 CONFIG (CONFIG)

Related Programming Command

Define List

Softkey that accesses a menu that specifies what elements of a table are output to the printer when OUTPUT REPORT is executed. If any of the elements are set to on, they will be included as part of the list portion of the report.

Key Path

Define (OUTPUT) List

Related Programming Command

TBLDEF

Define Report

Softkey that accesses a menu which specifies what elements of a report are output to the printer or the plotter. If any of the elements are set to on, they will be sent to the printer followed by a form feed. Only LOG ON OFF and LIN ON OFF can be used when outputting to a plotter. The report is generated by OUTPUT REPORT.

Key Path

Define (OUTPUT) Report

Related Programming Command

RPTDEF

DEFINE USER KEY

Softkey that sets the instrument in a mode for redefining a user-defined key. It freezes the display and presents instructions in the active function area. The mode is exited by pressing one of the two user-defined keys.

Key Path

More More DEFINE (SETUP) 1 of 3 2 of 3 USER KEY

Related Programming Command

UDKDEFINE, UDKSET

DELETE ALL SIGS

Softkey that deletes all signals from the signal list.

Key Path

	II O I O T O	

Related Programming Command

SIGDEL

DELETE FACTORS

Softkey that deletes all antenna, cable, or other amplitude-correction factors.

Key Path

More (SETUP) 1 of 3	Correctn Factors	Antenna Factors	EDIT ANTENN	More A 1 of 2
SETUP) 1 of 3 DELETE FACTORS	ractors	ractors	ANICAN	A 1 01 2
More	Correctn	Cable	EDIT	More
(SETUP) 1 of 3	Factors	Factors	CABLE	1 of 2
DELETE FACTORS				
More	Correctn	Other	EDIT	More
(SETUP) 1 of 3	Factors	Factors	OTHER	1 of 2
DELETE FACTORS				

Related Programming Command

none

DELETE FILE

Softkey that deletes an item from internal memory or a file from the floppy disk. Use the step keys to view different sections of the directory and use the knob to select the file or item to delete. Pressing DELETE FILE causes a message to appear on the screen: If you are sure, press key again to purge data. Press DELETE FILE again if you want to delete the memory item.

Note

Deleting items beginning with an underscore from the instrument is not recommended and may have unexpected results. Items beginning with an underscore are used by the instrument.

Key Path

(RECALL)	Recall Disk	*	DELETE FILE	
(RECALL)	Recall Disk	More 1 of 2	1	DELETE FILE
(RECALL)	Recall Interna	Catal l Inter	000 00 0 0 00 000 000	DELETE § FILE
	ave CAT isk DIS		LETE LE	
	ave nternal	Catalog Interna		DELETE FILE
	RECALL SETUP	DELETE FILE		
	More 1 of 3	Correctn Factors		DELETE FILE
TEST 1		Save/Rcl List	RECALL LIST	DELETE FILE
Receiver i	$mode\ onlight$	y		
(DISPLAY)	More 1 of 2	Limit Lines	RECALL LIMITS	DELETE FILE

^{*} Any of the following can be used to complete the key path: CATALOG DISK, RECALL SETUP, RECALL LIST, RECALL LIMITS, or RECALL ANTENNA.

Related Programming Command

PURGE

[†] Any of the following can be used to complete the key path: RECALL CABLE, RECALL OTHER, or RECALL TRACE.

 $[\]S$ Any of the following can be used to complete the key path: CATALOG ALL, CATALOG REGISTER, CATALOG VARIABLS, or CATALOG PREFIX.

Any of the following groups of softkeys can be used to complete the key path: Antenna Factors EDIT ANTENNA, or Cable Factors EDIT CABLE, or Other Factors EDIT OTHER.

DELETE LIMIT

Receiver mode only.

Softkey that deletes the selected limit-line table.

Key Path

(DISPLAY	More L 7 1 of 2 L	imit ines '	DELETE * LIMIT
(SETUP)	More Li	mit nes*	DELETE LIMIT

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Related Programming Command

LIMIDEL

DELETE MARKED

Softkey that deletes all marked signals from the signal list. Signals can be marked using MARK ALL SIGNALS, MARK SIGNAL, and Selectv Mark.

Key Path

	ΙΙΩΙΩΤΩ	

Related Programming Command

SIGDEL, SIGMARK

DELETE POINT

Softkey that deletes an amplitude-correction factor that was previously selected by SELECT POINT.

Key Path

	More	Correctn	Antenna	EDIT	More	
(SETUP)	1 of 3	Factors	Factors	ANTENNA	1 of	2
DELET	E					
POINT						
	More	Correctn	Cable	EDIT	More	DELETE
(SETUP)	1 of 3	Factors	Factors	CABLE	1 of 2	POINT
	More	Correctn	Other	EDIT	More	DELETE
(SETUP)	1 of 3	Factors	Factors	OTHER	1 of 2	POINT

Related Programming Command

none

DELETE SEGMENT

Softkey that deletes the limit-line entry for the selected segment number. Use the knob or step keys to highlight the segment number to be deleted, then press DELETE SEGMENT.

Key Path

Receiver Mode

More Limit (DISPLAY) 1 of 2 Lines	*	EDIT More DELETE LIMIT 1 of 2 SEGMENT
More Limit (SETUP) 1 of 3 Lines	*	EDIT More DELETE LIMIT 1 of 2 SEGMENT

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Signal Analysis Mode

(DISPLAY)	1 of 2	Limit Lines	Edit Limit		More * 1 of	2	DELETE SEGMENT
Mo	ore	Limit	Edit	*	More	DE	CLETE
(SETUP) 1	of 3	Lines	Limit .		1 of 2	SE	CGMENT

^{*} Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

Related Programming Command

SEGDEL

DELETE SIGNAL

Softkey that deletes the signal located at the cursor from the signal list.

Key Path

	 Delete	

Related Programming Command

SIGDEL

Delete Signals

Softkey that accesses a menu which deletes one or more signals from the signal list.

Key Path

		TITYTOT	
	More	EDIT	Delete
$(\overline{\pm \epsilon \alpha \pm})$	4 44 9	TTOT	Signals
TIESTI	1 01 3	LIST	Signais

Related Programming Command

SIGDEL

DELTA MEAS

Softkey that accesses the (PEAK SEARCH) menu. See (PEAK SEARCH) for more information.

Key Path

	More	DELTA
(MEAS/USER)	1 of 2	MEAS

Related Programming Command

none

DEMOD AM FM

Softkey that allows selection of amplitude (AM) or frequency (FM) demodulation.

Activating AM detection turns off FM demodulation (if it is on). When the frequency span is greater than 0 Hz, a 30 kHz intermediate frequency bandwidth is used during demodulation, regardless of the screen annotation.

Turning FM demodulation on turns off AM demodulation (if it is on). When the frequency span is greater than 0 Hz, a 100 kHz bandwidth is used during the demodulation, regardless of the screen annotation. When the span is equal to 0 Hz, the displayed bandwidth is used.

Key Path

DEMOD AM FM (SELECT)

Related Programming Command

DEMOD ON OFF

Softkey that turns the AM or FM demodulation on and off. If the instrument is in a nonzero span, a marker is placed at center screen if an onscreen marker is not already present. The marker pause is changed to equal the current dwell time value. Demodulation takes place on any signal that is indicated by the marker position during the marker pause. There is no change to the display during marker pause, but the demodulation signal is present on the AUX VIDEO OUT. Also see the SPEAKER ON OFF softkey description.

Pressing DEMOD ON OFF selects the sample peak detector for AM demodulation, the FMV detector for FM demodulation. If the instrument is in zero span, demodulation is done continuously, with or without an onscreen marker.

Key Path

DEMOD ON OFF (SELECT)

Related Programming Command

DEMOD

DESKJET

Softkey that specifies DeskJet as the printer connected to the output port.

Key Path

Print Printer More (CONFIG) Config Type 1 of 3 DESKJET

Related Programming Command

PRNTTYPE

DESKJET 500

Softkey that specifies DeskJet 500 as the printer connected to the output port.

Key Path

Print More DESKJET Printer 500 (CONFIG) Config Type 1 of 3

Related Programming Command

PRNTTYPE

DESKJET 500C

Softkey that specifies DeskJet 500C as the printer connected to the output port.

Key Path

Related Programming Command

PRNTTYPE

DESKJET 550C

Softkey that specifies DeskJet 550C as the printer connected to the output port.

Key Path

Related Programming Command

PRNTTYPE

DETECTOR PK QP AV

Softkey that turns automatic measuring on or off for the peak, quasi-peak, and average detectors. Underline the desired detector or detectors by pressing DETECTOR PK QP AV.

Key Path

(SETUP) 1 of 3	Setup	Measure Detecto	r PK QP AV
More (TEST) 1 of 3	LISI	Re- measure	DETECTOR PK OP AV

Related Programming Command

AUTOAVG, AUTOQPD

DETECTOR SMP PK

Softkey that selects either positive peak detection or sample detection. When sample detection is selected, SMPL appears in the upper-right corner of the screen. In sample mode, the instantaneous signal value at the present display point is placed in memory. Sample detection is activated automatically for noise level markers, during video averaging, and for FFT measurements.

When positive peak detection is selected, PEAK appears in the upper-right corner of the screen. Positive peak detection obtains the maximum video signal between the last display point and the present display point and stores this value in the trace memory address. Positive peak detection is selected at power on and by pressing (PRESET).

Key Path

	More	DETECTOR
(TRACE)	1 of 3	SMP PK

Related Programming Command

DET

Disk Config

Softkey that accesses a menu to format a 3.5 inch double-sided floppy disk in either LIF or DOS format. Disk Config also accesses the Catalog Disk and Protect functions.

Key Path

Disk (CONFIG) Config

Related Programming Command

none



Hardkey that activates the display line, hold, and threshold functions. It controls the display of the graticule and screen annotation, and provides for title and prefix entries. (DISPLAY) also accesses display configuration capabilities such as color adjustments and test pattern selections.

Related Programming Command

DISPLAY -> DISK

Softkey that saves display images to a floppy disk. To save display images press, DISPLAY -> DISK. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The display image has now been saved to a disk. For a DOS file system, the file is a standard *.BMP file which can be used in many windows applications.

Key Path

	Save	More	DISPLAY
	Jave	TIVE.	DIDIBAL
(SAVE)	Disk	1 of 2	-> DISK

Related Programming Command

none

DISPLAY CAL DATA

Softkey that displays the current correction-factor data generated by the frequency and amplitude self-calibration routines. This is a service diagnostic function and is for service use only.

Key Path

Related Programming Command

none

DISPLAY CNTL I

Available only for a standalone receiver RF section.

Softkey that displays the status of the auxiliary connector input (control line I) onscreen (high = 1 or low = 0, in TTL).

Key Path

	Aux Conn	DISPLAY
(AUX CTRL)	Control	CNTL I

Related Programming Command

CNTLI

Display Config

Softkey that accesses a menu that includes adjust color and test pattern menus along with softkeys to adjust the intensity and brightness of your display.

Key Path

Display (DISPLAY) Config

Related Programming Command

none

Display Sys Data

Softkey that accesses a menu to display system calibration data for input 1. These keys are for service use only.

Key Path

	X (). (()	**************************************		
(
			DIAGNOSTIC	NUS HATA

Related Programming Command

none

DISPOSE USER KEY

Softkey that frees internal memory that was previously allocated for the user-defined keys and reverts the keys to their factory definitions.

Key Path

MOTA	Dispose	
	ligar Mam	

Related Programming Command

DISPOSE

Dispose User Mem

Softkey that accesses a menu to dispose of all the user programs and variables that are in internal memory.

Note

Use DELETE FILE to selectively delete stored programs or variables from internal memory.

Using DISPOSE USER MEM may change the printer or plotter configuration. Pressing DISPOSE USER MEM sets the printer output to print a black and white print by selecting COLOR MONOCHRM, sets the copy device to print when COPY DEV PRNT PLT has PRNT

underlined, and sets the print menu to on when PRT MENU ON OFF has ON underlined. Use Print Config to change any of these functions.

Key Path

More Dispose 1 of 3 User Mem CONFIG

Related Programming Command

DISPOSE

DROOP

Softkey that disables the reset of the peak detector on the A16 processor/video assembly after each analog-to-digital conversion. This is a service diagnostic function and is for service use only.

Key Path

More More Service Diag More 3 (CALIBRATE) 1 of 3 2 of 3 More 1 ... DROOP

Related Programming Command

none

DSP LINE ON OFF

Softkey that activates an adjustable horizontal line that is used as a visual reference line. The line, which can be used for trace arithmetic, has amplitude values that correspond to its vertical position when compared to the reference level. The value of the display line appears in the active function block and on the left side of the screen. The display line can be adjusted using the step keys, knob, or data keys. To deactivate the display line, press DSP LINE ON OFF so that OFF is underlined. (Also see the VIDEO softkey description.)

Key Path

DSP LINE ON OFF (DISPLAY) More DSP LINE (MARKER FUNCTION) 1 of 2 ON OFF More DSP LINE (PEAK SEARCH) 1 of 2 ON OFF

Related Programming Command

DL

DWELL TIME

Softkey that sets the dwell time for marker pause, during which demodulation can take place in nonzero span sweeps. The dwell time can be set from 2 milliseconds to 100 seconds.

Key Path

DWELL TIME (SELECT)

Related Programming Command

none

EDIT ANNOTATN

Softkey that accesses the annotation editor. The annotation editor allows entry of up to 1500 characters of text using an external keyboard. The annotation text can be stored to a disk or printed using OUTPUT REPORT.

Key Path

EDIT OUTPUT) ANNOTATN

Related Programming Command

EDITANNOT

EDIT ANTENNA

Softkey that accesses a menu used to edit antenna amplitudecorrection factors.

Key Path

More Correctn Antenna EDIT (SETUP) 1 of 3 Factors Factors ANTENNA

Related Programming Command

AMPCOR

EDIT CABLE

Softkey that accesses a menu used to edit cable amplitude-correction factors.

Key Path

	More	Correctn	Cable	
(SETUP)	1 of 3	Factors	Factors	CABLE.
()				

Related Programming Command

AMPCOR

EDIT CAT ITEM

Softkey that starts the DLP editor function and loads the highlighted item from the catalog of instrument memory to be displayed and edited. It copies the item into the instruments internal DLP editor memory which is a 2500 byte memory buffer. If an item is edited, the new edited version will not be overwritten in the internal memory until it is processed by the SAVE EDIT softkey.

Key Path

Recall Inte	all Catalog ernal Internal	*	Editor	CAL LIEM
	Catalog nal Internal .	100 to 10	Editor (CAT TTEM

^{*} Any of the following can be used to complete the key path: CATALOG ALL, CATALOG VARIABLS, or CAT PREFIX.

Related Programming Command

none

Edit Colors

Softkey that accesses a menu to change the display screen colors.

Key Path

	Display	Adjust	Edit
(DISPLAY)	Config	Color	Colors

Related Programming Command

SETC

EDIT DONE Softkey that can be accessed through the amplitude-correction, menu the limit-line menu, and the change prefix menu. When accessed from the amplitude-correction menu, the amplitude-correction factors table is erased from the screen and the amplitude-correction menu is restored onscreen. When accessed from the limit-line menu, the limit-line table is erased from the screen and the limit-line menu is restored onscreen. Use EDIT DONE when all the amplitude-correction factors have been entered.

When accessed from the change prefix menu, EDIT DONE erases the prefix from the screen and restores the previous menu. Use EDIT DONE when prefix characters have all been entered.

Key Path

More	Change More	EDIT
CONFIG 1 of 3	Prefix 1 of 2	DONE
More	Change More	EDIT
(DISPLAY) 1 of 2	Prefix 1 of 2	DONE
Recall	Catalog Cha	nge More EDIT
(RECALL) Internal		fix 1 of 2 DONE
Save	Catalog Chang	e More EDIT
(SAVE) Internal	Internal Prefi	
Change M	ore EDIT	
	of 2 DONE	
Receiver Mode		
More	Limit E	EDIT EDIT
(DISPLAY) 1 of 2	4	IMIT DONE
More	Change More	EDIT
(DISPLAY) 1 of 2	Prefix 1 of 2	DONE
More	Limit Ed	it EDIT
		mit DONE
	Correctn	EDIT
	Factors †	DONE
Signal Analysis Mo	nde	
		More EDIT
More (DISPLAY) 1 of 2	Limit Edit Lines Limit	More EDIT § 1 of 2 DONE
		1 01 2 2012
	Limit Edit	More EDIT
(SETUP) 1 of 3	Lines Limit .	§ 1 of 2 DONE

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

† Any of the following groups of softkeys can be used to complete the key path: Antenna Factors EDIT ANTENNA, or Cable Factors EDIT CABLE, or Other Factors EDIT OTHER.

§ Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

Related Programming Command

none

FIDTT FLATNESS

Softkey that allows flatness-correction constants to be viewed or modified. This is a service calibration function and is for service use only.

Key Path

		Flatness	
	Cal		FLATNESS

Related Programming Command

none

EDIT LAST

Softkey that starts the DLP editor function and allows the most recent item that was being edited, in the DLP editor buffer, to be accessed again. The item will not be in the user memory of the instrument until it is processed by the SAVE EDIT softkey. The DLP editor memory remains intact when the instrument is preset and when it is powered off.

Key Path

Recall Catalog (RECALL) Internal Interna	1	* Edito	r LAST
Save Catalog (SAVE) Internal Internal	*	Editor	EDIT LAST

^{*} Any of the following can be used to complete the key path: CATALOG ALL, CATALOG VARIABLS, or CATALOG PREFIX.

Related Programming Command


Edit Limit

Signal analysis mode only.

Softkey that allows you to edit the current limit-line tables by accessing Edit Upper, Edit Lower, Edit Up/Low, and

Edit Mid/Delt. Use PURGE LIMITS under any of the above edit menus to dispose of the current limit-line table.

Key Path



Related Programming Command

none

EDIT LIMIT

Receiver mode only.

Softkey that allows you to edit the current limit-line tables for limit line 1 or limit line 2. Use DELETE LIMITS under this menu to dispose of the current limit-line table.

Key Path

(DISPLA)	More 7 1 of 2	Limit 2 Lines	*	EDIT LIMIT
(SETUP)	More 1 of 3	Limit Lines .	**	EDIT LIMIT

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Related Programming Command

none

EDIT LIST

Softkey that accesses a menu to edit signal marking functions.

Key Path

Related Programming Command

EDIT LOWER

Signal analysis mode only.

Softkey that allows you to view or edit the lower limit-line table. Up to 30 entries are allowed for the lower limit-line table. With the lower limit-line table format, the coordinates for the lower limit-line are specified, but none are specified for the upper limit line. Even if upper limit-line values exist or the values had been entered as an upper and lower limit-line table, the lower limit-line values are treated as a separate table from the upper limit-line values. The lower limit-line entries can have independent frequency (or time) and amplitude coordinates from upper limit-line table entries.

Key Path

(DISPLAY)	More	Limit	Edit	EDIT
	1 of 2	Lines	Limit	LOWER
(SETUP)	More	Limit	Edit	EDIT
	1 of 3	Lines	Limit	LOWER

Related Programming Command

LIMIMODE

EDIT MID/DELT

Signal analysis mode only.

Softkey that allows you to view or edit the upper and lower limit-line tables simultaneously. These tables are edited by entering a middle amplitude value and an amplitude deviation. Up to 30 entries are allowed for the upper and lower limit-line tables. Like the upper and lower limit-line table format, the mid/delta limit-line table format provides a means of specifying the upper and lower limit lines at the same time. Unlike the upper and lower table format, the amplitude values are specified as a middle amplitude value with a delta (the upper and lower limit lines are drawn equal positive and negative distance from the middle amplitude).

With the mid/delta format the frequency (or time), and the middle amplitude plus the delta comprise the upper limit line; the frequency (or time), and the middle amplitude minus the delta comprise the lower limit line. The difference between the mid/delta and the upper/lower format is the way the amplitude values are entered: the frequency (time) coordinate begins a segment regardless of the format chosen. The mid/delta format can be used if the upper and lower limit lines are symmetrical with respect to the amplitude axis. An upper and lower amplitude component are specified for every frequency (or time) component.

Key Path

DISPLAY	More 1 of 2	Lines	LULU	EDIT MID/DELT
(SETUP)	More		Edit Limit	EDIT MID/DELT

Related Programming Command

LIMIMODE

EDIT OTHER

Softkey that accesses the ampcor editor to edit correction factors for devices other than antennas and cables.

Key Path

	 · · · · · · · · · · · · · · · · · · ·		
		HACTORS	

Related Programming Command

AMPCOR

EDIT PA FLTNESS

Softkey that allows the service center or factory to view the preamp on flatness data of the instrument.

Note

The service password must be entered to execute this command.

Key Path

	More	Hlatness	
			PPARTATE

Related Programming Command

none

EDIT UP/LOW

Signal analysis mode only.

Softkey that allows you to view or edit the upper and lower limit-line tables simultaneously. Up to 30 entries are allowed for the upper and lower limit-line tables. With the upper and lower limit-line table format, the upper and lower limit-lines can be entered at the same time.

With the upper and lower limit-line format, the frequency (or time), upper amplitude, and lower amplitude are specified. The frequency (or time) and upper amplitude value comprise the coordinate point

for the upper limit line, the frequency (or time) and lower amplitude value comprise the coordinate point for the lower limit line. It is not necessary to specify both an upper and lower amplitude component for every frequency (or time) component.

Key Path

DISPLAY	More) 1 of 2	Lines	Edit Limit	EDIT UP/LOW
(SETUP)	More	Limit Lines	Edit Limit	EDIT UP/LOW

Related Programming Command

LIMIMODE

EDIT UPPER

Signal analysis mode only.

Softkey that allows you to view or edit the upper limit-line table. Up to 30 entries are allowed for the upper limit-line table. With the upper limit-line table format, the coordinates of the upper limit line are specified, but none are specified for the lower limit line. Even if lower limit-line values exist or the values had been entered as an upper and lower limit-line table, the upper limit-line values are treated as a separate table from the lower limit-line values. The upper limit-line entries can have independent frequency (or time) and amplitude coordinates from lower limit-line table entries.

Key Path

(DISPLAY	More	Limit	Edit	EDIT
) 1 of 2	Lines	Limit	UPPER
(SETUP)	More 1 of 3	Limit	Edit Limit	EDIT

Related Programming Command

LIMIMODE

EDIT UPR LWR

Signal analysis mode only.

Softkey that selects upper or lower limit-line tables. It switches to the limit-line table that is not currently being edited.

Key Path

(DISPLAY)	More 1 of 2	Limit Lines	Edit Limit	*	EDIT UPR LWR
(SETUP)	More 1 of 3	Limit Lines	Edit Limit	*	EDIT UPR LWR

 * Either EDIT UPPER or EDIT LOWER can be used to complete the key path.

Related Programming Command

none

Editor

Softkey that accesses the menu of down loadable program (DLP) editor softkeys. Programming commands can be used to write a program to control the instrument. The built-in DLP editor uses the instrument rather than an external computer to create, view, or edit programs. These programs can then be sent to the command parser of the instrument, which is similar to outputting them to the instrument from an external computer.

Key Path

(RECALL)	Recall Internal	Internal	*	Editor
(SAVE)	Save Internal	Catalog Internal	*	Editor

^{*} Any of the following can be used to complete the key path. CATALOG ALL, CATALOG VARIABLS, or CATALOG PREFIX.

Related Programming Command

none

EMI RECEIVER

Softkey that configures the instrument as an EMI receiver.

Key Path

EMI (MODE) RECEIVER

Related Programming Command

EPSON MX

Softkey that specifies EPSON MX as the printer connected to the output port.

Key Path

			MAY

Related Programming Command

PRNTTYPE

ERASE STATEALL

Softkey that disposes of any or all user-defined variables.

Key Path

	More	Dispose	ERASE
(CONFIG)	1 of 3	User Mem	STATEALL

Related Programming Command

none

ERASE TRACEALL

Softkey that disposes of any or all user-defined traces.

Key Path

	∀ore		H.B.ASH.
		Dispose	
(CONFIG)		User Mem	TRACEALL.

Related Programming Command

none

ERRORS

Softkey that activates the error portion of the display screen for color editing.

Key Path

	Display	Adjust	Edit	More	
(DISPLAY)	Config	Color	Colors	1 of 3	ERRORS

Related Programming Command

SETC

EXECUTE TITLE

Softkey that executes a programming command displayed in the screen title area of the instrument. The Change Title function can be used to print programming commands in the screen title area of the display. The commands can then be executed from the front panel of the instrument, without an external computer, by pressing the EXECUTE TITLE softkey.

Key Path

W O TO O	Mara	SOTUTOO	H Y H I H H H H
			······································
	Z U L U		

Related Programming Command

none

EXIT

Softkey that exits the EDIT FLATNESS menu. This is a service calibration function and is designed for service use only.

Key Path

	Voro	SOTUTOO		
MATA				

Related Programming Command


none

EXIT CATALOG

Softkey that returns the instrument to the state it was in before the current catalog function was invoked. It clears the catalog display and returns to a normal display.

Key Path

Receiver Mode

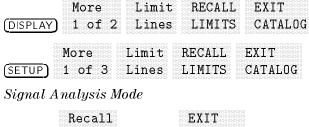

	Recall	EXL		
(RECALL)	Disk .	* CAT.	ALOG	
	Recall M	ore	EXI	Į.
(RECALL)	Disk 1	of 2	† CATA	
	Recall	Catalog	EXI'	ľ
(RECALL)	Internal	Internal	§ CAT.	ALOG

Save CATALOG EXIT Disk DISK CATALOG (SAVE)

Save Catalog EXIT Internal (SAVE) Internal CATALOG

RECALL EXIT (SETUP) SETUP CATALOG

More Save/Rcl RECALL EXIT (TEST) 1 of 3 List LIST CATALOG

Related Programming Command

none

EXIT EDIT Softkey that exits the annotation editor.

Key Path

EDIT EXIT (OUTPUT) ANNOTATN EDIT

Related Programming Command

EXITANNOT

EXIT GRAPH Softkey that exits the SAVE LIN GRAPH or SAVE LOG GRAPH report graph functions.

Key Path

(TEST)	More	Save/Rcl	SAVE	EXIT
	1 of 3	List	LIN GRAPH	GRAPH
(TEST)	More	Save/Rcl	SAVE	EXIT
	1 of 3	List	LOG GRAPH	GRAPH

^{*} Any of the following can be used to complete the key path. CATALOG DISK, RECALL SETUP, RECALL LIST, RECALL LIMITS or RECALL ANTENNA.

 $^{^{\}dagger}$ Any of the following can be used to complete the key path. RECALL CABLE, RECALL OTHER, or RECALL TRACE.

 $[\]S$ Any of the following can be used to complete the key path. CATALOG ALL, CATALOG VARIABLS, CATALOG PREFIX, or CATALOG REGISTER.

Related Programming Command

SIGGRAPH

EXIT LAST CAL Softkey that exits the LAST CAL menu.

Key Path

More EXIT (CALIBRATE) 1 of 3 Last Cal LAST CAL

Related Programming Code

none

EXIT MEASURE

Softkey that exits the MEAS STEPPED menu.

Key Path

	More	More	MEAS	EXIT	
TEST	1 of 3	2 of 3	STEPPED	MEASU	RE
	More	More	MEAS		EXIT
TEST	1 of 3	2 of 3	STEPPED	STOP	MEASURE
	More	More	MEAS	FREQ	EXIT
(TEST)	1 of 3	2 of 3	STEPPED	STEP	MEASURE

Related Programming Command

none

EXIT SHOW

Softkey that exits the SHW INST CONFIG function.

Key Path

	X1 (-) - f - (-)	~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~ ~	
(2011512)	 	CONFIG	CHIDII
I COM I G I			

Related Programming Command

HAVE, ID, REF, SER

EXTERNAL

Softkey that activates the trigger condition that allows the next sweep to start when an external voltage (connected to EXT TRIG INPUT on the rear panel) passes through approximately 1.5 volts. The external trigger signal must be a 0 V to +5 V TTL signal.

Key Path

TRIG

EXTERNAL

Related Programming Command

TM

EXTERNAL PREAMPG

Softkey that adds a positive or negative preamplifier gain value, which is subtracted from the displayed signal. EXTERNAL PREAMPG is similar to the REF LVL OFFSET; however, with the

EXTERNAL PREAMPG, the attenuation may be changed depending on the preamplifier gain entered. A preamplifier gain offset is used for measurements that require an external preamplifier or long cables. The offset is subtracted from the amplitude readout so that the displayed signal level represents the signal level at the input of the preamplifier. The preamplifier gain offset is displayed at the top left hand-side of the screen and is removed by entering zero. The preamplifier gain offset is entered using the data keys. Press CAL STORE if you want the instrument to use the current preamplifier gain offset when power is turned on. Preamplifier gain offset is set to zero when DEFAULT CONFIG is pressed. The preamplifier gain value is not affected by an instrument preset.

Key Path

More

EXTERNAL

(AMPLITUDE)

1 of 3 PREAMPG


Related Programming Command

PREAMPG

FAST STP ON OFF

Softkey that determines how stepped measurements are made. When OFF is selected, the MEAS STEPPED softkey performs a stepped measurement between the specified start and stop frequencies in increments set by the FREQ STEP softkey measuring all the selected detectors to the full accuracy of the instrument. When ON is selected and a limit margin is on (MARGIN # ON OFF), only the steps where the peak amplitude exceeds the limit margin are measured using the selected detectors. Using this softkey under normal conditions results in faster measurements due to the limited number of signals being measured.

Key Path



Related Programming Command

none

FFT MEAS

This softkey is only available when LIN is selected for the SWEEP LOG LIN softkey.

Softkey that activates a discrete fast Fourier transform based on the durrent setup. For additional information refer to Chapter 6, Making EMI Diagnostic Measurements, in the EMI Receiver Series User's Guide.

Key Path

(MEAS/USER) FFT MEAS


Related Programming Command

FFT

FINE TUNE DAC

Softkey that displays the output of the YTO fine-tune DAC, which is produced on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

FLAT

Softkey that draws a zero-slope line between the coordinate point of the current segment and the coordinate point of the next segment, producing limit-line values equal in amplitude for all frequencies between the two points. If the amplitude values of the two segments differ, the limit line "steps" to the frequency value of the second segment.

Key Path

Receiver Mode

INOT 6	Limit Lines	* LIMIT	Select Type FLAT
More	Limit	EDIT	Select
(SETUP) 1 of 3	Lines*	LIMIT	

Signal Analysis Mode

More (DISPLAY) 1 of	Limit Edit 2 Lines Limi	.,,	t m	t FLAT
More (SETUP) 1 of 3	Limit Edit Lines Limit	†	Туре	H L A L

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Related Programming Command

none

Flatness Data

Softkey that accesses a menu used to view or edit the flatnesscorrection constants. This is a service calibration function and is for service use only.

Key Path

	More	More	Service	Flatness
CALIDDATE	ገ 1 ለ£ 3	2 of 3	Cal	Nata
[CALIBRATE] 1 01 0	Z U1 U	val	раба

Related Programming Command

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

FM COIL DRIVE

Softkey that displays the output of the FM coil driver produced on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path

₩ oro	Moro			
		$\sim \gamma \omega + M + C \omega$		
			More 1	


Related Programming Command

none

FΜ GAIN

Softkey that adjusts the FM deviation display. The center graticule represents zero deviation. The top graticule is the positive deviation set by FM GAIN. The bottom graticule is the negative deviation set by FM GAIN. The range for FM gain is from 3 kHz to 1.175 MHz. The default value is 100 kHz. This is a service calibration function and is for service use only.

Key Path

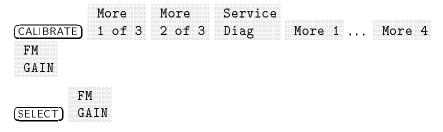


Related Programming Command

FMGAIN

FMOFFSET

Softkey that adjusts the horizontal trace for center-screen with no modulation on the carrier. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

FM SPAN

Softkey that displays the FM_SPAN signal from the span dividers on the A7 Analog Interface assembly. This is a service diagnostic function and is for service use only.

Key Path

WAT TO	More		

Related Programming Command

none

FORMAT DOS DISK

Softkey that formats a 3.5 inch double-sided floppy disk in DOS format.

A DOS filename consists of a:

prefix (optional) register number (required) file type descriptor (automatically supplied)

A DOS filename is defined as:

prefix = register #.file type descriptor for example "PREFIX3.SIG"

The filename, excluding the extension, cannot exceed eight characters. The file type descriptor is a three letter extension such as, "SIG" for a signal list.

Key Path

	Disk	FORMAT
CONFIG	Config	DOS DISK

Related Programming Command

FORMAT

FORMAT LIF DISK

Softkey that formats a 3.5 inch double-sided floppy disk in LIF format.

A LIF filename is defined as:

file type descriptor = prefix_register number for example, "tPREFIX_3"

The filename cannot exceed eight characters. The file type descriptor is a single character preceding the prefix such as, "t" for a trace.

Key Path

	FORMAT
	TTE DISK
I CONFIG I	

Related Programming Command

FORMAT

FREE RUN

Softkey that activates the trigger condition to start the next sweep as soon as possible after the last sweep.

Key Path

(TRIG) FREE RUN


Related Programming Command

TM

FREQ DIAG

Softkey that displays, in real-time, frequency diagnostic information for the local oscillator section. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

none

FRQ DISC NORM OFF

Softkey that indicates the status of the frequency discriminator as a function of LO span. This is a service diagnostic function and is for service use only.

Key Path

(CALIBRATE)	More 1 of 3	More 2 of 3	Service Diag	More 1	 More 4
FRQ DISC					
NORM OFF					

Related Programming Command

none

FREQ OFFSET

Softkey that inputs a frequency offset value that is added to the frequency readout, to account for frequency conversions external to the instrument. Offset entries are added to all frequency readouts including marker, start frequency, and stop frequency. Entering an offset does not affect the trace. Offsets are not added to the span. Frequency offsets are entered using the data keys.

When a frequency offset is entered, its value is displayed on the top left side of the screen. To eliminate an offset, press FREQ OFFSET and 0 (ENTER). Pressing (PRESET) also sets the offset to zero.

Key Path

	More	FREQ
(FREQUENCY)	1 of 2	OFFSET

Related Programming Command


FOFFSET

FREQ SCL LOG LIN

Softkey that specifies whether the limit line is derived from a logarithmic or linear frequency axis. Underline LIN to set the frequency axis to linear or LOG to set the frequency axis to logarithmic.

Key Path

Receiver mode

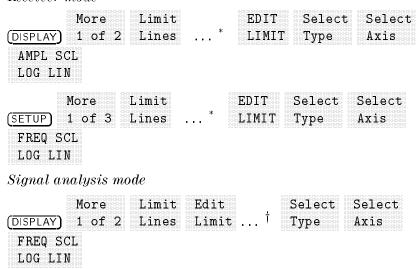

Edit More Limit Select Select (SETUP) 1 of 3 Lines Limit ... † Туре Axis FREQ SCL LOG LIN

Related Programming Command

LIMIFRQSCL

FREQ STEP

Softkey that sets the size of the frequency step for stepped measurements.

Key Path

	More	Inst	More	FREQ	
(SETUP)	1 of 3	Setup		STEP	
	More	More	MEAS	FREQ	
TEST	1 of 3	2 of 3	STEPPED	STEP	
	More	More	MEAS		FREQ
(TEST)		2 of 3	STEPPED	STOP	STEP

Related Programming Command

none

FREQUENCY

Hardkey that activates the center-frequency or start-frequency function and accesses a menu of other frequency functions. The center frequency or start frequency value appears below the graticule on the screen.

Although the instrument allows entry of frequencies greater than the specified frequency range, using frequencies greater than the frequency span of the instrument is not recommended.

Note

When changing both the center frequency and the span, change the frequency first since the span can be limited by the frequency value.

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

Related Programming Command

none

FRQ SCAN ON OFF

Softkey that reduces the signal span at the marker to zero span by performing an automatic zoom. When FREQ SCAN ON OFF is off, the instrument is restored to its previous setting with the exception of the marker which is placed at the same frequency as the zero scan (span) frequency.

Key Path

FRQ SCAN ON OFF (TEST)

Related Programming Command

none

FULL. SPAN

Softkey that changes the instrument span to full span. The span can be limited if harmonic band lock (BND LOCK ON OFF) is set to ON.

Key Path

FULL (SPAN) SPAN

Related Programming Command

FS

FULL WHITE

Softkey that replaces the standard display screen with a full-sized white box. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path


Display Test FULL WHITE (DISPLAY) Config Patterns

Related Programming Command

Gauss

Softkey that selects gauss as the transducer conversion units for the antenna amplitude-correction factors.

Key Path



Related Programming Command

XUNITS

GEO DST TEST

Softkey that replaces the standard display screen with a geometric distortion test pattern. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

		CEO DOT
		GEO DST
		COTTO PARTI
	Dattarno	
Config	manual transfer and the contract of the contra	

Related Programming Command

none

GHIJKL

Softkey that accesses the menu used for selecting screen title or prefix characters G through L.

Key Access

(CAL), (CONFIG), (DISPLAY), (RECALL), (SAVE), or (SETUP)

Related Programming Command

none

GND REF DETECTOR

Softkey that displays the output of the analog-ground reference produced on the A16 processor/video assembly. This is a service diagnostic function and is for service use only.

Key Path

	VIOTO	SOTUTO		
More		Service		(2MI) RHH
				DETECTOR
			MATA 1	

none

GRAT ON OFF

Softkey that turns the screen graticule on and off. This is helpful when alternative graphics are drawn on the screen through a remote controller and during plotting, when a graticule is not required.

Key Path

	More	GRAT
(DISPLAY)	1 of 2	ON OFF

Related Programming Command

GRAT

GRATICUL

Softkey that activates the graticule portion of the display screen for color editing.

Key Path

111511111		

Related Programming Command

SETC

GRAY SCALE

Softkey that replaces the standard display screen with a test pattern. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

	 	COATT

Related Programming Command

GREEN

Softkey that changes the intensity of the green portion of the primary light source output for the display annotation, traces, graticule, and so on.

Key Path

Related Programming Command

none

GREEN FILL

Softkey that replaces the standard display screen with a green box. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

			 Mama	
	DISDIAV		M() (C	" () (←
(DICDLAY)		Dattanna		
	(,()[] [] ()		/ ()	

`				
(

Related Programming Command

none

GRID

Softkey that replaces the standard display screen with a grid pattern. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

		More	More	More	
DIDPIG					
('ontion	Dattarna				

Related Programming Command

HALF FILL Softkey that replaces the standard display screen with half white screen. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

	1)7 cm 27	l'est	
	ртортау	1000	111111
(DICDLAY)	Config	Dattarna	
IDISPLAYI		Patterns	

Related Programming Command

none

HI VOLT TEST

Softkey that replaces the standard display screen with a high voltage regulation test pattern. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

	11700 277		
(DICDIAN)			
TIDISPLAY I	(,()[1] 0	Paulerns	

Related Programming Command

none

HOLD

Softkey that deactivates the active function and blanks the active function text from the display. No data can be accidentally entered using the knob, step keys, or data keys. Activating another function will turn off the hold function.

Key Path

(DISPLAY) HOLD

Related Programming Command

HD

HORIZ LINES

Softkey that replaces the standard display screen with a horizontal lines. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

Display		More		
Config	Pattarne	1 0f 4	2 of 4	

none

HSL RGB Softkey that accesses a menu to select one of the following: red, green, or blue (the three primary light sources that make up any color), hue (the pure color), saturation (the ratio of the pure color mixed with white), or luminosity (the brightness-per-unit area). When RGB is underlined, the softkeys RED, GREEN, and BLUE will be displayed. When HSL is underlined, the softkeys HUE, SATUR-ATION, and LUMIN-OSITY will be display.

Key Path

			01 01 01 01 01 01 01 01 01 01 01 01 01 0
	······································		

Related Programming Command

SETC

HUE

Softkey that changes the hue (pure color) of the specified portion of the display annotation.

Key Path

	Display	Adiust	Edit	
(DISPLAY) Config	Color	Colors	RGB HUE

Related Programming Command

SETC

IDNUM

Softkey that is used when the instrument is powered on the first time. It inputs the instrument model number and option information. This is a service calibration function and is for service use only.

Key Path

		VOTO	Service	
	MOTA	More		
				 1 1 3 M 1 1 M

Related Programming Command

IF BW AUTO MAN

Softkey that specifies the intermediate frequency bandwidth. When MAN is underlined, the coupling between sweep time and intermediate frequency bandwidth is disabled. When AUTO is underlined, coupling is reestablished.

Key Path

IF BW (BW) AUTO MAN

Related Programming Command

IFBW, RB

IF GAINS

Softkey that displays the gain setting of the following: RF Atten, 3rd Conv DAC, 21.4 Gain, Cal Atten, Lin Gain, and NBW Sgain. This is a service calibration function and is for service use only.

Key Path

	More	SATUICA	
	× () () (→		
			TE CATMS

Related Programming Command

none

INIT FLT

Softkey that is used when the instrument is powered on the first time. It sets the defaults for instrument flatness including the start and stop frequencies and the step size. All of the correction values are set to zero. This is a service calibration function and is for service use only.

Key Path

110 + 6	More	Service	rlatness	INIT
			D.G.G.G.	

Related Programming Command

INPT LCK ON OFF

Available only for an EMI receiver.

Softkey that limits tuning to values within the currently selected input path. For example, when input lock is on, and a stop frequency is selected out of the range of the currently selected input path, the actual stop frequency used will be the highest possible value allowed by the selected input path.

Key Path

More INPT LCK 1 of 2 ON OFF (FREQUENCY)

Related Programming Command

RFLINLK



Hardkey that accesses a menu to specify the input signal routing path through the RF filter section.

Related Programming Command

RFIN

Input

Softkey that accesses a menu that allows switching the 300 MHz calibrator signal so that it is routed to the RF input of the instrument.

Key Path

Inst More (SETUP) 1 of 3 Setup Input

Related Programming Command

none

INPUT 1

Softkey that displays the filter calibration data for input 1. This is a service calibration function and is for service use only.

Key Path

More More Service Display 1 of 3 2 of 3 Diag Sys Data INPUT 1 (CALIBRATE)

Related Programming Command

INPUT 1 9k-50M

Softkey that specifies the 9 kHz to 50 MHz input path (INPUT 1) as the signal routing path of the RF filter section.

Key Path

INPUT 1 9k-50M (INPUT)

INPUT 1 More Inst 1 of 3 Setup Input (SETUP) 9k-50M

Related Programming Command

RFIN

INPUT 1 PREAMP

Softkey that displays the calibration data for input 1, with the preamplifier on. This is a service calibration function and is for service use only.

Key Path

INPUT 1 More More Service Display (CALIBRATE) 1 of 3 2 of 3 Diag Sys Data PREAMP

Related Programming Command

none

INPUT 2 Softkey that is for service use only.

Key Path

More Display More Service 1 of 3 2 of 3 Sys Data INPUT 2 (CALIBRATE) Diag

Related Programming Command

none

INPUT 2 20M-2.9G

Softkey that specifies the 20 MHz to 2.9 GHz input path (INPUT 2) as the signal routing path of the RF filter section.

Key Path

INPUT 2 (INPUT) 20M-2.9G

INPUT 2 More Inst (SETUP) 1 of 3 Setup Input 20M-2.9G

RFIN

INPUT 2 1-6.5G

For an HP 8546A/HP 85462A only.

Softkey that specifies the 1 MHz to 6.5 GHz input path (INPUT 2) as the signal routing path of the HP 85420E/HP 85460A RF filter section.

Key Path

INPUT 2 1-6.5G (INPUT)

Inst INPUT 2 More (SETUP) 1 of 3 Setup Input 1-6.5G

Related Programming Command

RFIN

INPUT 2 BYPASS

Softkey that specifies the bypass input path (INPUT 2) as the signal routing path of the HP 85420E/HP 85460A RF filter section.

Key Path

INPUT 2 (INPUT) BYPASS

Inst INPUT 2 More (SETUP) 1 of 3 Setup Input BYPASS

Related Programming Command

BYPASS, RFIN

INPUT 2 PREAMP

Softkey that is for service use only.

Key Path

INPUT 2 More More Service Display (CALIBRATE) 1 of 3 2 of 3 Diag Sys Data PREAMP

Related Programming Command

INPUT Z 50Ω 75Ω

Softkey that sets the input impedance for voltage-to-power conversions. The impedance you select is for computational purposes only, since the actual impedance of 50Ω is set by internal hardware. The preset value can be changed by using a service function. Select the computational input impedance by pressing INPUT Z 50Ω 75Ω or by entering 50 or 75 using the data keys.

Key Path

INPUT Z More 1 of 3 50Ω 75Ω (AMPLITUDE)

Related Programming Command

INZ

Inst Setup

Softkey that accesses a menu which sets up the instrument for making EMI measurements.

Key Path

More Inst 1 of 3 Setup (SETUP)

Related Programming Command

none

INTENSITY

Softkey that changes the intensity or contrast of the display. The intensity level is shown on the top left-hand side of the screen. Use the knob or step keys to adjust the intensity level.

Key Path

Display (DISPLAY) Config INTENSITY INTENSITY (DISPLAY)

Related Programming Command

INTERNAL -> STATE

Softkey that recalls the saved instrument state from the selected state register. To recall a state, press INTERNAL -> STATE and use the data keys to enter a state register number (valid state register numbers are 1 through 9). State register 9 contains a previous state; state register 0 contains the current state. If windows are being used, the instrument state can only be recalled into the active window,

Key Path

	TNTERNAL.
Intornal	

Related Programming Command

RCLS

Internal -> Trace Softkey that accesses a menu that allows you to either; select the trace in which the trace data is to be recalled (trace A, trace B, or trace C), or recall the current limit-line tables. When recalling a trace, select the trace in which the trace data is to be recalled, enter the trace register number, and press (ENTER). If windows are being used, only the trace of the active window can be recalled.

When recalling a limit-line table, press LIMIT LINES, enter the trace register number, and press (ENTER). Valid trace register numbers are 0 through the maximum register number. The maximum register number is the number displayed after MAX REG # = during a save or recall operation. If a screen title is present, it is recalled with the trace data (but not with the limit-line table). If the screen title does not exceed 34 characters, the time and date when the data was stored will also be displayed. INVALID SAVEREG is displayed if data has not been stored in the trace register.

Key Path

	Recall	Internal
(RECALL)	Internal	-> Trace

Related Programming Command

RCLT

LASERJET

Softkey that specifies an HP LaserJet as the printer connected to the output port.

Key Path

(on tag	

Related Programming Command

PRNTTYPE

LASERJET

Softkey that specifies an HP LaserJet II as the printer connected to the output port.

Key Path

	Print	Printer	LASERJET
(=====	A		T T
CONFIG	Conrig	туре	

Related Programming Command

PRNTTYPE

LASERJET III

Softkey that specifies an HP LaserJet III as the printer connected to the output port.

Key Path

	Print.	Printer	LASERJET
(CONFIG)	Config	Туре	<u>III</u>

Related Programming Command

PRNTTYPE

Last Cal

Available only for an EMI receiver.

Softkey that displays the date of the last calibration for both the receiver RF section and the RF filter section.

Key Path

	More	Last
(CALIBRATE)	1 of 3	Cal

none

Last Hrd Key Menu

Softkey that changes the menu to the last hardkey menu that was active. This provides quick access between two separate hardkey menus.

Key Path

	More	More	Last Hrd
(SETUP)	1 of 3	2 of 3	Key Menu

Related Programming Command

LASTKEYMENU

LAST. SPAN

Softkey that changes the frequency span of the instrument to the previous span setting.

Key Path

LAST (SPAN) SPAN

Related Programming Command


LSPAN

Limit 1

Receiver mode only.

Softkey that accesses the menu for displaying, testing, deleting, and editing of limit 1 and its corresponding margin.

Key Path



Related Programming Command

LIMINUM

LIMIT 1 ON OFF

Receiver mode only.

Softkey that displays limit line 1 when ON is underlined.

Key Path

DISPLAY	More 7) 1 of 2	Limit Lines	Limit 1	ON OFF
(SETUP)	More 1 of 3	Lines	Limit 1	LIMIT 1 ON OFF


Related Programming Command

LIMILINESTA

Limit 2 Receiver mode only.

Softkey that accesses a menu for displaying, testing, deleting, and editing of limit 2 and its corresponding margin.

Key Path



Related Programming Command

LIMINUM

LIMIT 2 ON OFF

Receiver mode only.

Softkey that displays limit line 2 when ON is underlined.

Key Path

(DISPLAY	More 1 of 2	Limit Lines	; Limit 2	Z UN UFF
(SETUP)	More	Limit Lines	Limit 2	LIMIT 2 ON OFF

Related Programming Command

LIMILINESTA

LIMIT LINE 1

Softkey that activates the limit line 1 portion of the display screen for color editing.

Key Path

		UISDIAV			**************************************	
						1111111 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1
- 1	DICDLAY:	i contro	- $ -$	(a lare		
- 1	DISELAT			CLLLLO		


Related Programming Command

SETC

Limit Lines

Softkey that accesses the limit-line menus.

Key Path



Related Programming Command

none

LIMIT LINES

Softkey that saves or recalls limit-line tables in a trace register to or from a floppy disk or internal memory.

When accessed by (SAVE), the current limit-line table is stored to a trace register in internal memory or on a floppy disk. To save a limit-line table press, LIMIT LINES. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to: FILENAME is displayed. The limit-line table has now been saved to a disk.

When accessed by (RECALL), the limit-line table will be recalled from a trace register in internal memory. To recall a limit-line table press, LIMIT LINES, use the step keys or knob to highlight the desired file then press LOAD FILE.

Key Path

RECALI	Recall Dinternal	Internal -> Trace	LIMIT LINES
(SAVE)	Save Internal	Γrace -> INTRNL	LIMIT LINES
(SAVE)	Save More Disk 1 of	Trace 2 -> Disl	LIMIT t LINES

none

LIMITS -> DISK

Softkey that saves the current limit-line data to a floppy disk. To save a limit line press, LIMITS -> DISK. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The limit line has now been saved to a disk.

Key Path

Save LIMITS

SAVE Disk -> DISK

Related Programming Command

none

LIMITS FIX REL

Signal analysis mode only.

Softkey that allows you to choose fixed or relative type of limit lines. The fixed (FIX) type uses the current limit line as a reference with fixed frequency and amplitude values. The relative (REL) setting causes the current limit-line value to be relative to the displayed center frequency and reference-level amplitude values. When limit lines are specified with time, rather than frequency, the relative setting only affects the amplitude values. The current amplitude values will be relative to the displayed reference-level amplitude, but the time values will always start at the left edge of the graticule.

As an example, assume you have a frequency limit line. If the limit line is specified as fixed, entering a limit-line segment with a frequency coordinate of 300 MHz displays the limit-line segment at 300 MHz. If the same limit-line table is specified as relative, it is displayed relative to the center frequency and reference level of the instrument. If the center frequency is at 1.2 GHz, a relative limit-line segment with a frequency coordinate of 300 MHz will display the limit-line segment at 1.5 GHz. If the amplitude component of the relative limit-line segment is -10 dB, then -10 dB is added to the reference level value to obtain the amplitude of the given component (reference level offset included).

RELATIVE is displayed in the limit-line table when the limit-line type is relative; FIXED is displayed when limit-line type is fixed.

A limit line entered as fixed may be changed to relative, and one entered as relative may be changed to fixed. When changing between fixed and relative limit-lines, the frequency and amplitude values in the limit-line table change so that the limit line remains in the same position for the current frequency and amplitude settings of the

instrument. If a time and amplitude limit line is used, the amplitude values change but the time values remain the same.

Key Path

(DISPLAY)	More	Limit Lines	Limit		Mor * 1 o	e f 2	LIMITS FIX REL
(SETUP) 1	lore of 3	Limit Lines	Edit Limit	*	More	2	LIMITS

^{*} Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

Related Programming Command

LIMIREL

LIMITS FRQ TIME

Signal analysis mode only.

Softkey that selects whether limit lines will be entered using frequency or sweep time to define the segments. Limit lines can be created by the user to test trace data. They can be specified as a table of limit-line segments of amplitude versus frequency, or of amplitude versus time. Time values are evaluated with respect to the spectrum analyzer sweep time. A time value of zero corresponds to the start of the sweep, which is the left edge of the graticule.

Switching the limit line definition between frequency and time will erase the current limit-line table. The message If you are sure, press key again to purge data will appear. Press LIMITS FRQ TIME again to purge the limit-line table and switch between frequency and time.

Key Path

DISPLAY	More) 1 of 2	Limit Lines	Edit Limit	FRQ TIME
(SETUP)	More	Limit	EQIT	LIMITS
	1 of 3	Lines	Timi+	FRQ TIME

Related Programming Command

LIMIFT

LINE

Softkey that activates the trigger condition that allows the next sweep to be synchronized with the next cycle of the line voltage.

Key Path

(TRIG) LINE

Related Programming Command

TM

LINEARITY

Softkey that replaces the standard display screen with a linearity test pattern. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

	T		
	DISDIAV	lest	
(DISPLAY)	Config	Patterns	LINEARITY

Related Programming Command

none

(LINEARITY CHECK)

Hardkey that modifies the input RF attenuation to determine if a measured signal level is undergoing compression. (LINEARITY CHECK) is designed to be used with the Marker Subsystem in order to measure a specific signal level at different RF attenuation values.

Related Programming Command

LINCHK

LIN ON OFF Softkey that turns on or off the generation of a linear graph of the signal list. The linear graph is sent to the printer or plotter when OUTPUT REPORT is executed.

Key Path

Define LIN (OUTPUT) ON OFF Report

Related Programming Command

RPTDEF

LIST -> DISK Softkey that saves the current signal list to a floppy disk. To save a signal list press, LIST -> DISK. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The signal list has now been saved to a disk.

Key Path

Save LIST (SAVE) Disk -> DISK

Related Programming Command

none

LIST ON OFF

Softkey that enables or disables the generation of a tabular listing of a signal list. The listing is sent to a printer when OUTPUT REPORT is executed.

Key Path

Define LIST (OUTPUT) Report ON OFF

Related Programming Command

RPTDEF

LMT DISP Y N AUTO

Signal analysis mode only.

Softkey that displays any portion of the limit lines that are currently within the display boundary of the spectrum analyzer. If Y (yes) is underlined the limit lines are displayed. If N (no) is underlined they are not displayed. If AUTO is underlined, the display of the limit lines is dependent on the limit test function. The limit lines will be displayed while the limit test function is turned on, otherwise they will be turned off.

Key Path

LMT DISP More Limit 1 of 2 Lines Y N AUTO (DISPLAY) LMT DISP Limit More 1 of 3 Lines Y N AUTO (SETUP)

Related Programming Command

LIMIDISP

LMT TEST ON OFF

Softkey that turns the limit-line testing and (if LMT DISP AUTO is selected) turns the display of the limit lines on and off. When limit-line testing is enabled, every measurement sweep of trace A is compared to the limit lines.

Key Path

Receiver Mode

(DISPLAY)	More 1 of 2	Limit Lines	*	LMT TEST ON OFF
(SETUP) 1	ore of 3	Lines	*	ON OFF

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Signal Analysis Mode

(<u>DISPLAY</u>	More	Limit	LMT TEST
) 1 of 2	Lines	ON OFF
(SETUP)	More 1 of 3	Limit Lines	LMT TEST

Related Programming Command

LIMIFAIL, LIMITEST

LOAD FILE

Softkey that loads a file from the disk in the disk drive or a register into instrument memory.

Use the step keys or knob to view sections of the directory, then press LOAD FILE to select the highlighted file or register.

Note

Use of the LOAD FILE softkey is not recommended for recalling limit-line tables or amplitude-correction factors stored in internal memory.

Key Path

(RECALL)	Recall Disk	*	LOAI FILE		
(RECALL)	Recall Disk	More 1 of	2	LOAD † FILE	
(RECALL)	Recall Interna		alog ernal	Catalog Register	LOAD FILE
	ave CA isk DI	TALOG SK	LOAD FILE		

(SAVE)	Save Internal	Catalog Internal	CATAL		LOAD FILE
SAVE			CIDENI	L-E-IV	
	RECALL	LOAD			
(SETUP)	SETUP	FILE			
	More	Correctn	0	LOAD	
(SETUP)	1 of 3	Factor	§	FILE	
	More	Save/Rcl	RECALL	LOAI)
(TEST)	1 of 3	List	LIST	FILE	To the state of th

^{*} Any of the following can be used to complete the key path: CATALOG DISK, RECALL SETUP, RECALL LIST, RECALL LIMITS, or RECALL ANTENNA.

Receiver Mode

(DISPLAY	More) 1 of 2	Lim 2 Lin	it es	RECAL	S FILE
(SETUP)	More	Limit	RE	CALL	LOAD
	1 of 3	Lines	LI	MITS	FILE

Related Programming Command

LOAD

(LOCAL)

Pressing (CONFIG) (LOCAL) after the instrument has been placed in the remote mode places the instrument in the local mode and enables front-panel control. During remote operation, "R" appears in the lower-right corner of the screen indicating remote and talk. A "T" or "L" may appear during remote operation, indicating talk or listen. Pressing the (CONFIG) key removes the "R" symbol in the lower-right corner.

[†] Any of the following can be used to complete the key path: RECALL CABLE, RECALL OTHER, or RECALL TRACE.

[§] Any of the following groups of softkeys can be used to complete the key path: Antenna Factors RECALL ANTENNA, or Cable Factors RECALL CABLE, or Other Factors RECALL OTHER.

LOG ON OFF

Softkey that turns on or off the generation of a logarithmic graph of the signal list. The logarithmic graph is sent to the printer or plotter when OUTPUT REPORT is executed.

Key Path

Define LOG Report ON OFF (OUTPUT)

Related Programming Command

RPTDEF

LOGF SPD STD FAST

This softkey is only available when LOG is selected for the SWEEP LOG LIN softkey.

Softkey that selects between optimizing the frequency accuracy or minimizing the scan time. When "STD" is selected the frequency accuracy of the sweep is optimized. When "FAST" is selected the scan time of the sweep is minimized.

Note

Selecting the LOGF SPD STD FAST function has an effect on the minimum sweep time selected by the SWP TIME AUTO MAN function. The minimum sweep time is less than or equal to the minimum sweep time when SWP TIME AUTO MAN (AUTO) is selected.

Key Path

More LOGF SPD (FREQUENCY) 1 of 2 STD FAST

LOGF SPD STD FAST (SWEEP)

Related Programming Command

LOGSWEEPSPD

LUMIN-OSITY

Softkey that changes the luminosity (the brightness-per-unit area) of the specified portion of the display annotation.

Key Path

Display Adjust Edit HSL LUMIN-(DISPLAY) Config Color Colors ... RGB OSITY

SETC

MAIN COIL DR

Softkey that displays the output produced by the main-coil driver on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path

	Mara		
		Moro 1	

Related Programming Command

none

MATN SPAN

Softkey that displays the main-coil-span signal, MC_SPAN, from the span dividers on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path

	More	Mora	Service		MΔTN
	11010	TIOTO	COLVICO		
(CALIBRATE)		2 of 3		More 2	SPAN
GITEIDITITE					

Related Programming Command

none

MAN TRK ADJUST

Softkey that allows the user to adjust the frequency of the tracking-generator oscillator manually using the step keys or knob. The tracking adjust is tuned to maximize the amplitude of the trace.

Tracking error occurs when the output frequency of the tracking generator is not exactly matched to the input frequency of the instrument. The resulting mixing product from the instrument input mixer is not at the center of the IF bandwidth. Any tracking errors may be compensated for by manually adjusting the oscillator of the tracking generator, or by performing an automatic tracking routine, which is initiated by pressing TRACKING PEAK.

Key Path

MAN TRK TRACK GEN ADJUST

SRCTK

MARGIN 1 ON OFF

Softkey that sets the amplitude (in negative decibels) and display state for limit margin 1. The limit margin is a fixed amplitude relative to the limit line.

Key Path

(DISPLAY)	1 of 2	Limit Lines	Limit 1	ON OFF
(SETUP)	More 1 of 3	Lines	Limit 1	MARGIN 1 ON OFF

Related Programming Command

LIMIMARGAMP, LIMIMARGSTA

MARGIN 2 ON OFF

Softkey that sets the amplitude (in negative decibels) and display state for limit margin 2. The limit margin is a fixed amplitude relative to the limit line.

Key Path

(DISPLAY)	More 1 of 2	Limit Lines	Limit 2	ON OFF
(SETUP)	More 1 of 3	Lines	Limit 2	MARGIN 2 ON OFF

Related Programming Command

LIMIMARGAMP, LIMIMARGSTA

MARK ALL DUPLICAT

Softkey that marks all identical signals in the signal list.

Key Path

	More	FDTT	Signal	Selectv	MARK ALI.
(TEST)	1 of 3	LIST	Marking	Mark	DUPLICAT

Related Programming Command

SIGMARK

MARK ALL SIGNALS

Softkey that marks all signals in the signal list.

Key Path

More EDIT Signal MARK ALL (TEST) 1 of 3 LIST Marking SIGNALS			
More EDIT Signal MARK ALL (TEST) 1 of 3 LIST Marking SIGNALS			
More EDIT Signal MARK ALL (TEST) 1 of 3 LIST Marking SIGNALS			
More EDIT Signal MARK ALL (TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
(TEST) 1 of 3 LIST Marking SIGNALS			
TEST TOT S LIST MAINTING SIGNALS			
TEST TOT S LIST MAINTING SIGNALS			
TEST TOT S LIST MAINTING SIGNALS			
TEST TOT S LIST MAINTING SIGNALS			
TEST TOT S LIST MAINTING SIGNALS			
ILS I LOT OF BEAT HOLD STORAGE			

Related Programming Command

SIGMARK

MARK LWR DUPLICAT

Softkey that marks all duplicate signals in the list that are lower in peak amplitude.

Key Path

	More	EDIT	Signal	Selectv	MARK LWR
(TEST)	1 of 3	LIST	Marking	Mark	DUPLICAT

Related Programming Command

SIGMARK

MARK SIGNAL

Softkey that marks the highlighted signal in the signal list.

Key Path

	More	EDIT	Signal	MARK
(TEST)	1 of 3	LIST	Marking	SIGNAL
$\overline{}$				

Related Programming Command

SIGMARK

MARK TO END

Softkey that marks all signals, after the highlighted signal, to the end of the list.

Key Path

N.	iore	エリエエ	Signal	Selectv	MARK TO
	of 3	LIST		Mark	END

Related Programming Command

SIGMARK

MARKER

Softkey that activates a single marker at the center frequency on the active trace if an onscreen marker is not already displayed. If there is an onscreen marker, a frequency marker is enabled at the position of the first marker. Use the knob and data keys to position the marker. When a measurement point is selected with the marker, the frequency and the selected detectors (peak, quasi-peak, and average detectors) are displayed in the marker box.

Key Path

(TEST)	More 1 of 3	More 2 of 3	MEAS STEPPED		MARKER
(TEST)	More 1 of 3	More 2 of 3	MEAS STEPPED	FREQ STEP	MARKER

Related Programming Command

none

MARKER Δ

Softkey that activates a second marker at the position of the first marker. (If no marker is present, two markers appear at the center of the display.) The amplitude and frequency of the first marker is fixed, and the second marker is under your control. Annotation in the active function block and in the upper-right corner of the screen indicates the frequency and amplitude differences between the two markers. The display mode must not be changed between log and linear while using a delta marker.

Note

If there are already four markers when MARKER Δ is pressed, a nonactive marker disappears, the active marker becomes a reference marker, and the delta marker becomes the active marker.

Key Path

MARKER Δ (MKR)

PEAK SEARCH) MARKER Δ

Related Programming Command

MKD

MARKER Δ SPAN

Softkey that sets the start and stop frequencies to the values of the delta markers. The start and stop frequencies will not be set if the delta marker is off.

Key Path

MARKER (MKR->) ΔSPAN

Related Programming Command

MKSP

MARKER ->CF

Softkey that changes the instrument settings so that the frequency at the marker becomes the center frequency.

Key Path

MARKER ->CF (MKR ->)MARKER (PEAK SEARCH) ->CF

Related Programming Command

MKCF

MARKER ->CF STEP

Softkey that changes the center-frequency step size to match the value of the active marker. Press (FREQUENCY) then

CF STEP AUTO MAN to view the step size. If marker delta is active, the step size will be set to the frequency difference between the markers.

Key Path

MARKER MKR ->->CF STEP

Related Programming Command

MKSS

MARKER-> MINIMUM

Softkey that moves the active marker to the minimum detected amplitude value.

Key Path

MARKER-> MINIMUM (MKR ->)

Related Programming Command

MKMIN

MARKER ->PK-PK

Softkey that finds and displays the frequency and amplitude differences between the highest and lowest trace points. Pressing MARKER ->PK-PK performs the routine similar to pressing the following keys: (PEAK SEARCH), MARKER Δ, and MARKER-> MINIMUM.

Key Path

More MARKER (MKR ->) 1 of 2 ->PK-PK

Related Programming Command

MKPK

MARKER ->REF LVL

Softkey that changes the instrument settings so that the amplitude at the active marker becomes the reference level.

Key Path

MARKER ->REF LVL (MKR ->)

Related Programming Command

MKRL

MARKER ->START

Softkey that changes the start frequency so that it is equal to the frequency of the active marker. This moves the active marker to the left edge of the display.

Key Path

More MARKER (MRK ->) 1 of 2 ->START

Related Programming Command

none

MARKER ->STOP

Softkey that changes the stop frequency so that it is equal to the frequency of the active marker. This moves the active marker to the right edge of the display.

Key Path

More MARKER 1 of 2 ->STOP (MRK ->)

Related Programming Command

MKSTOP

MARKER 1 ON OFF

Softkey that makes marker 1 the active marker. If there is more than one marker displayed on the display, marker 1 must be made active before it can be manipulated.

Key Path

MARKER 1 (MKR) ON OFF

Related Programming Command

MKACTV

MARKER 2 ON OFF

Softkey that makes marker 2 the active marker. If there is more than one marker displayed on the display, marker 2 must be made active before it can be manipulated.

Key Path

MARKER 2 ON OFF (MKR)

MKACTV

MARKER 3 ON OFF

Softkey that makes marker 3 the active marker. If there is more than one marker displayed on the display, marker 3 must be made active before it can be manipulated.

Key Path

MARKER 3 ON OFF (MKR)

Related Programming Command

MKACTV

MARKER 4 ON OFF

Softkey that makes marker 4 the active marker. If there is more than one marker displayed on the display, marker 4 must be made active before it can be manipulated.

Key Path

MARKER 4 (MKR) ON OFF

Related Programming Command

MKACTV

MARKER ALL OFF

Softkey that turns off all of the markers, including markers used for marker track and demodulation. Marker annotation is also removed.

Key Path

MARKER More (MKR) 1 of 2 ALL OFF

Related Programming Command

MKOFF

MARKER AMPTD

Softkey that keeps the active marker at the requested amplitude on the screen. Once activated, the marker remains at the amplitude selected by the step keys, knob, or data keys, even if the signal frequency is changed. The marker will be placed on the signal furthest left at that amplitude. If no signal exists at that amplitude, it will be placed above the highest signal amplitude (or below the lowest trace element if it is below all trace elements). When marker delta is active in addition to marker amplitude, the behavior of the active marker is useful for measuring signal bandwidths. For example, place a marker 20 dB below the peak of a signal, press MARKER Δ, MARKER AMPTD. The marker readout shows the 20 dB bandwidth.

Key Path

MARKER (MKR) AMPTD

Related Programming Command

MKA, MKTYPE

(MARKER FUNCTION)

Hardkey that accesses the marker function softkeys. These softkeys can be used to access the marker table and to turn on marker functions for tracking the signal and counting its frequency. Noise markers and the marker pause are also accessed under MARKER FUNCTION).

Related Programming Command

none

MARKER NORMAL

Softkey that activates a single frequency marker at the center frequency on the active trace if an onscreen marker is not already displayed. If there is an onscreen marker before the MARKER NORMAL function is enabled, a frequency marker is enabled at the position of the first marker. Use the data controls to position the marker. Annotation in the active function block and in the upper-right corner indicates the frequency and amplitude of the marker. The marker stays on the trace at the horizontal screen position where it was left unless MK TRACK ON OFF,

MARKER AMPTD, or a "marker to" softkey function (such as MARKER ->CF, MARKER ->REF LVL, MARKER ->CF STEP, MARKER Δ ->SPAN, or MARKER-> MINIMUM) is selected. Pressing MARKER NORMAL turns off the marker-delta function.

Key Path

MARKER (MKR) NORMAL

Related Programming Command

MKN

MARKERS

Softkey that activates the markers portion of the display screen for color editing.

Key Path

	Display	Adjust	Edit	More	More
(DISPLAY)	Config	Colors	Colors	1 of 3	2 of 3
MARKER	S				

Related Programming Command

SETC

MARKER TUNE SPN

Softkey that modifies the behavior of the marker positioning functionality of the instrument when accessed through the data keys, knob, or stepkeys.

When MARKER TUNE SPN is activated and TUNE is underlined:

- Data key input, positions frequency and time markers at the specified numeric frequency input, tuning the instrument to the specified frequency if necessary. Numeric key-pad input terminators are "Hz, kHz, MHz, or GHz".
- Knob input, repositions the marker position as a function of frequency, tuning the instrument to its specified frequency if the knob input places the marker position beyond the limits of the current span.
- Step-key input:
 - □ Zero-span, steps the marker to the edge of the display and retunes the instrument on succeeding step-key presses.
 - \square Non-zero span, positions the marker at the next peak left ((\mathbb{T})) or next peak right (1) by one half of the intermediate frequency bandwidth. If no signals exist, the marker is positioned at the left edge ((1)) or the right edge ((1)) of the display. If the marker is already at the edge of the display, subsequent steps retune the instrument by a step equal to the size of the current span.

Key Path

MARKER (TEST) TUNE SPN

Related Programming Command

RCVRMRKR

MAX HOLD A

Softkey that maintains the maximum level for each trace point of trace A and updates each trace point if a new maximum level is detected in successive sweeps.

Key Path

MAX (TRACE) HOLD A

Related Programming Command

MXMH

MAX HOLD B

Softkey that maintains the maximum level for each trace point of trace B and updates each trace point if a new maximum level is detected in successive sweeps.

Key Path

MAX HOLD B (TRACE)

Related Programming Command

MXMH

MAX MXR LVL

Softkey that lets you change the maximum input mixer level in 10 dB steps from -10 dBm to -100 dBm. The mixer level is equal to the reference level minus the attenuator setting. As the reference level changes, the input attenuator setting is changed to keep the power levels less than the selected level at the input mixer. Pressing (PRESET) resets the maximum input mixer level to -10 dBm.

Key Path

More MAX MXR (AMPLITUDE) 1 of 3 LVL

ML

MEAS SNG CONT

Softkey that sets the stepped measurements for either single or continuous sweep mode.

Key Path

(TEST)	More	More 2 of 3		MEAS SNG C	
(IEST)				SNG G	
(TEST)	1 of 3	2 of 3	STEPPED	STOP	SNG CONT
(TEST)	More	More	MEAS	FREQ STEPA	MEAS

Related Programming Command

none

MEAS STEPPED

Softkey that initiates a stepped measurement. The stepped measurement is taken between the specified start and stop frequencies in conjunction with the selected step size (FREQ STEP), step type (STEP LOG LIN), and step mode (MEAS SNG CONT).

Key Path

	More	More	MEAS
(TEST)	1 of 3	2 of 3	STEPPED

Related Programming Command

none

(MEAS/USER)

Hardkey that switches between the User Menu and the menu containing FFT MEAS, 3 dB POINTS, 6 dB POINTS, 99% PWR PW, % AM, 3rd ORD MEAS, DELTA MEAS, and PK-PK MEAS. If no keys have been defined in the user menu, No User Menu is displayed.

MEASURE AT MKR

Softkey that makes a measurement, using specified detectors, with the marker position as the measurement frequency.

Note

When the selected bandwidth is a non-CISPR bandwidth the message, Non-CISPR bandwidth being used, press CONTINUE to resume or press USE CISPR to change, is displayed.

Key Path

MEASURE AT MKR (TEST)

Related Programming Command

MEASSIG

Measure Detector

Softkey that accesses a menu to select automatic measuring or the measurement time of the specified detectors.

Key Path

More Measure Inst (SETUP) 1 of 3 Setup Detector

Related Programming Command

none

MEM LOCKED

Softkey available only when SAV LOCK ON OFF is on.

Softkey that locks all the current internal state and trace registers against further data storage. With the state and trace memory locked, the STATE -> INTRNL and Trace -> Intrnl softkey functions are no longer accessible; MEM LOCKED is displayed instead. Pressing DEFAULT CONFIG or (PRESET) sets SAV LOCK ON OFF to OFF.

Note

When SAVE LOCK ON OFF is set to ON, none of the state registers can be overwritten, including state register nine. The instrument automatically updates state register nine with the last state unless the save lock function is on.

Key Path

Save MEM Internal LOCKED SAVE

PSTATE

MIN HOLD C

Softkey that updates trace C with the minimum level detected.

Key Path

MIN (TRACE) HOLD C

Related Programming Command

MINH

MIXER BIAS DAC

For an HP 8546A/HP 85462A only.

Softkey that displays the output of the mixer-bias DAC from the first-converter driver on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

Key Path

More More Service (CALIBRATE) 1 of 3 2 of 3 Diag More 1 ... More 5 MIXER BIAS DAC

Related Programming Command

none

MK COUNT ON OFF

Softkey that turns on the marker counter when ON is underlined. If no marker is active before MK COUNT ON OFF is pressed, a marker is activated at center screen. Press MK COUNT ON OFF (so that OFF is underlined), to turn the marker counter off. Press CNT RES AUTO MAN to change the marker counter resolution to an uncoupled value.

An (*) may appear in the upper right of the display along with the message Marker Count. The ratio of the intermeditate frequency bandwidth to span must be greater than 0.01 for the marker count function to work properly. Reduce Span appears on screen if the bandwidth to span ratio is less than 0.01. The function will count the largest signal in a 300 Hz bandwidth even if a narrower bandwidth setting is used.

Key Path

MK COUNT MARKER FUNCTION ON OFF

Related Programming Command

MKFC

MK NOISE ON OFF

Softkey that reads out the average noise level, referenced to a 1 Hz noise power bandwidth, at the marker position. If no marker is present, a marker appears at the center of the screen. The root-mean-square noise level, normalized to a 1 Hz noise power bandwidth, is read out. The sample detector is activated.

Key Path

MK NOISE (MARKER FUNCTION) ON OFF

Related Programming Command

MKNOISE

MK PAUSE ON OFF

Softkey that stops the instrument sweep at the marker position for the duration of the dwell time. The dwell time can be set from 2 milliseconds to 100 seconds.

Key Path

MK PAUSE ON OFF (MARKER FUNCTION)

Related Programming Command

MKPAUSE

(MKR)

Hardkey that accesses the marker control softkeys which select the type and number of markers and turn them on and off. Markers are diamond-shaped characters that identify points of traces and allow the traces to be manipulated and controlled on the screen. During manual operation, four markers may appear on the display simultaneously; only one can be controlled at a time. The marker that is controlled is called the "active" marker. Pressing (MKR) activates the MARKER NORMAL softkey.

Related Programming Command

none

(MKR ->)

Hardkey that accesses a menu of marker-to-functions such as,

- MARKER -> CF
- MARKER -> REF LVL
- MARKER -> CF STEP
- MARKER -> MINIMUM
- MARKER -> START
- MARKER -> STOP
- MARKER -> PK-PK
- MARKER Δ SPAN

Related Programming Command

none

MK READ FTIP

Softkey that selects the marker readout to be displayed in signal frequency, sweep time, the inverse of the sweep time, or the period which is the inverse of the frequency. When the instrument is in zero span the frequency type readout cannot be selected.

Key Path

More MK READ (MKR) 1 of 2 F T I P

Related Programming Command

MKREAD

MK TRACE AUTO ABC

Softkey that assigns a marker to a trace. Pressing

MK TRACE AUTO ABC will activate a marker on trace A if there are no markers turned on. If a marker is currently active, press MK TRACE AUTO ABC until A, B, or C are underlined. The active marker will be moved to the selected trace.

Selecting the auto mode will move the marker to the trace that is automatically selected. The selection order is to first look for a trace in the clear-write mode, in trace A, then trace B, then trace C. If no traces are currently being written, it will select a trace in the view-store mode, again in the order of trace A, B, then C.

Key Path

More MK TRACE (MKR) 1 of 2 AUTO ABC

Related Programming Command

MKTRACE

MK TRACK ON OFF

Softkey that moves the signal that is nearest to the active marker to the center of the screen and keeps the signal there. MKR-TRK or CNTR-TRK appears in the upper-right corner of the display. An (*) may appear in the upper-right corner of the display while the instrument is verifying that it has the correct signal.

Pressing MK TRACK ON OFF, (PRESET), MARKER NORMAL, or MARKER ALL OFF turns off the marker-track function.

When marker track is on and the span is reduced, an automatic zoom is performed: the span is reduced in steps so that the signal remains at the center of the screen. If the span is zero, marker track cannot be activated.

Key Path

MK TRACK (MARKER FUNCTION) ON OFF

Related Programming Command

MKTRACK

MNOPQR

Softkey that accesses a menu for selecting screen title or prefix characters M through R.

Key Access

(CAL), (CONFIG), (DISPLAY), (RECALL), (SAVE), or (SETUP)

Related Programming Command

(MODE)

Hardkey that accesses the menu for selecting EMI RECEIVER or SIGNAL ANALYSIS modes of operation.

Related Programming Command

none

MONO-CHROME

Softkey that sets the screen display to green monochrome. The monochrome display is uses different shades of green for each green value. This is especially useful for driving external monochrome monitors from the green video output.

Key Path

		MONO-
	~nac-13-	
		CHRUME
(Ontro	(A A A A C	

Related Programming Command

SETC

NEW EDIT

Softkey that starts the DLP editor function, clearing the DLP editor memory to create a new item in the 2500 byte DLP editor memory. The item will not be in the user memory of the instrument until it is processed by the SAVE EDIT softkey. The DLP editor memory buffer remains intact when the instrument is preset and when it is powered off.

Key Path

	l Internal	*	Editor	EDIT
Save [SAVE] Internal	Catalog Internal		Editor	NEW EDIT

^{*} Any of the following can be used to complete the key path: CATALOG ALL, CATALOG VARIABLS, or CATALOG PREFIX.

Related Programming Command

NEXT

Hardkey that selects the upper or lower window as the active window. When the windows display mode is activated, there will be two windows displayed on the screen. Only one of the windows is active (the active window will have a highlighted line around the graticule). Pressing (NEXT) consecutively, will toggle between the two windows.

Related Programming Command

WINNEXT

NEXT PAGE

Softkey that displays the next page of the instrument setup. For example, if you are currently viewing page 2 of the instrument setup pressing NEXT PAGE will display page 3 of the instrument setup.

Key Path

	More	SHOW	NEXT
(===:==)		armin	EN A COLET
ISETUP	LOIS	SEIUP	PAGE

Related Programming Command

none

NEXT PEAK

Softkey that moves the active marker to the next signal peak of higher amplitude. The signal peak must exceed the threshold value. (Also see the PEAK EXCURSN and THRESHLD ON OFF softkey descriptions.)

Key Path

NEXT PEAK (PEAK SEARCH)

Related Programming Command

MKPK

NEXT PK LEFT

Softkey that moves the marker to the next peak left of the current marker. The signal peak must exceed the threshold value. If there is no peak to the left, the marker will not move. (Also see the PEAK EXCURSN and THRESHLD ON OFF softkey descriptions.)

Key Path

NEXT PK PEAK SEARCH LEFT

Related Programming Command

MKPK

NEXT PK RIGHT

Softkey that moves the marker to the next peak right of the current marker. The signal peak must exceed the threshold value. If there is no peak to the right, the marker will not move. (Also see the PEAK EXCURSN and THRESHLD ON OFF softkey descriptions.)

Key Path

NEXT PK (PEAK SEARCH) RIGHT

Related Programming Command

MKPK

NΟ CONVERSN

Softkey that specifies that no conversion units are used for the antenna amplitude-correction factors.

Key Path

(SETUP) 1	ore	Correctn Factors	Antenna Factors	EDIT ANTENNA	More 1 of 2
Antenna Units	NO CONV	ERSN			

Related Programming Command

XUNITS

No User Menus

Softkey that is displayed if no user menus have been defined by the user.

Key Path

User No User (MEAS/USER) Menus Menus

Related Programming Command

NORMLIZE ON OFF

Softkey that subtracts trace B from trace A and adds the result to the display line. The result is displayed in trace A. The trace data is normalized with respect to the display line even if the value of the display line is changed. This function is executed on all subsequent sweeps until it is turned off. A minus sign (-) appears between the trace A status and the trace B status in the screen annotation while the function is active. To turn off the normalize function, press NORMLIZE ON OFF so that OFF is underlined.

The normalize function is useful for applying correction data to a trace. For example, store a measurement sweep of the response of a system in trace B. Trace A can be used to measure the response of the system after a device is added. Set NORMLIZE ON OFF to ON to subtract the system response from the response of the device under test, to characterize the response of a device under test.

Key Path

			NORMALIZE
		More	NURMALIZE
١	(TRACE)	1 of 3	ON OFF

Related Programming Command

AMBPL

NORMLIZE POSITION

Softkey that displays the display line and makes the display line function active. The trace data is normalized with respect to the display line even if the value of the display line is changed.

Key Path

	More		MALTZE
			TTTON
ITRACEI			

Related Programming Command

none

ON/OFF

Hardkey that turns the AM or FM demodulation on and off. If the instrument is in a nonzero span, a marker is placed at center screen if an onscreen marker is not already present. The marker pause is changed to equal the current dwell time value. Demodulation takes place on any signal that is indicated by the marker position during the marker pause. There is no change to the display during marker pause, but the demodulation signal is present on the AUX VIDEO OUT. Also see the SPEAKER ON OFF softkey description.

Pressing (ON/OFF) selects the sample peak detector for AM demodulation, the FMV detectors for FM demodulation. If the instrument is in zero span, demodulation is done continuously, with or without an onscreen marker.

Related Programming Command

DEMOD

OPTICAL FILTER

Softkey that selects a vision enhanced mode where an optical filter is used to accommodate the use of protective goggles when viewing lasers.

Key Path

	Display	Adjust	Special	OPTICAL
		11 11 11 11 11 11 11 11 11 11 11 11 11	10 10	
				
(DISPLAY)	Config	Color	Colors	FILTER

Related Programming Command

SETC

OTHER -> DISK

Softkey that saves *other* two-port amplitude-correction factors to a disk. To save *other* amplitude-correction factors press, OTHER -> DISK. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The other two-port amplitude-correction data has now been saved to a disk.

Key Path

	Samo	More	OTHER
		110.11.0	
(CAVE)	Diek	1 of 2	-> DICK
SAVE	DION	L VI	

Related Programming Command

none

Other Factors

Softkey that accesses a menu to turn on, recall, edit, or save other amplitude-correction factors for any two-port device, excluding antenna and cable factors, placed between the antenna and the instrument.

Key Path

	Vara	(:orrectn	Other
(CETIID)		Hactore	Hartore
		racturs	
()			

Related Programming Command

AMPCOR

OTHER ON OFF

Softkey that turns on or off other two-port amplitude-correction factors, excluding antenna and cable factors, placed between the antenna and the instrument.

Key Path

			Other	OTHER
	More	('orrectn		
	\	Factore	Factors	ON OFF

Related Programming Command

AMPCOR



Hardkey that accesses a menu to output reports to a plotter or a printer, or send a copy of the current display to the printer.

Related Programming Command

none

OUTPUT REPORT

Softkey that outputs a report to the specified plotter or printer.

Key Path

OUTPUT (OUTPUT) REPORT

Related Programming Command

none

OVLD ON OFF

Softkey that enables or disables RF and IF overload status.

Key Path

OVLD (AMPLITUDE) ON OFF

More OVLD Inst (SETUP) 1 of 3 Setup ON OFF

Related Programming Command

OVLD

PAINTJET

Softkey that specifies an HP PaintJet as the printer connected to the output port.

Key Path

Related Programming Command

PRNTTYPE

PALETTE BARS

Softkey that replaces the standard display screen with palette bars. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

Display Config	Display Test Config Patterns	Display Test More Config Patterns 1 of 4

Related Programming Command

none

PEAK EXCURSN

Softkey that sets the minimum amplitude variation of signals that the marker can identify as a peak. If a value of 10 dB is selected, the marker moves only to peaks that rise and fall more than 10 dB above the threshold line (or the noise floor of the display). Pressing (PRESET) or turning on power resets the excursion to 6 dB, and the threshold to 70 dB below the reference level.

Note

When a peak has a lump on its skirt that is the peak-excursion value above the threshold, the lump is considered a peak in its own right only if it has a peak excursion drop on both sides. Two peaks that are so close that only a valley divides them are not differentiated if the valley is not the peak-excursion value deep.

When the peak excursion value is less than 6 dB, the marker-peaking functions may not recognize signals less than 6 dB above the noise floor. To correct this, when measuring signals near the noise floor, the excursion value can be reduced even further. To prevent the marker from identifying noise as signals, reduce the noise floor variance to a value less than the peak-excursion value by reducing the average video bandwidth or by using video averaging.

Key Path

	More	PEAK
(PEAK SEARCH)	1 of 2	EXCURSN

PEAK (CTRL) EXCURSN

Related Programming Command

MKPX

Peak Menu

Softkey that accesses the softkeys that are available when (PEAK SEARCH) is pressed (see the key description for (PEAK SEARCH) below). Pressing Peak Menu instead of (PEAK SEARCH) allows you to use the peak-search functions without initiating a new peak search.

Key Path

More Peak $\overline{\text{MKR}} \rightarrow 1 \text{ of } 2$ Menu

Related Programming Command

none

(PEAK SEARCH)

Hardkey that automatically places a marker on the highest amplitude of a trace, and displays the amplitude and frequency of the marker. It also accesses the menus of marker peak functions.

Related Programming Command

MKPK

PK DWELL TIME

Softkey that sets the measurement time when the peak detector is measured. This key is used in conjunction with MEASURE AT MKR, RE-measure, AUTO-MEASURE, and MEAS STEPPED.

Key Path

More Inst Measure PK DWELL (SETUP) 1 of 3 Setup Detector

Related Programming Command

MEASTIMEPK

PK-PK MEAS

Softkey that initiates an automatic measurement of the frequency and amplitude differences of the highest and lowest signals displayed on the screen. Pressing PK-PK MEAS performs a routine that is similar to MARKER Δ and then moving the second marker to the lowest detected signal.

Key Path

	More	PK-PK
(MEAS/USER)	1 of 2	MEAS

Related Programming Command

none

Plot Config

Softkey that accesses the menu used to address the plotter and to select plotter options. See the (COPY) key for more information.

Key Path

Plot (CONFIG) Config

Related Programming Command

none

PLOTTER ADDRESS

Softkey that changes the HP-IB address of the plotter. The plotter address is set to 5 when DEFAULT CONFIG is pressed.

Key Path

Plot PLOTTER Config ADDRESS (CONFIG)

Related Programming Command

PLT MENU ON OFF

Softkey that allows the softkey labels to be plotted along with the display. This function operates when the (COPY) key is used in a plot configuration. The plot menu function is set to on when DEFAULT CONFIG is pressed.

Key Path

Plot PLT MENU (CONFIG) Config ON OFF

Related Programming Command

none

PLTS/PG 1 2 4

Softkey that allows you to choose a full-page, half-page, or quarter-page plot. Press PLTS/PG 1 2 4 to underline the number of plots per page desired. If two or four plots per page are chosen, a softkey function is displayed that allows you to select the location of the plotter output on the paper. If two plots per page are selected, [] LOC _ _ is displayed. If four plots per page are selected, [] _LOC _ _ is displayed. Press the softkey until the rectangular marker is in the desired section of the softkey label. The upper and

lower sections of the softkey label graphically represent the position

Note

The HP 7470A plotter does not support two plots per page output, you can select one or four plots per page.

of the page where the plotter output will be located.

Key Path

PLTS/PG Plot (CONFIG) Config 1 2 4

Related Programming Command

none

POINT

Softkey that specifies a limit value for one coordinate point, so that a point segment specifies a limit value for a single frequency. (For signal analysis mode only, the point segment can specify a limit value for time also.) The point segment type is generally used as the last segment in the limit-line table. However, if the last segment in the table is not of the point segment type, an implicit point is automatically added at the right-hand side of the screen.

Key Path

Receiver Mode

More Limit (DISPLAY) 1 of 2 Lines		EDIT Select LIMIT Type POINT
More Limit (SETUP) 1 of 3 Lines	*	EDIT Select LIMIT Type POINT

Signal Analysis Mode

(DISPLAY	More) 1 of 2	Limit Lines	Edit Limit	†		t POINT
(SFTUP)	More 1 of 3	Limit Lines	Edit Limit	<u> </u>	Type	POINT

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

Related Programming Command

none

POWER ON IP LAST

Softkey that determines the state of the instrument when the instrument is powered on. If the POWER ON function is set to IP, the state of the instrument is the same as it is after (PRESET) is pressed, when the instrument is powered on. If the POWER ON function is set to LAST, then the state that the instrument was left in when it was powered off is recalled.

The setting (IP or LAST) of the POWER ON function is not changed by pressing (PRESET). Use the POWER ON IP LAST softkey function to change the setting of the instrument state which is recalled at power on. Limit lines are not recalled when the instrument is powered up.

Note

If you have a downloadable program or "personality" installed in internal memory, the following changes apply to the operation of the POWER ON function: When using a downloadable program or personality, the last state of the personality is not recalled. We recommend that if you are using a downloadable program or personality, you set POWER ON IP LAST to IP. If

POWER ON IP LAST is set to LAST, you must press (PRESET) whenever you power on the instrument.

Key Path

	Mara	VIOTO	POWER ON
		WI O T O	
			TINTAME
(CONFIG)			

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

	Momo	100	POWER ON
	More	More	PUWER UN
(OFTUD)			TINTAME
[SETUP]	1 01 3	2 OI 3	IP LASI

Related Programming Command

POWERON



Hardkey that switches the system preamplifier in and out of the input path. (PREAMP) acts as an on or off toggle switch. This key performs the same function as the PREAMP ON OFF softkey.

PREAMP ON OFF

Softkey that switches the system preamplifier in and out of the input path.

When the preamplifier is on:

The receiver RF section with RF filter section adds 12 dB of gain to the path of either INPUT 1 (9 kHz to 50 MHz) or INPUT 2 (20 MHz to 2.9 GHz).

The EMI receiver and standalone receiver RF section adds 27 dB of gain to either the path of INPUT 2 (1 GHz to 6.5 GHz) or the bypass path of INPUT 2.

Note

INPUT 2 (1 GHz to 6.5 GHz) is available only for the HP 8546A EMI receiver or the HP 85462A receiver RF section.

When the RF filter section is present in the system, the following input path selections set the preamplifier as follows:

- INPUT 1 (9 kHz to 50 MHz): PREAMP OFF
- INPUT 2 (20 MHz to 2.9 GHz): PREAMP OFF
- INPUT 2 (1 GHz to 6.5 GHz): PREAMP ON
- INPUT 2 bypass: PREAMP OFF

Key Path

	More	Inst	PREAMP
(SETUP)	1 of 3	Setup	ON OFF

Related Programming Command


PREAMP

PRESEL DAC

For an HP 8546A/HP 85462A only.

Softkey that peaks the YTF preselector by allowing the user to manually adjust the YTF fine-tune DAC. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

none

PRESEL DEFAULT

For an HP 8546A/HP 85462A only.

Softkey that enables default preselector data to allow maximum frequency response without peaking the preselector. The CAL YTF routine should be performed before pressing PRESEL DEFAULT.

Key Path

	More	PRESEL
CAMPLITUDE	1 4 2 9	DEFAILT
(AMPLITUDE)	1 01 3	DEFAULI

Related Programming Command

none

PRESEL PEAK

For an HP 8546A/HP 85462A only.

Softkey that optimally centers the preselector on a given signal for the most accurate measurement of amplitude. The maximum response found for the frequency at the marker determines the future adjustment values that will be provided to the preselector.

Key Path

PRESEL PEAK (AMPLITUDE)

Related Programming Command

PP

PRESET

Hardkey that provides a convenient starting point for making most measurements. Pressing (PRESET) displays softkeys used for accessing the operating modes available for your instrument. See Table 4-6 and Table 4-7 for the conditions established by pressing (PRESET).

The instrument preset function performs a processor test, but does not affect CAL data. Pressing (PRESET) clears both the input and output buffers, but does not clear trace B. The amplitude values of trace C are set to the reference level. Amplitude-correction factors are turned off. Limit-line testing is turned off, but the limit-line tables remain in internal memory. The status byte is set to 0. Instrument preset affects all operating modes. (See the key description for (MODE) for more information about other operating modes.)

Note

Turning the instrument on performs an instrument preset. Turning on the instrument also fetches CAL data; completes a processor test; clears trace B, trace C, and both the input and output buffers; turns off amplitude correction factors; turns off limit-line testing; and sets the status byte to 0. The last state of the instrument (before it was switched off) is recalled, unless instrument preset has been set by the power on function.

Table 4-6. Preset Conditions for Receiver Mode of Operation

A - B -> A	off
Amplitude correction factors	off
Amplitude units	default values
Annotation and graticule display	on
Attenuation	10 dB (auto-coupled)
Average bandwidth	1 MHz (auto-coupled)
AV/IFBW ratio	0.3
Center frequency	600 MHz
CF step size	100 MHz
Coupled functions	all set to AUTO
Coupling	AC
Detector	positive peak
Display line level	2.5 graticule divisions below reference level, display off
Frequency offset	0 Hz
Intermediate frequency bandwidth	120 kHz (auto-coupled)
Limit-line testing	off
Log scale	10 dB/division
Marker counter	off
Marker counter resolution	auto-coupled
Markers	off
Mixer level	-10 dBm
Operating mode	receiver
Preselector peak	reset
Reference level	92 dBμV in power-on units
Reference level offset	0 dB
Reference level position	top (8th) graticule
Span	6.5 GHz
SRQ mask	octal 50
Start Frequency	200 MHz
Stop Frequency	1 GHz.
State registers 1—8	unaffected
Sweep	continuous
Threshold level	one graticule above baseline, display off
Title	cleared
Trace A	clear-write
Trace B	store-blank
Trace C	store-blank, at reference level
Trace registers	unaffected
Trigger	free run
Video averaging	off

Table 4-7. Preset Conditions for Signal Analysis Mode of Operation

A - B -> A	off
Amplitude correction factors	off
Amplitude units	default values
Annotation and graticule display	on
Attenuation	10 dB (auto-coupled)
Average bandwidth	1 MHz (auto-coupled)
AV/IFBW ratio	0.3
Center frequency	3.25 GHz
CF step size	100 MHz
Coupled functions	all set to AUTO
Coupling	AC
Detector	positive peak
Display line level	2.5 graticule divisions below reference level, display off
Frequency offset	0 Hz
Limit-line testing	off
LIMIHI and LIMILO	cleared
Log scale	10 dB/division
Marker counter	off
Marker counter resolution	auto-coupled
Markers	off
Mixer level	-10 dBm
Operating mode	signal analysis
Preselector peak	reset
Reference level	0 dB in power-on units
Reference level offset	0 dB
Reference level position	top (8th) graticule
Resolution bandwidth	3 MHz (auto coupled)
Span	800 MHz GHz
SRQ mask	octal 50
Start Frequency	0 Hz
Stop Frequency	6.5 GHz.
State registers 1—8	unaffected
Sweep	continuous
Threshold level	one graticule above baseline, display off
Title	cleared
Trace A	clear-write
Trace B	store-blank
Trace C	store-blank, at reference level
Trace registers	unaffected
Trigger	free run
Video averaging	off
Video bandwidth	120 kHz

PRESET RECEIVER

Softkey that allows the receiver mode only to be preset. Table 4-8 lists the conditions affected by the preset receiver function. Other operating modes will not be affected. See the description of the (MODE) key.

Table 4-8. Preset Receiver Conditions

A - B -> A	off
Annotation and graticule	on
Attenuation	coupled
Average video bandwidth	300 kHz (coupled)
AV/IFBW ratio	0.3
Center frequency	1.46 GHz
Center frequency step size	100 MHz
Coupled functions	all set to AUTO
Coupling	AC
Detector	positive peak
Display line	off
Frequency offset	0 Hz
Harmonic lock	off
IF Bandwidth	120 kHz (coupled)
Limit-line testing	off
Marker counter	off
Marker counter resolution	6 kHz (auto-coupled)
Markers	off
Reference level	92 dBμV in power-on units
Reference level offset	– 15 dBm
Reference level position	top (8th graticule)
Scale	log 10dB/div
Span	2.88 MHz
Start Frequency	20 MHz
Stop Frequency	2.9 GHz
State registers 1—8	unaffected
Sweep	continuous
Sweep time	2.70 s (auto-coupled)
Threshold	off
Trace A	clear write
Trace B	store-blank
Trace C	store-blank
Trace math	cleared
Trace registers	unaffected
Trigger	free
Video averaging	off

Key Path

 ${f (MODE)}$ PRESET RECEIVER, when the instrument mode of operation is $receiver\ and\ the\ (MODE)\ hardkey\ is\ pressed\ twice.$

Related Programming Command

none

PRESET SPECTRUM

Softkey that allows the signal analysis mode only to be preset. Table 4-9 lists the conditions affected by the preset spectrum function. Other operating modes will not be affected. See the description of the (MODE) key.

Table 4-9. Preset Spectrum Conditions

	ectium conditions
A - B -> A	off
Annotation and graticule	on
Attenuation	10 dB (coupled)
AV/IFBW ratio	0.3
Center frequency	3.25 GHz
Center frequency step size	100 MHz
Coupled functions	all set to AUTO
Coupling	AC
Detector	positive peak
Display line	off
Frequency offset	0 Hz
Harmonic lock	off
Limit-line testing	off
Marker counter	off
Marker counter resolution	2 kHz (auto-coupled)
Markers	off
Reference level	0 dBm in power-on units
Reference level offset	$107~\mathrm{dB}\mu\mathrm{V}$
Reference level position	top (8th graticule)
Resolution bandwidth	3 MHz (coupled)
Scale	log 10dB/div
Span	6.5 GHz
Start Frequency	0 Hz
Stop Frequency	6.5 GHz
State registers 1—8	unaffected
Sweep	continuous
Sweep time	130 ms (auto-coupled)
Threshold	off
Trace A	clear write
Trace B	store-blank
Trace C	store-blank
Trace math	cleared
Trace registers	unaffected
Trigger	free
Video averaging	off
Video bandwidth	1 MHz (coupled)

Key Path

 $\begin{tabular}{ll} \hline \texttt{MODE} \end{tabular} \begin{tabular}{ll} \verb+PRESET \end{tabular} \begin{tabular}{ll} \verb+SPECTRUM+ & when the instrument mode of operation is \\ \hline \end{tabular}$ receiver and the MODE hardkey is pressed twice.

Related Programming Command

Print Config

Softkey that accesses a menu used to address the printer, select a black and white print or a color print (a color print requires either an HP PaintJet, HP DeskJet 500C, or HP DeskJet 550C printer), and reset the printer. See the (COPY) key for more information.

Key Path

Print (CONFIG) Config

Related Programming Command

none

Print Options

Softkey that accesses a menu of print options such as; prints per page, low or high resolution, and color or black and white prints.

Key Path

Print Print (CONFIG) Config Options

Related Programming Command

none

PRINTER ADDRESS

Softkey that changes the HP-IB address of the printer. The printer address is set to 1 by pressing DEFAULT CONFIG.

Key Path

Print PRINTER (CONFIG) Config ADDRESS

Related Programming Command

PRNTADRS

PRINTER SETUP

Softkey that resets the printer, sets the printer to 60 lines per page, and skips line perforations. This function enables you to obtain up to two printouts per page. The printer paper should be at the top of the form before using this function.

Key Path

Print PRINTER (CONFIG) Config SETUP

Related Programming Command

none

Printer Туре

Softkey that access a menu to specify what type of printer is connected to the output port.

Key Path

Print Printer (CONFIG) Config Type

Related Programming Command

PRNTTYPE

PROTECT ON OFF

Softkey that selects whether files on a floppy disk can be silently overwritten in the event that a file by the same name already exists on the medium.

When ON is underlined, an error message will appear if you try to overwrite a file that already exists.

Key Path

PROTECT Disk (CONFIG) Config ON OFF

Related Programming Command

PROTECT

PRN/PG 1 2

Softkey that specifies the number of prints per page for printing.

Note

On some printers 1 print per page will generate a full page printout, other printers are unaffected by the prints per page setting.

Key Path

Print Print PRN/PG Config Options (CONFIG) 1 2

Related Programming Command

PRNTPPG

PRT MENU ON OFF

Softkey that allows the softkey labels to be printed along with the display. This function operates when the (COPY) key is used in a print configuration. The print menu function is set to ON when DEFAULT CONFIG is pressed.

Key Path

	PRT MENII
	ON OTTO

Related Programming Command

none

pTesla

Softkey that selects pTesla as the transducer conversion units for the antenna amplitude-correction factors.

Key Path

	Moreo	Α,	atn	Antonno	CATA	Moro
			711 EC 011	Hilbeillia	ED L 1	HULT
(SETUP) 1 of	3 F	actors	Factors	ANTENNA	1 of 2
Ant∈	nna					
Unit	s p	Tesla				

Related Programming Command

XUNITS

PURGE LIMITS

Signal analysis mode only.

Softkey that clears the current limit-line table from internal memory. Pressing PURGE LIMITS displays the message: If you are sure, press key again to purge data. Press PURGE LIMITS again if you wish to clear the current limit-line table. Press SAVE LIMIT to save the current limit-line table, and then press PURGE LIMITS to clear the current limit-line table.

Key Path

More Limit Edit (DISPLAY) 1 of 2 Lines Limit	More PURGE* 1 of 2 LIMITS
More Limit Edit (SETUP) 1 of 3 Lines Limit	More PURGE * 1 of 2 LIMITS

^{*} Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

Related Programming Command

LIMIDEL

PWR SWP ON OFF

This softkey is only available when LIN is selected for the SWEEP LOG LIN softkey.

Softkey that activates (ON) or deactivates (OFF) the power-sweep function, which sweeps the output power of the tracking generator over the selected power-sweep range. The value of the power-sweep range is displayed in the active-function block when PWR SWP ON OFF is turned on. The available power-sweep range is a function of the source attenuator setting: For power sweeps, press SRC ATN MAN AUTO until (MAN) is underlined so the instrument source attenuator is manually set (decoupled).

For a given source attenuation setting, the maximum specified power-sweep range is shown in Table 4-10.

Table 4-10.

Attenuator Setting	Power Sweep Range
0 d B	-1 to -10
8 dB	-10.1 to -18
16 dB	-18.1 to -26
24 dB	-26.1 to -34
$32~\mathrm{dB}$	-34.1 to -42
40 dB	-42.1 to -50
48 dB	−50.1 to −58
56 dB	-58.1 to -66

The output power of the tracking generator is swept with the sweep voltage of the instrument. The output power is always swept from the source power setting to a higher power setting (negative source power sweep values are not allowed). Refer to the calibration guide for your instrument for more information regarding source power and source attenuation relationships.

Power-sweep measurements are particularly useful in making gain compression measurements or output power versus frequency measurements.

Key Path

PWR SWP TRACK GEN ON OFF

Related Programming Command

SRCPSWP

QP/AVG 10X OFF

This key is only active if either (QUASI-PEAK) or (AVERAGE) is used first.

Softkey that turns off the linear 10X gain stage in the quasi-peak and average detector signal path.

Key Path

		More	OP/AVG
	More		
	1 4 9	2 of 3	10X OFF


Related Programming Command

QPGAIN

QP DET ON OFF

Softkey that turns the quasi-peak detector on and off. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

none

QP DWELL TIME

Softkey that sets the measurement time when the quasi-peak detector is measured. This key is used in conjunction with MEASURE AT MKR, RE-measure, AUTO-MEASURE, and MEAS STEPPED.

Key Path

			OD DURT
MATA		Meagnre	
	nst		
		Detector	TIME


Related Programming Command

MEASTIMEQPD

QP GAIN ON OFF

Softkey that amplifies the video signal ten times (20 dB). This is a service diagnostic function and is for service use only.

Key Path




Related Programming Command

none

QPD OFFSET

Softkey that sets the offset of the quasi-peak detector. This is a service diagnostic function and is for service use only.

Key Path




Related Programming Command

none

QPD RST ON OFF

Softkey that discharges and resets the quasi-peak detector. This is a service diagnostic function and is for service use only.

Key Path



Related Programming Command

QUASI-PEAK

Hardkey that toggles the quasi-peak detector on and off. When on, the instrument is placed in linear amplitude detection, the detector is turned on, and the system settings are optimized to accurately measure the quasi-peak amplitudes.

Related Programming Command

none

QUIETJET

Softkey that specifies QuietJet as the printer connected to the output port.

Key Path

	Printer		
	Type		QUIETJET

Related Programming Command

none

(RECALL)

Hardkey that accesses softkey menus that allow you to recall data from the floppy disk or internal memory. When Recall Internal is selected, states, traces, and limit-line tables can be recalled from internal memory. When Recall Disk is selected, states, traces, limit-line tables, and amplitude-correction factors, display images, setups, and lists can be recalled from the floppy disk.

In addition, pressing (RECALL) accesses the cataloging functions used to catalog the saved data that is in internal memory or on the floppy disk.

Related Programming Command

SAVRCLF

RECALL ANTENNA

Softkey that recalls antenna-correction factors from a floppy disk. To recall antenna-correction data press, RECALL ANTENNA use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path

	Recall	R.F.C.A.I.I.
(RECALL)	Disk	ANTENNA

Related Programming Command

AMPCOR

RECALL CABLE

Softkey that recalls cable-correction factors from a floppy disk. To recall cable factors press, RECALL CABLE use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path

Related Programming Command

AMPCOR

RECALL COLORS

Softkey that recalls previously saved display palettes (the color definitions for the features on the display) from the recall number specified. To recall a display palette press, RECALL COLORS the message RECALL COLOR (1-4) will be display on the top left-hand side of the display. Use the data keys to select the desired recall register.

Key Path

			RECATI
	IIISDIAV	LOTIET	
IDISPLAVI	f contract	$(\alpha \mid \alpha r)$	COLORS

Related Programming Command

RCLC

Recall Disk

Softkey that accesses a menu to recall instrument setups, signals lists, states, traces, display images, limit-line tables, and amplitude-correction factors from a floppy disk.

Key Path

Recall (RECALL) Disk

Related Programming Command

Recall Internal

Softkey that accesses a menu to recall states, traces, and limit-line tables from internal memory.

Key Path

Recall (RECALL) Internal

Related Programming Command

none

RECALL LIMITS

Softkey that recalls limit-line tables from a floppy disk. To recall a limit-line table press, RECALL LIMITS use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path

(DISPLAY)	More	Limit	RECALL
	1 of 2	Lines	LIMITS
(RECALL)	Recall Disk	RECALL LIMITS	
(SETUP)	More	Limit	RECALL
	1 of 3	Lines	LIMITS

Related Programming Command

none

RECALL LIST

Softkey that recalls signal lists from a floppy disk. To recall a signal list press, RECALL LIST use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path

RECALI	Recall Disk	RECALL LIST	
(TEST)	1 of 3	Save/Rcl	RECALL LIST

Related Programming Command

RECALL OTHER

Softkey that recalls other two-port device factors from a floppy disk. To recall other data press, RECALL OTHER use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path

(RECALL)	Recall Disk	More 1 of 2	RECALL OTHER	
(SETUP)	More 1 of 3	Correctr Factors	ı Other	RECALI

Related Programming Command

AMPCOR

RECALL SETUP

Softkey that recalls instrument setups from a floppy disk. To recall an instrument setup press, RECALL SETUP use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path

RECALL	Recall Disk	RECALL SETUP
[SETUP]	Recall Setup	

Related Programming Command

none

RECALL TRACE

Softkey that recalls traces from a floppy disk. To recall a trace press, RECALL TRACE use the step keys or knob to highlight the desired file, then press LOAD FILE.

Key Path


	VATA	
		TRACE

Related Programming Command

RECEIVER ADDRESS

Softkey that allows you to set the HP-IB address of the instrument. The address is set to 18 by pressing DEFAULT CONFIG.

Key Path



Related Programming Command

none

RED

Softkey that changes the intensity of the red portion of the primary light source output for the display annotation, trace, graticule, and so

Key Path

	111511111		

Related Programming Command

none

RED FILL

Softkey that replaces the standard display screen with a red box. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

Key Path

		WIES F C	
- DIOPIG			
-1	Dattama		

Related Programming Command

none

REF LVL

Softkey that allows the reference level to be changed. This function is activated when (AMPLITUDE) is pressed. The reference level is the amplitude power or voltage represented by the top graticule line on the screen. Changing the value of the reference level changes the absolute amplitude level (in $dB\mu V$) of the top graticule line. The reference level can be changed using the data keys, knob, or step keys.

Key Path

REF LVL (AMPLITUDE)

Related Programming Command

RL

REF LVL OFFSET

Softkey that adds an offset value to the displayed reference level. Offsets are entered by using the data keys. Entering an offset does not affect the trace or the attenuation value. Reference-level offsets are used when gain or loss occurs between a device under test and the instrument input. Thus, the signal level measured by the instrument is the level at the input of an external amplitude-conversion device. When an amplitude offset is entered, its value is displayed on the top left-side of the screen. To eliminate an offset, press REF LVL OFFSET, 0 (-dBm) or (+dBm). Pressing (PRESET) also sets the offset to zero. See also the EXTERNAL PREAMPG softkey description.

Key Path

		More	REF LVI.
	IIVL	11016	IVLIL LIVL
	4 -2 0	0 -4 0	OFFCET
TAMPLITUDEL		2 OI 3	UFFSEI

Related Programming Command

ROFFSET

REMEAS ALL SIGS

Softkey that remeasures all signals in the signal list. To remeasure each signal the algorithm spans down on the signal using the initial frequency listed in the table. When zero span is reached, up to three detectors can be used to measure the signal. These detectors are selected using DETECTOR PK QP AV.

Key Path

			T.P.M.P.A.S
	The second secon		
		maagura	

Related Programming Command

REMEASSIG

REMEAS MARKED

Softkey that remeasures marked signals in the signal list. To remeasure each signal the algorithm spans down on the signal using the initial frequency listed in the table. When zero span is reached, up to three detectors can be used to measure the signal. These detectors are selected using DETECTOR PK QP AV.

Key Path

	More	EDIT	Re-	REMEAS
$\overline{}$	4 6 6	TTOO		MADICED
(TEST)	1 01 3	LISI	measure	MARKED

Related Programming Command

REMEASSIG

REMEAS SIGNAL

Softkey that remeasures the signal specified in the signal list. To remeasure each signal the algorithm spans down on the signal using the initial frequency listed in the table. When zero span is reached, up to three detectors can be used to measure the signal. These detectors are selected using DETECTOR PK QP AV.

Key Path

	DNTH		DEMINAC
			H H W H U S
		Re-	
More			
1 of 3	TTST		STGMAI
		maagura	

Related Programming Command

REMEASSIG

Remeasure

Softkey that accesses a menu that remeasures one or more signals in the signal list.

Key Path

	More	EDIT	Re-
		TTCT	
LTEST	1 OI 3	LISI	measure

Related Programming Command

REMEASSIG

RESOLUTN LOW HIGH

Softkey that sets the resolution of subsequent prints to low or high resolution. High resolution shows more detail, but takes a longer time to print. Print resolution and print speed will vary with the printer type. Refer to the specific printer manual for more information.

Key Path

			DECOLUTM
(CONFIG)		lintione	TOM HIGH
	('Antig	lintione	

Related Programming Command

PRNTRES

RESTART

Softkey that restarts a stepped measurement. The stepped measurement is taken between the specified start and stop frequencies in conjunction with the selected step size (FREQ STEP), step type (STEP LOG LIN) and step mode (MEAS SNG CONT).

Key Path

TES	More □ 1 of 3	More	MEAS STEPPED	STOP	RESTART
(TES	More 1 of 3	2 of 3	MEAS STEPPED	FREQ STEP	RESTART

Related Programming Command

none

SATUR-ATION

Softkey that changes the saturation (the ratio of pure color mixed with white) of the specified portion of the display annotation.

Key Path

111011211		

Related Programming Command

SETC

SAVE

Hardkey that accesses menus that allow you to store state data, trace data, and limit-line tables in internal memory. The SAVE function also allows you to save instrument setups, state data, trace data, limit-line tables, amplitude-correction factors, signal lists, and display images on the floppy disk. In addition, pressing (SAVE) accesses the menus used to catalog the saved data in internal memory or on the floppy disk.

Saving state data saves the instrument settings, but not the trace data. Saving trace data saves both the trace data and the state data. Display images can only be saved to or recalled from the floppy disk.

States and traces are saved in internal memory even if the instrument is turned off or (PRESET) is pressed. Eight internal state registers and many trace and limit-line registers are available for the user. The Catalog Internal softkey is used to access the catalog functions.

Related Programming Command

SAVRCLF

SAVE ANTENNA

Softkey that saves antenna amplitude-correction data to a floppy disk. To save antenna data press, SAVE ANTENNA. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The antenna data has now been saved to a disk.

Key Path

	(correctn	Antenna	
	HOCTOTO	HACTORS	ΔΝΤΓΝΝΔ

Related Programming Command

AMPCOR

SAVE CABLE

Softkey that saves cable amplitude-correction data to a floppy disk. To save cable data press, SAVE CABLE. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The cable data has now been saved to a disk.

Key Path

AMPCOR

SAVE COLORS

Softkey that saves a display palette (the color definitions for the features on the display) to the save number specified. To save a display palette press, SAVE COLORS the message SAVE COLORS (1-4) will be displayed at the top left-hand side of the display. Use the data keys to select the desired register to save to.

Key Path

Display Adiust SAVE	
THE STATE ACTION AND	
Dioping ingluor bird	
.	
(DISPLAY) Config Color COLOR	0.00
IDISPLAYI CONTIG COLOR CILLUR	-
(Didi Erri) Odisa and Odisa	

Related Programming Command

SAVEC

Save Disk

Softkey that accesses a menu to save instrument setups, signals lists, states, traces, display images, limit-line tables, and amplitude-correction factors to a floppy disk.

Key Path

Save Disk (SAVE)

Related Programming Command

none

SAVE EDIT

Softkey that passes the text from the DLP editor memory through the parser to execute as instrument commands. If the text (commands) is a valid user-defined function, it passes through the parser and into the instrument user memory. It will replace an existing user defined function of the same name.

RECALL Recall Catalog Internal		*	
Save Catalog (SAVE) Internal Internal .	*	Editor	SAVE EDIT

^{*} Any of the following can be used to complete the key path: CATALOG ALL, CATALOG VARIABLS, or CATALOG PREFIX.

none

Save Internal

Softkey that accesses a menu to save states, traces, and limit-line tables to internal instrument memory.

Key Path

Save SAVE Internal

Related Programming Command

none

SAVE LIMITS

Softkey that saves the current limit-line table to a floppy disk. To save a limit-line table press, SAVE LIMITS. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The limit-line table has now been saved to a disk.

Key Path

DISPLAY	More 1 of 2		SAVE LIMITS
(SETUP)	More 1 of 3	Limit Lines	SAVE

Related Programming Command

none

SAVE LIN GRAPH

Softkey that draws an EMI report graph on the display. SAVE LIN GRAPH draws a full-screen graticule, linear frequency-axis with limited annotation. Drop lines for peak amplitude signals with cross-bars for quasi-peak and average amplitude readings are drawn on the graticule. The quasi-peak cross-bar is the same color as trace B (default is blue) and the average cross-bar is the same color as trace C (default is magenta). The start and stop frequencies are defined based on the frequencies in the signal list.

More	Save/Rcl	SAVE LIN
	List	GRAPH

SIGGRAPH

SAVE LIST

Softkey that saves the current signal list to a floppy disk. To save a signal list press, SAVE LIST. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The signal list has now been saved to a disk.

CAUTION

When saving internal data and signal lists are displayed, disk warning messages do not appear. Therefore it is recommended that you verify that a file has been saved before clearing the data from your display.

For example, before saving signal list data, make sure that your disk is *not* write protected. To verify that the file was saved, press RECALL LIST to catalog signal lists that have been saved to the disk, then check that the correct file was saved by inspecting the file name, date, and time stamp.

Key Path

	~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~~	

## **Related Programming Command**

none

# SAVE LOG GRAPH

Softkey that draws an EMI report graph on the display. SAVE LOG GRAPH draws a full-screen graticule, logarithmic frequency-axis with limited annotation. Drop lines for peak amplitude signals with cross-bars for quasi-peak and average amplitude readings are drawn on the graticule. The quasi-peak cross-bar is the same color as trace B (default is blue) and the average cross-bar is the same color as trace C (default is magenta). The start and stop frequencies are defined based on the frequencies in the signal list.

#### **Key Path**

		CAUTION
WATER A TOTAL CONTRACTOR OF THE PARTY OF THE		
	\2WQ/HC	
MOTA		
		CDADU

# **Related Programming Command**

**SIGGRAPH** 

# SAVE OTHER

Softkey that saves other two-port amplitude-correction factors to a floppy disk. To save *other* amplitude-correction factors press, SAVE OTHER. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. Other two-port amplitude-correction data has now been saved to a disk.

#### **Key Path**

		$\cdots$	
	OOLLOUII		kerikarikarikarikarikari
		HACTORS	

## **Related Programming Command**

AMPCOR

# Save/Rcl List

Softkey that accesses a menu used to save and recall signal lists. Save/Rcl List also draws report graphs on the display.

## **Key Path**

	More	
		Save/Rcl

## **Related Programming Command**

none

# SAVE SETUP

Softkey that saves the current setup to a floppy disk. To save a setup press, SAVE SETUP. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number then press (ENTER). The message Saving to :FILENAME is displayed. The setup has now been saved to a disk.

#### **Key Path**

		01	re			A	۷E
(SETUP)	1		١ſ		S	E	${ t TUP}$

## **Related Programming Command**

SAV LOCK ON OFF

Softkey that locks all the current internal state and trace registers against further data storage, when ON is underlined. With the state and trace memory locked, the STATE -> INTRNL and

Trace -> Intrn1 softkey functions are no longer accessible; the MEM LOCKED softkey function is displayed instead. Pressing DEFAULT CONFIG or (PRESET) sets SAV LOCK ON OFF to OFF.

Note

When SAV LOCK ON OFF is set to ON, none of the state registers can be overwritten, including state register nine. The instrument automatically updates state register nine with the last state unless the save lock function is on.

#### **Key Path**

Save SAV LOCK SAVE Internal ON OFF

#### **Related Programming Command**

**PSTATE** 

# SCALE LOG LIN

Softkey that scales the vertical graticule divisions in logarithmic units when LOG is underlined. When LOG is the active function, the logarithmic units per division can be changed. Values may range from 0.1 to 20 dB per division. When LIN is underlined, the vertical scale is in linear mode which has a range of 1 kW to 1 pW. The reference-level value is set to the top of the screen and the bottom graticule becomes zero volts. (Each division of the graticule is one-eighth of the reference level in volts.)

Pressing SCALE LOG LIN always sets the units specified for the current amplitude scale. Pressing (PRESET) or powering on the instrument sets the default units.

#### **Key Path**

SCALE (AMPLITUDE) LOG LIN

#### **Related Programming Command**

LG, LN

SELECT

Hardkey that directly accesses the menus that selects AM or FM demodulation, FM gain, dwell time, and squelch levels.

#### **Related Programming Command**

none

SELECT 1 2 3 4 Softkey that selects one of the four possible markers. A marker can be turned on once it is selected. A marker that has already been turned on will become active when it is selected. If a marker has already been turned on and assigned to a specific trace it will become active on that trace and the MK TRACE AUTO ABC softkey will have the appropriate trace letter underlined.

## **Key Path**


SELECT 1 2 3 4 (MKR)

#### **Related Programming Command**

MKACT

# SELECT AMPLITUD

Softkey that enters either the amplitude value for the displayed (upper or lower) limit-line segment or the amplitude value for the current amplitude-correction point. Enter the amplitude value for the selected frequency (or time, for signal analysis mode only) by using the data keys. Change an amplitude value by using the step keys or the knob. Press (BK SP) to correct errors.

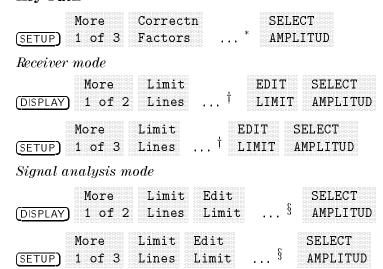

AMPCOR, LIMSEG

# Select Axis

Softkey that accesses a menu which allows the selection of the frequency and the amplitude scales for the limit line to be either logarithmic or linear.

## **Key Path**

More (DISPLAY) 1 of 2	Lines *	EDIT	Select Type	Select Axis
More I	.imit	EDIT :	Select	Select
(SETUP) 1 of 3 I	.ines *		Type	Axis

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

## **Related Programming Command**

none

# SELECT DELT AMP

Softkey that sets the delta amplitude value for a segment of a mid/delta type of limit line. Press (BK SP) to correct errors.

#### **Key Path**

DISPLAY	More ) 1 of 2	Lines	Edit Limit	EDII MID/DELT	SELECT DELT AMP
(SETUP)	More	Limit	Edit	EDIT	SELECT
	1 of 3	Lines	Limit	MID/DELT	DELT AMP

# **Related Programming Command**

^{*} Any of the following group of softkeys can be used to complete the key path: Antenna Factors, EDIT ANTENNA, or Cable Factors, EDIT CABLE or Other Factors, EDIT OTHER.

[†] Either Limit 1 or Limit 2 can be used to complete the key path.

 $[\]S$  – Either EDIT UPPER, or EDIT LOWER can be used to complete the key path.

# SELECT FREQ

Softkey that enters the frequency value for a limit-line segment or for an amplitude-correction point. Enter the frequency value for the frequency by using the data keys. Change the frequency value by using the step keys or the knob. Press (BK SP) to correct errors.

A frequency coordinate must always be specified for either limit lines or amplitude-correction factors.

#### Note

Limit-line data is sorted in frequency order in the limit-line table. The sorting occurs after you have entered the frequency and at least one amplitude value.

For amplitude-correction factors, only two entries with the same frequency are valid. Only the first and last points of a series with the same frequency values are used; the middle points are ignored.

Amplitude-correction data is sorted in the table by frequency. The sorting occurs immediately after you have entered the frequency value via the front panel.

#### **Key Path**

More	Correctn	SELE	CT	
(SETUP) 1 of 3	Factors .	rs * FREQ		
$Receiver\ mode$				
More	Limit	EDIT	SELECT	
(DISPLAY) 1 of	2 Lines	† LIMIT	FREQ	
More	Limit .	EDIT	SELECT	
(SETUP) 1 of 3	Lines †	LIMIT	FREQ	
Signal analysis	mode			
More	Limit Edi		SELECT	
(DISPLAY) 1 of	2 Lines Lim	it§	FREQ	
More	Limit Edit		SELECT	
(SETUP) 1 of 3	Lines Limi	t§	FREQ	

^{*} Any of the following groups of softkeys can be used to complete the key path: Antenna Factors, EDIT ANTENNA, or Cable Factors, EDIT CABLE or Other Factors, EDIT OTHER.

# **Related Programming Command**

AMPCOR, LIMISEG

[†] Either Limit 1 or Limit 2 can be used to complete the key path.

[§] Any of the following keys can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW or EDIT MID/DELT.

# **SELECT** FRM LIST

Softkey that controls the cursor position in the signal list.

## **Key Path**

	More	SELEC	T	
(TEST)	1 of 3	FRM L		
	More	EDIT	SELECT	
TEST	1 of 3	LIST	FRM LIST	
	More	EDIT	Sort	SELECT
TEST	1 of 3	LIST	Signals	FRM LIST
	More	EDIT	Delete	SELECT
(TEST)	1 of 3	LIST	Signals	FRM LIST

#### **Related Programming Command**

**SIGPOS** 

# SELECT LWR AMPL

Signal analysis mode only.

Softkey that enters the amplitude value for the lower limit-line segment. Enter the amplitude value for the selected frequency or time by using the knob or data keys. Press (BK SP) to correct errors.

# **Key Path**

( <u>DISPLAY</u>	More 7) 1 of 2	Limit Lines	Edit Limit	EDIT UP/LOW	SELECT LWR AMPL
(SETUP)	More	Limit	Edit	EDIT	SELECT
	1 of 3	Lines	Limit	UP/LOW	LWR AMPL

## **Related Programming Command**

none

# SELECT MID AMPL

Signal analysis mode only.

Softkey that enters the amplitude value for the middle of the limit-line segment. Enter the amplitude value for the selected frequency or time by using the knob or data keys. Press (BK SP) to correct errors.

	More	Lımıt	Edit	ED11	SELECT
(DISPLAY	7) 1 of 2	Lines	Limit	M1D1DEL1	MID AMPL
	More	Limit		EDII	SELECT
(SETUP)		Lines	Limit	MIDIDELLI	MID AMPL

none

# SELECT POINT

Softkey that creates or edits an amplitude-correction factor data point. Enter the point number to be created or edited by using the data keys, then press (ENTER). Press (BK SP) to correct errors.

## **Key Path**


	More	Correctn	Antenna	Edit	SELECT
(SETUP)	1 of 3	Factors	Factors	Antenna	POINT
	More	Correctn	Cable	Edit	SELECT
(SETUP)	1 of 3	Factors	Factors	Cable	POINT
	More	Correctn	Other	Edit	SELECT
(SETUP)	1 of 3	Factors	Factors	Other	POINT

# **Related Programming Command**

**AMPCOR** 

# SELECT PREFIX

Softkey that allows you to select an already existing prefix of a cataloged file and changes the current prefix to this selected prefix. This provides a convenient method for saying and recalling data to and from the floppy disk and for cataloging by the prefix. Use either the knob or step keys to select the file.

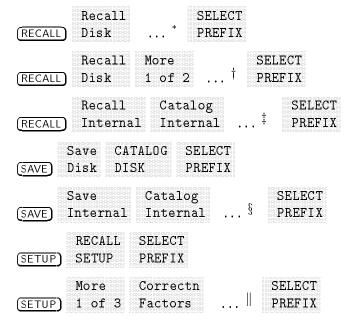

More Save/Rcl RECALL SELECT (TEST) 1 of 3 List LIST PREFIX

Receiver mode

More Limit RECALL SELECT (DISPLAY) 1 of 2 Lines LIMITS PREFIX

- * Any of the following keys can be used to complete the key path: CATALOG DISK, RECALL SETUP, RECALL LIST, RECALL LIMITS, or RECALL ANTENNA.
- † Any of the following keys can be used to complete the key path: RECALL CABLE, RECALL OTHER, or RECALL TRACE.
- ‡ Any of the following keys can be used to complete the key path: CATALOG ALL, CATALOG VARIABLS, or CATALOG PREFIX.
- § Any of the following keys can be used to complete the key path: CATALOG ALL, CATALOG REGISTER, CATALOG VARIABLS or CATALOG PREFIX.
- || Any of the following groups of softkeys can be used to complete the key path: Antenna Factors, EDIT ANTENNA, or Cable Factors, EDIT CABLE or Other Factors, EDIT OTHER.

#### **Related Programming Command**

none

# SELECT SEGMENT

Softkey that creates or edits a limit-line segment. Limit lines are created by entering frequency (or time) and amplitude values into a limit-line table. The frequency (or time, for signal analysis mode only) and amplitude values specify a coordinate point from which a limit-line segment is drawn. The coordinate point is the lowest frequency or time point of the line segment. Limit lines are constructed from left to right. To select a segment, press SELECT SEGMENT, enter the segment number you wish to specify, then press a units key.

Up to 30 segments can be specified per limit-line table.

 $Receiver\ mode$ 

More (DISPLAY) 1 of 2	Limit Lines	*	EDIT LIMIT	SELECT SEGMENT	•
More (DISPLAY) 1 of 2	Limit Lines	*	EDIT LIMIT	More 1 of 2	SELECT SEGMENT

(DISPLAY	More ) 1 of 2	Limit Lines	*	EDIT LIMIT	Select Type	SELECT SEGMENT
	More	Limit	*	EDIT	SELECT	
(SETUP)	1 of 3	Lines		LIMIT	SEGMENT	
	More	Limit		EDIT	More	SELECT
(SETUP)	1 of 3	Lines	*	LIMIT	1 of 2	SEGMENT
	More	Limit		EDIT	Select	SELECT
(SETUP)	1 of 3	Lines	*	LIMIT	Туре	SEGMENT

# **Key Path**

 $Signal\ analysis\ mode$ 

	More	Limit	Edit		SELECT	
(DISPLAY	) 1 of 2	Lines	Limit	⊺	SEGMEN'	<b>I</b>
	More	Limit	Edit		More	SELECT
DISPLAY	) 1 of 2	Lines	Limit	†	1 of 2	SEGMENT
	More	Limit	Edit		SELECT	
(SETUP)	1 of 3	Lines	Limit	†	SEGMENT	
	More	Limit	Edit		More	SELECT
(SETUP)	1 of 3	Lines	Limit	†	1 of 2	SEGMENT

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

## **Related Programming Command**

none

Select Type Softkey that accesses the menu used to select the limit-line type of line. Press FLAT to select a flat line, press SLOPE to select a sloped line, or press POINT to select a point.

# **Key Path**

Receiver mode

(DISPLAY) 1 of 2	Limit Lines	*	EDIT LIMIT	Select Type
More (SETUP) 1 of 3	Limit Lines	*	EDIT LIMIT	Select Type

Signal analysis mode

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

DISPLAY		Limit Lines	Edit Limit	†	Select Type
(SETUP)	More 1 of 3	Limit Lines	LULU Limit	†	Select Type

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

none

# SELECT UPR AMPL

Signal Analysis mode only.

Softkey that enters the amplitude value for the upper limit-line segment. Enter the amplitude value for the selected frequency or time by using the knob or data keys. Press (BK SP) to correct errors.

# **Key Path**

(DISPLAY	More 7) 1 of 2	Lines	Edit Limit	UP/LOW	UPR AMPL
(SETUP)	More 1 of 3	Lines	Edit Limit	EDIT UP/LOW	SELECT UPR AMPL

## **Related Programming Command**

none

# Selectv Mark

Softkey that accesses a menu that marks one or more signals on the signal list.

## **Key Path**

	More	TIT	Cional	TT20 TQ2
	TIOLG	LID L	DIEHUI	Detecon
TEST	1 0 9	TTCT	Marking	Mark
[   L ]			HULKINE	L:+ C4-4

# **Related Programming Command**

SIGMARK

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

# Service Cal

Softkey that accesses several service calibration functions. The service calibration functions are designed for service use only.

#### **Key Path**

-1		
	 	······································
( -, -, -, -, -, -, -, -, -, -, -, -, -,		

## **Related Programming Command**

none

# Service Diag

Softkey that accesses several service diagnostic functions. The service diagnostic functions are designed for service use only.

# **Key Path**

	More	
Mara		Service
More		
		Dian
1 O+ 3		

## **Related Programming Command**

none

# SET ATTN ERROR

Softkey that sets the calibration attenuator-error factors (this is not the same as the input attenuator). This is a service calibration function and is for service use only.

## **Key Path**

	MATA	

#### **Related Programming Command**

none

# SET DATE

Softkey that allows you to set the date of the real-time clock. To enter the date in the YYMMDD format use the data keys then press (ENTER). Valid year (YY) values are 00 through 99. Valid month (MM) values are from 01 to 12, and valid day values are from 01 to 31.

	VIOTO		
		1 7 m $\triangle$	
(2011=10)			TA A CTIT
LCONFIG I		DATA	13. H
$\overline{}$			

SETDATE

# SET TIME

Softkey that allows you to set the time of the real-time clock. To enter the time in 24 hour, HHMMSS format, use the data keys then press (ENTER). Valid hour (HH) values are from 00 to 23. Valid minute (MM) and second (SS) values are from 00 to 59.

#### **Key Path**

(CONFIG)	More Time SE 1 of 3 Date TI	ET EME
(CALIBRA	Cal At SET  Time TIME	

## **Related Programming Command**

CALTIME, SETTIME

# SETTINGS ON OFF

Softkey that turns on or off the generation of a tabular listing of current instrument settings. The listing will be sent to the printer when OUTPUT REPORT is executed.

#### **Key Path**

	Define	SETTINGS
(OUTPUT)	Report	ON OFF
(001101)		

### **Related Programming Command**

none

(SETUP)

Hardkey that accesses softkey functions that control the receiver settings to be used in a measurement, such as frequency range, antenna correction factors, and limit lines.

## **Related Programming Command**

**SETUP** -> DISK

Softkey that stores the settings of the instrument to the disk. This includes: windows and the states associated with them, limit lines, correction factors, and other settings.

#### **Key Path**

Save SETUP Disk -> DISK (SAVE)

#### **Related Programming Command**

none

# SHOW Δ1 PK QP AV

Softkey that specifies that any or all of the following are included in the list portion of the report: peak detector delta from limit 1, quasi-peak detector delta from limit 1, or average detector delta from limit 1.

#### **Key Path**

Define SHOW ∆1 PK QP AV (OUTPUT) List

## **Related Programming Command**

**TBLDEF** 

SHOW  $\Delta 2$ PK QP AV Softkey that specifies that any or all of the following are included in the list portion of the report: peak detector delta from limit 2, quasi-peak detector delta from limit 2, or average detector delta from limit 2.

#### **Key Path**

Define SHOW A2 List (OUTPUT) PK QP AV

## **Related Programming Command**

**TBLDEF** 

# SHOW COR ON OFF

Softkey that specifies the total correction factors are included as part of the list portion of the report. The listing is sent to the printer upon receipt of an OUTPUT REPORT.

#### **Key Path**

	Define	SHOW COR
(OUTPUT)	List	ON OFF

## **Related Programming Command**

**TBLDEF** 

# SHOW DET PK QP AV

Softkey that specifies that any or all of the following are included in the list portion of the report: the peak detector, quasi-peak detector, and the average detector. The listing is sent to the printer upon receipt of an OUTPUT REPORT.

## **Key Path**

	Define	SHOW DET
(OUTPUT)	List	PK QP AV

#### **Related Programming Command**

**TBLDEF** 

# SHOW MKR ON OFF

Softkey that specifies signals that are marked in the signal list will be included as part of the list portion of the report.

## **Key Path**

	Define	SHOW MKR
(OUTPUT)	List	ON OFF

## **Related Programming Command**

**TBLDEF** 

# SHOW SETUP

Softkey that shows current settings of the instrument on the display. SHOW SETUP consists of four pages of information, including existing filenames, correction-factor data, limit-line data, frequency settings, trace data, and so on. To access each succeeding page of information press NEXT PAGE. To exit, press Previous Menu.

#### **Key Path**

		M	o	r	9			Ş	ЗΗ	01	πĪ	
(SETUP)	333		1		31	•	3		ŀΕ	T	11-	3

#### **Related Programming Command**

**SHOWSETUP** 

# SHW INST CONFIG

Softkey that displays information about the configuration of the instrument including; model number, serial number, and the firmware revision date. Also included are the specific devices installed; HP-IB interface, RS-232 interface, tracking generator (TG), quasi-peak detector (QPD), FM demodulator (Demod), precision frequency reference (oven), narrow bandwidths (NBW), and additional information about the disk drive (DISK).

#### **Key Path**

Γ
L
100

#### **Related Programming Command**

HAVE, ID, REF, SER

# SIG LIST ON OFF

Softkey that turns on or off the signal list viewing and editing functions.

#### **Key Path**

		CTC TTCT
	More	
$(\overline{z} = \overline{z} = \overline{z})$		OM OFF
1 1 4 5 1 1		

## **Related Programming Command**

SIGLIST

# SIGNAL ANALYSIS

Softkey that configures the instrument as a signal analyzer.

# **Key Path**

SIGNAL (MODE) ANALYSIS

#### **Related Programming Command**

none

# Signal Marking

Softkey that accesses a menu to mark one or more signal on the signal list.

## **Key Path**

Signal More EDIT LIST Marking 1 of 3 (TEST)

#### **Related Programming Command**

**SIGMARK** 

(SINGLE)

Hardkey that initiates a sweep when in single-sweep mode.

## **Related Programming Command**


none

## SLOPE

Softkey that draws a straight line between the coordinate point of the current segment and the coordinate point of the next segment, producing limit-line values for all frequencies between the two points.

### **Key Path**

Receiver mode

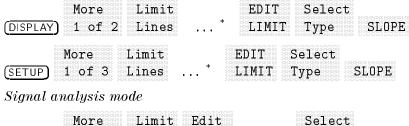

(DISPLAY	More  1 of 2	Limit Lines	Edit Limit		Select Type	SLOPE
(SETUP)	More 1 of 3	Limit Lines	Edit Limit	†	Туре	SLOPE

none

## SOFTKEYS

Softkey that activates the softkey portion of the display screen for color editing.

#### **Key Path**

	Display	Adjust	Edit	More	More	
(DISPLAY)	Config	Color	Colors	1 of 3	2 of 3	
SOFTKEYS						

#### **Related Programming Command**

SETC

# SORT BY AVG AMP

Softkey that sorts the internal signal list by average amplitude. This list is sorted in descending order.

# **Key Path**

		AADA DA
		A T T T T A A A A T T
		A 11 ( A 14) L

#### **Related Programming Command**

SIGSORT

# SORT BY FREQ

Softkey that sorts the internal signal list by the frequency of the signals. The list will be sorted in ascending order.

#### **Key Path**

	TYPYTOT	CODT DV
MATA		
	T T / T	 PRFO

# **Related Programming Command**

SIGSORT

^{*} Either Limit 1 or Limit 2 can be used to complete the key path.

[†] Any of the following can be used to complete the key path: EDIT UPPER, EDIT LOWER, EDIT UP/LOW, or EDIT MID/DELT.

# SORT BY DLTA LIM

This key is only active when VIEW  $\Delta$  OFF is pressed first.

Softkey that sorts the internal signal list by delta limits. The list will be sorted in descending order.

#### **Key Path**

	Mara		

## **Related Programming Command**

SIGSORT

# SORT BY PK AMP

Softkey that sorts the internal signal list by peak amplitude. The list will be sorted by descending order.

## **Key Path**

	The second secon	CODT DV
More		
		 PK AMP

#### **Related Programming Command**

SIGSORT

# SORT BY QP AMP

Softkey that sorts the internal signal list by quasi-peak amplitude. The list will be sorted by descending order,

# **Key Path**

More EDIT Sort SORT BY (TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
(TEST) 1 of 3 LIST Signals QP AMP			
[TEST] 1 of 3 LIST Signals UP AMP			
TEST 1 OT 3 LIST SIGNALS UP AMP			
ES     1 O1 3 LIST SIGNAIS WE AME			
ES     1 O1 3 LIST SIGNAIS WE AME			
[3   1 Of O DIDI DIRIGIO WI HII			
[3   I OI O LIDI DIRIGIO WI RIII			
ILDII TOTO DIDI DIRIGID WI MIII			

## **Related Programming Command**

SIGSORT

# Sort Signals

Softkey that accesses a menu to sort the internal signal list based on the softkey selected. Softkeys available are:

- SORT BY FREQ
- SORT BY PK AMP
- SORT BY QP AMP
- SORT BY AVG AMP
- SORT BY DLTA LIM

SORT BY DLTA LIM is only available when VIEW  $\Delta$  OFF is pressed.

## **Key Path**

	TOTAL TOTAL	
Mora		
		~ 1 mm a l d

## **Related Programming Command**

SIGSORT

SPAN (SPAN) or

Hardkey and softkey that activates the SPAN function and accesses the frequency-span functions. Pressing SPAN allows the user to change the frequency range symmetrically about the center frequency. The frequency-span readout describes the total displayed frequency range; to determine frequency span per horizontal graticule division, divide the frequency span by 10.

#### **Key Path**

SPAN (SPAN)

#### **Related Programming Command**

SP

SPAN ZOOM Softkey that finds the highest signal peak onscreen. If a marker is not already on the peak, it places a marker on it, turns on the marker-track function, and activates the span function. Pressing SPAN ZOOM performs the routine similar to pressing the following keys: (PEAK SEARCH), (MARKER FUNCTION), MK TRACK ON OFF (ON), and (SPAN).

#### **Key Path**

SPAN (SPAN) ZOOM

#### **Related Programming Command**

SPZOOM

SPEAKER ON OFF

Softkey that turns the internal speaker on and off. The volume from the speaker is controlled by the front-panel volume control knob and FM GAIN (when using FM demodulation). There is no output from the speaker unless demodulation is turned on. Pressing (PRESET) sets SPEAKER ON OFF to ON.

#### **Key Path**

SPEAKER ON OFF (SELECT)

## **Related Programming Command**

SPEAKER

# Special Colors

Softkey that accesses a menu of predefined color schemes designed to enhance viewing under specific situations. These color schemes are Monochrome, Vision Enhance 1 and 2 (for two types of deficeint blindness), and Optical Filter (to accommodate the use of protective goggles when viewing lasers).

#### **Key Path**

Display Adjust Special (DISPLAY) Config Colors Colors		
Display Adjust Special (DISPLAY) Config Colors Colors		
Display Adjust Special (DISPLAY) Config Colors Colors		
Display Adjust Special (DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISPLAY) Config Colors Colors		
(DISTERNI) CONTERN COTOLD COTOLD		

## **Related Programming Commands**

SETC

# SQUELCH

Softkey that adjusts the squelch level. The squelch level mutes weak signals and passes strong signals. The squelch level affects the audio output only. If the internal speaker is on, audio signals are not output unless the signal strength exceeds the squelch threshold. The squelch level does not affect the rear-panel AUX VIDEO OUT signal. Squelch level is indicated onscreen by the unitless numbers 0 to 100, with 0 being minimum squelch threshold (all signals are passed), and 100 being maximum squelch threshold (no signals are passed). The default squelch value is 0.

#### **Key Path**

SELECT SQUELCH

#### **Related Programming Command**

**SQLCH** 

# SRC ATN MAN AUTO

Softkey that allows you to select between automatic and manual adjustment of the tracking generator's switching attenuator. It can be manually adjusted from 0 to 56 dB in 8 dB steps. When auto-coupled, the SRC ATN function automatically adjusts the attenuator to yield the source amplitude level specified by the SRC PWR ON OFF softkey function. Set SRC ATN MAN AUTO so that MAN is underlined (decoupled) for power sweeps greater than 8 dB.

#### **Key Path**

SRC ATN (TRACK GEN) MAN AUTO

#### **Related Programming Command**

SRCAT

# SRC PWR OFFSET

Softkey that offsets the displayed power of the tracking generator (SRC). Offset values may range from -327 dB to +327 dB.

Using the source-power-offset capability of the tracking generator allows you to take system losses or gains into account, thereby displaying the actual power delivered to the device under test.

#### **Key Path**

More SRC PWR 1 of 2 OFFSET TRACK GEN

## **Related Programming Command**

**SRCPOFS** 

# SRC PWR ON OFF

Softkey that activates (ON) or deactivates (OFF) the output power of the tracking generator (SRC). The power level can then be adjusted using the data keys, step keys, or knob.

#### **Key Path**

SRC PWR (TRACK GEN) ON OFF

#### **Related Programming Command**

SRCPWR

SRC PWR STP SIZE

Softkey that sets the step size of the source-power level, source-power offset, and power-sweep range functions. The step size may be values from -327 dB to 327 dB. The default setting is one vertical scale division.

#### **Key Path**

	More	SRC PWR
TRACK GEN	) 1 of 2	STP SIZE

## **Related Programming Command**

SRCPSTP

# START FREQ

Softkey that sets the frequency at the left side of the graticule. The left and right sides of the graticule correspond to the start and stop frequencies. When these frequencies are activated, their values are displayed below the graticule in place of center frequency and span.

## **Key Path**

START (FREQUENCY) FREQ

#### **Related Programming Command**

FA

# STATE -> INTRNL

Softkey that saves the current instrument state in the selected state register. To save the current state, press STATE -> INTRNL, and use the data keys to enter a state register number (valid state register numbers are 1 through 8). If windows are being used, only the state of the active window will be saved.

# **Key Path**

	Save	
		-> TNTRNI.
(CAVE)	Internal	
		> INTRA

#### **Related Programming Command**

SAVES

## STATUS

Softkey that activates the status portion of the display screen for color editing.

## **Key Path**

	Display	H'ATT		
		(1.44.40		
		 Colors		 CONTRACTOR
			1 of 3	

## **Related Programming Command**

SETC

# STEP LOG LIN

Softkey that initiates a logarithmic or linear stepped measurement. The stepped measurement is taken between the specified start and stop frequencies in conjunction with the selected step size (FREQ STEP), and step mode (MEAS SNG CONT). The parameter specified is multiplied by the intermediate frequency bandwidth to determine the actual step size.

#### **Key Path**

	More		<del></del>
	Vara	Vara	
		**************************************	
			TOC ITM
		- AT	

## **Related Programming Command**

none

## STOP

Softkey that stops a stepped measurement.

#### **Key Path**

	More	More		
			LLIFL	
			ammonno	~~~~
TEST	1 1 01 3	ンロエコ	S [ H.P P H.I )	
1 1 2 1				

#### **Related Programming Command**

none

# STOP FREQ

Softkey that sets the frequency at the right side of the graticule. The left and right sides of the graticule correspond to the start and stop frequencies. When these frequencies are activated, their values are displayed below the graticule in place of center frequency and span.

## **Key Path**

STOP (FREQUENCY) FREQ

FΒ

# STORE FLATNESS

This key is only active when either EDIT FLATNESS or EDIT PA FLATNESS are pressed first.

Softkey that stores amplitude versus frequency calibration factors.

## **Key Path**

Mara	Mara	Service	Hilathogg	
MOLE		DETATOR	TTGLIESS	
				TTATMECO

# **Related Programming Commands**

none

# STOR PWR ON UNITS

Softkey that sets the default settings for the units used in the linear and the logarithmic modes when the instrument is powered on. The settings for the units can be changed during normal instrument operation but they will return to the default settings when the instrument is powered on again. This is a service calibration function.

## **Key Path**

	More	More	Service	STOR PWR
(CALIBRATE)	1 of 3	2 of 3	Cal	ON UNITS

#### **Related Programming Command**

none

# STP GAIN ZERO

Softkey that disables the two 20 dB step-gain amplifiers on the A12 amplitude control assembly. This is a service diagnostic function and is for service use only.

#### **Key Path**

	10 10 10 10 10 10 10 10 10 10 10 10 10 1	

## **Related Programming Command**

## STUVWX

Softkey that accesses the menu used for selecting screen title or prefix characters S through X.

#### **Key Access**

(CAL), (CONFIG), (DISPLAY), (RECALL), (SAVE), or (SETUP)

## **Related Programming Command**

none

## (SWEEP)

Hardkey that accesses the sweep-time menu and the sweep-time softkey functions SWP TIME AUTO MAN and SWEEP CONT SGL.

## **Related Programming Command**

CONTS

# SWEEP CONT SGL

Softkey that switches the instrument between continuous-sweep mode and single-sweep mode. If the instrument is in single-sweep mode, SGL is underlined. Press (SINGLE) to enable a sweep when in single-sweep mode. When continuous-sweep mode is in use, one sweep follows another as soon as it is triggered. Pressing (PRESET) and turning the power on, selects continuous sweep.

#### **Key Path**

SWEEP (SWEEP) CONT SGL

SWEEP TRIG CONT SGL

## **Related Programming Command**

CONTS, SNGLS

# SWEEP LOG LIN

Softkey that selects between a logarithmic and linear frequency axis.

## **Key Path**

SWEEP (FREQUENCY) LOG LIN


SWEEP (SWEEP) LOG LIN

**SWEEPTYPE** 

# SWEEP RAMP

Softkey that displays the RAMP signal from the sweep-ramp generator that is located on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

#### **Key Path**



## **Related Programming Command**

none

# SWEEP TIME DAC

Softkey that displays the output of the sweep-time DAC (SWP_DAC) from the sweep-ramp generator that is on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

## **Key Path**

(CALIBRATE)	More 1 of 3	2 of 3	Service Diag	More 1	
SWEEP TIME DAC					

## **Related Programming Command**

none

# SWP CPLG SR RECV

Softkey that selects stimulus-response (SR) or receiver (RECV) auto-coupled sweep time. In stimulus-response mode, auto-coupled sweep times are usually much faster for swept-response measurements. Stimulus-response auto-coupled sweep times are typically valid in stimulus-response measurements when the frequency span of the instrument is less than 20 times the bandwidth of the device under test.

(TRACK	GEN)	1 of 2	SR RECV

MEASURE, SWPCPL

# SWP TIME AUTO MAN

Softkey that selects the length of time in which the instrument sweeps the displayed frequency span. In all non-zero frequency spans, the sweep time varies from 20 milliseconds to 100 seconds. In zero frequency span, the fastest sweep time is 15 milliseconds. Reducing the sweep time increases the rate of sweeps. The sweep time can be changed using the step keys, the knob, or the data keys.

## **Key Path**

SWP TIME (AUTO COUPLE) AUTO MAN

SWP TIME (SWEEP) AUTO MAN

#### **Related Programming Command**

ST

(TEST)

Hardkey that provides control for measuring signals and manipulating lists of measured signals.

#### **Related Programming Command**

none

Test Patterns Softkey that accesses a menu consisting of 18 test patterns used for display-troubleshooting and screen-alignment procedures.

#### **Key Path**

Display Test DISPLAY Config Patterns

#### **Related Programming Command**

#### THINKJET

Softkey that specifies ThinkJet as the printer connected to the output port.

#### **Key Path**

## **Related Programming Command**

PRNTTYPE

# THRESHLD ON OFF

Softkey that sets a lower boundary to the active trace. The threshold line "clips" signals that appear below the line when this function is on. The boundary is defined in amplitude units that correspond to its vertical position when compared to the reference level.

The value of the threshold appears in the active-function block and on the lower-left side of the screen. The threshold level does not influence the trace memory or marker position. The peaks found by the markers must be at least the peak-excursion value above the threshold level. The value of the threshold level can be changed using the step keys, the knob, or the data keys. If a threshold is active, press THRESHLD ON OFF until OFF is selected to turn the threshold display off. The threshold value affects peak searching even when the THRESHLD function is set to off.

#### **Key Path**

	More	THRESHLD
(DISPLAY)	1 of 2	ON OFF

#### **Related Programming Command**

ТН

# Time Date

Softkey that accesses the menu used to set and display the real-time clock.

#### **Key Path**

	More	Time
(CONFIG)	1 of 3	Date

## **Related Programming Command**

TIMEDATE

# TIMEDATE ON OFF

Softkey that turns the display of the real-time clock on or off. Pressing DEFAULT CONFIG sets TIMEDATE ON OFF to ON.

Options ON OFF

## **Key Path**

(CONFIG)	More 1 of 3	Time Date	TIMEDATE ON OFF	
	Print	Print	;	1

#### **Related Programming Command**

TIMEDSP

(CONFIG) Config



Hardkey that accesses the trace softkeys that store and manipulate trace information. Each trace is comprised of a series of data points that form a register where amplitude information is stored. The instrument updates the information for any active trace with each sweep. If two traces are being written to, they are updated on alternating sweeps.

#### **Related Programming Command**

none

# TRACE A B C

Softkey that selects the menu used for trace A, trace B, or trace C functions. Press TRACE A B C until the letter of the desired trace is underlined.

## **Key Path**

TRACE (TRACE) A B C

#### **Related Programming Command**


## TRACE A As accessed from (DISPLAY)

Softkey that activates the trace A portion of the display screen for color editing.

As accessed from either (RECALL) or (SAVE).

Softkey that saves trace A data to a floppy disk. To save trace A data press, Trace -> Disk, TRACE A. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number. The message Saving to: FILENAME is displayed. Trace A data has now been saved to a disk.

## **Key Path**

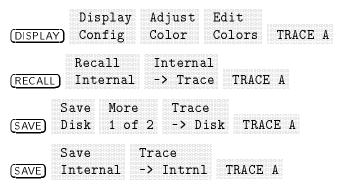

## **Related Programming Command**


SETC

# TRACE B As accessed from (DISPLAY).

Softkey that activates the trace B portion of the display screen for color editing.

As accessed from either (RECALL) or (SAVE).

Softkey that saves trace B data to a floppy disk. To save trace B data press, Trace -> Disk, TRACE B. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number. The message Saving to: FILENAME is displayed. Trace B data has now been saved to a disk.

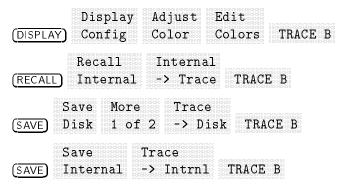

SETC

# TRACE C


As accessed from (DISPLAY).

Softkey that activates the trace C portion of the display screen for color editing.

As accessed from either (RECALL) or (SAVE).

Softkey that saves trace C data to a floppy disk. To save trace C data press, Trace -> Disk, press, Trace -> Disk, TRACE C. REGISTER # and PREFIX= are displayed on the screen. Use the data keys to enter the desired register number. The message Saving to :FILENAME is displayed. Trace C data has now been saved to a disk.

#### **Key Path**

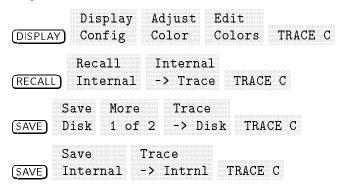

## **Related Programming Command**

SETC

Trace -> Disk

Softkey that accesses a menu to select the item to be stored on a floppy disk: the trace to be saved (trace A, trace B, or trace C), or a limit-line table.

#### **Key Path**

		Save	More	Trace
,				
[	SAVE	Disk	1 OI 2	-> Disk

#### **Related Programming Command**

# Trace -> Intrnl

Softkey that accesses a menu to select the item to be stored in internal memory: the trace to be saved (trace A, trace B, or trace C), or a limit-line table. To save a trace, select the trace to be saved, enter the trace-register number, and press (ENTER). To save a limit-line table press, LIMIT LINES, enter the trace-register number, then press (ENTER). Valid trace-register numbers are 0 through the maximum register number. The maximum register number is the number x displayed after MAX REG # = x during a save or recall operation. If a screen title is present, it is saved with the trace data. The time and date that the trace was stored is appended to the screen title. If windows are being used, only the trace of the active window will be saved.

#### **Key Path**

	Save	Trace
(SAVE)	Internal	_\ Tn+vn1
SAVE	Incernar	_/ III (III I

## **Related Programming Command**

SAVET

TRACK GEN

Hardkey that accesses a menu that controls the built-in tracking generator.

#### **Related Programming Command**

none

TRACKING PEAK

Softkey that activates a routine to adjust the tracking adjustment for the peak response of the tracking generator.

Note

For tracking peak to function properly, the tracking generator must be connected to the instrument.

Before making a stimulus-response measurement, care must be taken to maximize the tracking adjustment of the tracking generator to ensure maximum available dynamic range.

## **Key Path**

TRACKING (TRACK GEN) PEAK

#### **Related Programming Command**

SRCTKPK

TRIG

Hardkey that accesses a menu that selects the sweep mode and trigger mode. (Also see "Screen Annotation" in Chapter 1 of the User's Guide.)

#### Note

With some delayed trigger functions (for example, external or video triggering), the softkey menu is not updated until after the trigger has occurred.

#### **Related Programming Command**

TM

# TUNE SLO FAST

Softkey that makes center frequency the active function and, when FAST is underlined, increases the speed of the marker positioning and center frequency tuning functionality of the knob and step keys.

For marker positioning, the knob changes the marker position by four times the normal rate (FAST).

For center frequency, the knob tuning is eight times the normal rate. (FAST)

#### **Key Path**

TUNE (TEST) SLO FAST

## **Related Programming Command**

**FASTMRKR** 

#### UNDO

Softkey that cancels any changes made in any of the Edit Colors functions.

#### **Key Path**

Display Adjust Special (DISPLAY) Config Colors Colors UNDO

## **Related Programming Command**

VERT LINES

Softkey that replaces the standard display screen with a vertical lines. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

# **Key Path**

DISPIAN	1est .	MOLE	nore	V C.D.I
				TTMTC
	Pattarne			
COLLE	TOPPOTIE			

## **Related Programming Command**

none

User Menus

Softkey that accesses a menu available for your use for user-defined programs and key functions.

# **Key Path**

User Menus (MEAS/USER)

# **Related Programming Command**

**SRCTKPK** 

VID AVG ON OFF

Softkey that initiates a digital averaging routine that averages displayed signals and noise. This function does not affect the sweep time, bandwidth, or other analog characteristics of the instrument. Annotation on the left side of the screen indicates the current number of sweeps averaged. The default number of sweeps is 100. Increasing the number of sweeps smooths the trace. To turn off the video averaging function, press VID AVG ON OFF so that OFF is underlined. The number of sweeps can be entered using the data keys.

# **Key Path**

More VID AVG ON OFF (BW) 1 of 2 More VID AVG 1 of 3 ON OFF (TRACE)

# **Related Programming Command**

VAVG, CLRAVG

# VIDEO

Softkey that activates the trigger condition that allows the next sweep to start if the detected RF envelope voltage rises to a level set by the display line. When VIDEO is pressed, the display line appears on the screen. For example, connect the CAL OUT signal to the instrument input, change the trigger mode to video, and lower the display line. The instrument triggers when the display line reaches the noise floor.

#### **Key Path**

(TRIG) VIDEO

# **Related Programming Command**

TM

# VIEW A OFF

Softkey that accesses a menu to select which delta from the limit-line table is viewed by the display signal list. Each time this softkey is pressed, it changes sequentially as follows:

- VIEW PK ∆ LIM 1
- VIEW PK ∆ LIM 2
- VIEW QP ∆ LIM 1
- VIEW QP ∆ LIM 2
- VIEW AVG ∆ LIM 1
- VIEW AVG ∆ LIM 2
- VIEW ∆ OFF

# **Key Path**

More VIEW A (TEST) 1 of 3 OFF

#### **Related Programming Command**

**SIGDLTAVIEW** 

# VIEW A

Softkey that holds and displays the amplitude data that is in the trace A register. The trace A register is not updated as the instrument sweeps. If trace A is deactivated by pressing STORE BLANK A, the stored data can be retrieved by pressing VIEW A.

#### **Key Path**

(TRACE) VIEW A

# **Related Programming Command**

**VIEW** 

# VIEW B

Softkey that holds and displays the amplitude data that is in the trace B register. The trace B register is not updated as the instrument sweeps. If trace B is deactivated by pressing STORE BLANK B, the stored data can be retrieved by pressing VIEW B.

# **Key Path**

(TRACE) VIEW B

# **Related Programming Command**

**VIEW** 

# VIEW C

Softkey that holds and displays the amplitude data that is in the trace C register. The trace C register is not updated as the instrument sweeps. If trace C is deactivated by pressing STORE BLANK C, the stored data can be retrieved by pressing VIEW C.

## **Key Path**

(TRACE) VIEW C

# **Related Programming Command**

VIEW

# VIEW CAL ON OFF

Softkey that switches the 300 MHz calibrator signal so that it is routed internally to the input of the instrument or externally to the 300 MHz output of the instrument.

# **Key Path**

VIEW CAL ON OFF (INPUT)

VIEW CAL More Inst 1 of 3 Setup Input ON OFF (SETUP)

# **Related Programming Command**

**CALSW** 

VIEW PK QP AV Softkey that toggles between the different detection modes, peak (PK), quasi-peak (QP), and average (AV). This function is only active if QUASI-PEAK) or (AVERAGE) have been selected. VIEW PK QP AV does not affect any other settings except the selected detector.

# **Key Path**

More More VIEW 1 of 3 2 of 3 PK QP AV

# **Related Programming Command**

none

# VISION ENHANCE1

Softkey that sets the display screen to vision enhance. The special colors built into vision enhance 1 and 2 accommodate most color deficient vision problems.

# **Key Path**

Display Adjust Special VISION (DISPLAY) Config Color Colors ENHANCE1

# **Related Programming Command**

SETC

# VISION ENHANCE2

Softkey that sets the display screen to vision enhance. The special colors built into vision enhance 1 and 2 accommodate most color deficient vision problems.

# **Key Path**

Adjust Special VISION Display Config Color Colors ENHANCE2 DISPLAY

## **Related Programming Command**

SETC

Volts Softkey that changes the amplitude units to volts.

# **Key Path**

More Amptd (AMPLITUDE) 1 of 3 Units Volts

# **Related Programming Command**

none

# Watts

Softkey that changes the amplitude units to watts.

## **Key Path**

More Amptd 1 of 3 Units Watts (AMPLITUDE)

# **Related Programming Command**

none

# WHITE DOTS

Softkey that replaces the standard display screen with white dots. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

## **Key Path**

Display Test More WHITE (DISPLAY) Config Patterns 1 of 4 DOTS

# **Related Programming Command**

none

# WHITE FILL

Softkey that replaces the standard display screen with a white box. This is one of 18 test patterns that can be used for display-troubleshooting and screen-alignment procedures.

#### **Key Path**

WHITE Display Test More More Config Patterns 1 of 4 2 of 4 FILL (DISPLAY)

# **Related Programming Command**

none

# WINDOWS OFF

Softkey that turns off the windows display mode and returns to the normal full-sized display. The state of the last active window will become the instrument state when the windows display is turned off.

# **Key Path**

(CTRL) WINDOWS OFF

# **Related Programming Command**

WINOFF

# X FINE TUNE DAC

Softkey that displays the output of the YTO extra-fine-tune DAC (FM_TUNE) that is on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

# **Key Path**

(CALIBRATE)	More 1 of 3	More	More 1	 More 3
X FINE TUNE DAC				

## **Related Programming Command**


none

# YTF DRIVER

For an HP 8546A/HP 85462A only.

Softkey that displays the output of the sample-and-hold circuit in the YTF span divider and driver located on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

# **Key Path**



# **Related Programming Command**

none

# YTF SPAN

For an HP 8546A/HP 85462A only.

Softkey that displays a trace of the voltage driving the YTF as it sweeps through the displayed span. This is a service diagnostic function and is for service use only.

# **Key Path**

	More	More	Service		YTF
CALIBRATE	1 of 3	2 of 3	Diag	More 2	SPAN

# **Related Programming Command**

none

# YTF TUNE COARSE

For an HP 8546A/HP 85462A only.

Softkey that displays the output produced by the YTF coarse-tune DAC located on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

# **Key Path**

(CALIBRATE)	More 1 of 3	More 2 of3	Service Diag	More 1	 More 5
YTF TUNE COARSE					

# **Related Programming Command**

none

# YTF TUNE FINE

For an HP 8546A/HP 85462A only.

Softkey that displays the output produced by the YTF fine-tune DAC located on the A7 analog interface assembly. This is a service diagnostic function and is for service use only.

# **Key Path**

(CALIBRATE)	More 2 of3	Service Diag	More 1	 More 5
YTF TUNE FINE				

# **Related Programming Command**

none

YZ_# Spc Clear

Softkey that accesses the menu used for selecting the characters Y, Z, underscore (_), #, space, or for clearing the screen title.

# **Key Access**

(CAL), (CONFIG), (DISPLAY), (RECALL), (SAVE), or (SETUP)

## **Related Programming Command**

none

# ZERO SPAN

Softkey that changes the frequency span to zero and turns off marker track if it is on.

# **Key Path**

ZERO (SPAN) SPAN

# **Related Programming Command**

# ZONE CENTER

Softkey that moves the zone markers in frequency without changing the zone span. The zone markers are vertical lines marking the zone on the upper window. They correspond with the frequency range displayed in the lower window. As the zone markers are moved the center frequency of the lower window is changed but the lower window will not be updated unless it is active.

The zone can be moved beyond the frequency range that is being displayed in the upper window. Its movement is limited to the frequency range of the instrument. The zone markers will be displayed at the edges of the upper window when the zone is moved beyond the displayed frequency range.

#### **Key Path**

ZONE WINDOWS (CTRL) CENTER

# **Related Programming Command**

**ZMKCNTR** 

ZONE PK LEFT Softkey that searches for the next frequency peak outside and to the left of the zone markers on the upper window trace and then moves the zone so that it is centered around the new peak. The zone span is not changed. The center frequency of the lower window changes to reflect the new zone center frequency. The lower window will not be updated until it is made active. If no peak is found the zone will not be moved. A signal must have a 6 dB peak excursion to be identified as a peak signal. The definition of a peak excursion can be changed by selecting PEAK EXCURSN while the upper window is active.

Pressing ZONE PK LEFT will have no effect if the upper window is in zero span.

# **Key Path**

ZONE

WINDOWS (CTRL) PK LEFT

# **Related Programming Command**

ZMKPKNL

ZONE PK RIGHT Softkey that searches for the next frequency peak outside and to the right of the zone markers on the upper window trace and then moves the zone so that it is centered around the new peak. The zone span is not changed. The center frequency of the lower window changes to reflect the new zone center frequency. The lower window will not be updated until it is made active. If no peak is found the zone will not be moved. A signal must have a 6 dB peak excursion to be identified as a peak signal. The definition of a peak excursion can be changing by selecting PEAK EXCURSN while the upper window is active.

Pressing ZONE PK RIGHT will have no effect if the upper window is in zero span.

# **Key Path**

ZONE

WINDOWS (CTRL) PK RIGHT

# **Related Programming Command**

**ZMKPKNR** 

ZONE SPAN

Softkey that changes the span of the zone markers without changing the center frequency. The zone markers are vertical lines marking the zone on the upper window. They correspond with the frequency range displayed in the lower window. As the zone markers are moved the span of the lower window is changed but the lower window will not be updated unless it is active.

The zone can be expanded beyond the frequency range that is being displayed in the upper window. Its movement is limited to the frequency range of the instrument. The zone markers will be displayed at the edges of the upper window when the zone is moved beyond the displayed frequency range.

## **Key Path**

ZONE WINDOWS (CTRL) SPAN

# **Related Programming Command**

**ZMKSPAN** 



Hardkey that switches between the split-screen windows display and a full size display of the window that is currently active. Once the ZOOM function is active the (NEXT) key can be used to switch between the two windows while remaining zoomed (full sized).

# **Related Programming Command**

WINZOOM

# **Error Messages**

The instrument can generate various messages that appear on its screen during operation to indicate a problem.

There are three types of messages: hardware error messages (H), user-created error messages (U), and informational messages (M).

- Hardware error messages indicate the instrument hardware is probably broken.
- User-created error messages appear when the instrument is used incorrectly. They are usually generated during remote operation (entering programming commands using either a controller or the external keyboard).
- Informational messages provide information indicating the progress of the instrument within a specific procedure.

The messages are listed in alphabetical order on the following pages; each message is defined, and its type is indicated by an (H), (U), or (M).

# φ LOCK OFF

Indicates slow YTO tuning. This message may appear if the instrument is using default correction factors. If this message appears constantly, perform the self-calibration routine to try to eliminate this message.  $\phi$  LOCK OFF appears briefly during the self-calibration routine, during instrument preset, or when the frequency value is changed; this is normal and does not indicate a problem. (U) and (H)

#### ADC-2V FAIL

Indicates a hardware failure. (H)

#### ADC-GND FAIL

Indicates a hardware failure, (H)

#### ADC-TIME FAIL

Indicates a hardware failure. (H) and (U)

#### Bad device type in msus

An attempt has been made to read a disk that is neither LIF nor DOS format or a communication failure between the main processor and the floppy disk subsystem. If the disk in use is LIF or DOS format, try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative. (U) (H)

#### Bad mass storage parameter

May be reported if an attempt is made to read a disk that is neither

LIF nor DOS format. Attempt a catalog operation on the disk or try a different disk. (U)

## Bad mass storage volume label

May be reported if an attempt is made to read a disk that is neither LIF nor DOS format. Attempt a catalog operation on the disk or try a different disk. (U)

#### Bad mass storage volume spec

May be generated if the user removes media while it is being accessed or if a read or write operation is attempted on unformatted media. Try the operation again or try the operation on media you are sure has been appropriately formatted.

# Cal harmonic > = 5.7 GHz NOT found For an HP 8546A/HP 85462A only.

Indicates that the CAL YTF routine cannot find a harmonic of the 300 MHz calibration signal. If this happens, perform the CAL FREQ and CAL AMP routines, and then perform the CAL YTF routine again. For the HP 8546A, press CAL ALL then perform the CAL YTF routine again. (U) and (H)

#### CAL: MAIN COIL SENSE FAIL

The instrument could not set up span sensitivity of the main coil. If this message appears, press (FREQUENCY), CENTER FREQ, -37, (Hz), (CALIBRATE), More 1 of 3, More 2 of 3, DEFAULT CAL DATA, and perform the self-calibration routine again. (H)

#### CAL: NBW 200 Hz notch amp failed

Indicates that the 200 Hz IF bandwidth is not the correct shape for the calibration routine. (H)

#### CAL: NBW 200 Hz notch failed

Indicates that the 200 Hz IF bandwidth is not the correct shape for the calibration routine. (H)

# CAL: NBW 200 Hz width failed

Indicates that the 200 Hz IF bandwidth is not the correct bandwidth for the calibration routine. (H)

# CAL: NBW gain failed

Indicates that one of the IF bandwidths is not the correct amplitude for the calibration routine. (H)

#### CAL: NBW width failed

Indicates that one of the IF bandwidths is not the correct width for the calibration routine. (H)

#### CAL: PASSCODE NEEDED

Indicates that the function cannot be accessed without the pass code. For the DEFAULT CAL DATA function, the pass code is setting the center frequency of the instrument to -37 Hz. (M)

# CAL: RES BW AMPL FAIL

The relative insertion loss of the IF bandwidth is incorrect. This message also sets SRQ 110. (H)

#### CAL SIGNAL NOT FOUND

Indicates the calibration signal cannot be found. Check that

the instrument input connectors are connected properly. If the calibration signal is connected properly but cannot be found, press (FREQUENCY), CENTER FREQ, -37, (Hz), (CALIBRATE), More 1 of 3, More 2 of 3, DEFAULT CAL DATA. If the calibration signal still cannot be found, press (FREQUENCY), CENTER FREQ, -37, (Hz) and perform the CAL FREQ and CAL AMP (receiver RF section) or CAL ALL (EMI receiver) self-calibration routines. This message also sets SRQ 110. (U) and (H)

#### CAL: SPAN SENS FAIL

The self-calibration span sensitivity routine failed. This message also sets SRQ 110. (H)

#### CAL: USING DEFAULT DATA

Indicates that the calibration data is corrupt and the default correction factors are being used. Interruption of the self-calibration routines or an error can cause this problem. (M)

CAL YTF FAILED For an HP 8546A/HP 85462A only. Indicates that the CAL YTF routine could not be successfully completed. Perform the self-calibration routines, then perform the CAL YTF routine again. (U) and (H)

#### CAL: ZERO FAIL

The instrument could not set up the tuning sensitivity of the main coil. If this message appears, press (FREQUENCY), CENTER FREQ, -37, (Hz), (CALIBRATE), More 1 of 3, More 2 of 3, DEFAULT CAL DATA, and perform the self-calibration routines again. (H)

Cannot engage phase lock with current CAL FREQ data Indicates that the CAL FREQ routine needs to be performed before phase locking can be turned on. (U)

#### Cannot BYPASS Input 1

An attempt was made to execute the BYPASS command while the signal path is routed through INPUT 1 of the RF filter section. Only INPUT 2 of the RF filter section can be bypassed.

#### Checkread error

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, ((ENTER)), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

# COMMAND ERROR:_ _ _

The specified programming command is not recognized by the instrument. (U)

#### **Configuration Error**

This error indicates a serious problem in the ability of the instrument to use the floppy disk drive. Try presetting the instrument. If the condition persists, contact your HP representative. (H)

#### CONF TEST FAIL

Indicates that the confidence test failed. Perform the self-calibration routines, and then perform the confidence test again. This message also sets SRQ 110. (H) and (U)

#### Directory not empty

Reported if an attempt is made to purge a non-empty directory. Ensure that all files in any directory have been purged or moved before attempting to purge the directory. (U)

## Directory overflow

Reported if the disk directory runs out of room. Change the media. (M)

#### Drive not found or bad address

An attempt has been made to read a disk that is neither LIF nor DOS format or a communications failure between the main processor and the floppy disk subsystem. If the disk in use is LIF or DOS format, try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative. (U) (H)

# Duplicate file name

Reported if the file system tries to write data to a file that already exists, but did not exist previously. May be due to changing media just before an operation attempts to create a new file. (U)

# Duplicate file name, PROTECT is on

Reported if the user attempts to overwrite a previously existing file with PROTECT status set to ON (the default state). Use a different file name, purge the file, or turn off the PROTECT feature. (U)

# End of file or buffer found

Reported if an attempt is made to read or write beyond the current file or directory is made. Also reported if an attempt is made to add files to a directory that is already full. Try using a new disk. (U)

#### End of rec found, random mode

Reported if an attempt is made to read or write beyond the current record being accessed. Try the operation again. (U)

#### FAIL:_ _ _

An error was discovered during the power-up check. The 4-digit by 10-digit code indicates the type of error, (H)

#### File name is undefined

May be reported if the user changes media immediately before a read operation is attempted on a file of a specific name. Ensure that the file exists on the disk by using the catalog feature. (U)

# File not currently assigned

May be generated if the user removes media while it is being accessed. Try the operation again. (U)

#### File open on target device

May be due to conflicting file operations invoked simultaneously from the front-panel keys and the remote I/O port. Attempt the operation again. (U)

## File type incompatible

Indicates that the selected file is not a display image file. The file name for a display image file is always preceded by an "i." (U)

#### FREQ UNCAL

The FREQ UNCAL message appearing constantly, indicates a YTO-tuning error. Perform the CAL FREQ (receiver RF section) or CAL ALL (EMI receiver) routines. (U) and (H)

#### Function not available in current Mode

Indicates that the function that you have selected can only be used with the instrument mode. You can use the MODE key to select the instrument mode. (U)

# HFS disc may be corrupt

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, (ENTER), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

#### Improper destination type

Reported if an attempt is made to append data to a file and the file cannot be extended. Try the operation using another disk. (U)

## Improper file name

Reported if a file or directory name is specified that in some manner does not conform to file name conventions: too many characters, illegal character in file name, and so on.

# Improper file type

Reported in the event that an operation appropriate for a data file is attempted on a directory. Check the contents of the disk using the catalog function. (U)

#### Improper value or out of range

Indicates an internal error in computing the amount of data to read from the disk or an invalid parameter. This may indicate corrupt media; try a new disk. If the condition persists, contact your HP representative. (H)

#### Incorrect unit code in msus

An attempt has been made to read a disk that is neither LIF nor DOS format or a communications failure between the main processor and the floppy disk subsystem. If the disk in use is LIF or DOS format, try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative. (U) (H)

#### Incorrect volume code in msvs

An attempt has been made to read a disk that is neither LIF nor DOS format or a communications failure between the main processor and the floppy disk subsystem. If the disk in use is LIF or DOS format, try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative. (U) (H)

#### **Insufficient Memory**

Indicates a temporary memory overflow condition. Attempt to free

memory that may have been temporarily allocated by performing the following steps:

- 1. If there is a disk catalog on the display, exit the catalog.
- 2. Execute the dispose softkeys under Dispose User Mem in the (CONFIG) menu. (U)

# **INTEGER** overflow

Indicates a computation error during disk access. This may indicate corrupt media; try a new disk. If the condition persists, contact your HP representative. (H)

#### Internal error

Indicates a failure of the floppy disk controller or a failure in communications between the main processor and the floppy disk controller. Try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative. (H)

#### INTERNAL LOCKED

The internal trace and state registers of the instrument have been locked. To unlock the trace or state registers, press (SAVE), Save Internal, SAV LOCK ON OFF so that OFF is underlined. (U)

## INVALID AMPCOR: FREQ

For the AMPCOR command, the frequency data must be entered in increasing order. See the description for the AMPCOR programming command for more information. (U)

# INVALID ENTER FORMAT

The enter format is not valid. See the appropriate programming command description to determine the correct format. (U)

# INVALID <file name> NOT FOUND

Indicates that the specified file could not be loaded into internal memory or purged from memory because the file name cannot be found. (U)

#### INVALID FILENAME

Indicates the specified file name is invalid. A file name is invalid if there is no file name specified, if the first letter of the file name is not alphabetic, or if the specified file type does not match the type of file. See the description SAVRCLW or STOR programming commands for more information. (U)

# INVALID FILE: NO ROOM

Indicates that there is insufficient space available on the floppy disk to store the data. (U)

# INVALID HP-IB ADRS/OPERATION

An HP-IB operation was aborted due to an incorrect address or invalid operation. Check that there is only one controller (the EMI receiver) connected to the printer or plotter. (U)

#### INVALID HP-IB OPERATION REN TRUE

The HP-IB operation is not allowed. (This is usually caused by trying to print or plot when a controller is on the interface bus with the instrument.) To use the instrument print or plot functions, you must disconnect any other controllers on the HP-IB. If you are using programming commands to print or plot, you can use an HP

BASIC command instead of disconnecting the controller. See the description for the PRINT command for more information. (U)

#### INVALID ITEM:_ _ _

Indicates an invalid parameter has been used in a programming command. (U)

#### INVALID KEYLBL: _ _ _

Indicates that the specified key label contains too many characters. A key label is limited to 8 printable characters per label line. (U)

#### INVALID KEYNAME:_ _ _

The specified key name is not allowed. (The key name may have conflicted with a instrument programming command.) To avoid this problem, use an underscore as the second character in the key name, or avoid beginning the key name with the following pairs of letters: LB, OA, OL, TA, TB, TR, MA, MF, TS, OT, and DR. (U)

# INVALID OUTPUT FORMAT

The output format is not valid. See the appropriate programming command description to determine the correct format. (U)

# **INVALID RANGE: Stop < Start**

Indicates that the first trace element specified for a range of trace elements is larger that ending trace element. When specifying a trace range the starting element must be less than the ending element. For example, TRA[2,300] is legal but TRA[300,2] is not. (U)

#### INVALID REGISTER NUMBER

The specified trace register number is invalid. (U)

#### INVALID RS-232 ADRS/OPERATION

An RS-232 operation was aborted due to an invalid operation. (U)

# INVALID SAVE REG

Data has not been saved in the specified state or trace register, or the data is corrupt. (U)

#### INVALID SCRMOVE

Indicates the instrument may have a hardware failure. (H)

#### INVALID START INDEX

Indicates that the first trace element specified for a range of trace elements is not within the trace range of the specified trace. (U)

# INVALID STOP INDEX

Indicates that the ending trace element specified for a range of trace elements is not within the trace range of the specified trace. (U)

#### INVALID TRACE: _ _ _

The specified trace is invalid. (U)

# INVALID VALUE PARAMETER: _ _ _

The specified value parameter is invalid. (U)

# INVALID WINDOW TYPE: _ _ _

The specified window is invalid. See the description for the TWNDOW programming command. (U)

#### LOST SIGNAL

This message indicates that an internal hardware connection problem exists. (H)

#### LO UNIVL

Indicates that the local oscillator in the EMI receiver distribution amplifier is not functioning properly. (H)

#### Marker Count Reduce SPAN

Indicates the IF bandwidth to span ratio is too small to use the marker count function. Check the span and IF bandwidth settings,

#### Marker Count Widen RES BW

Indicates that the current IF bandwidth setting is too narrow to use with the marker counter function. The marker counter function can be in narrow IF bandwidths (bandwidths that are less than 1 kHz) with the following procedure:

- 1. Place the marker on the desired signal.
- 2. Increase the IF bandwidth to 1 kHz and verify the marker is on the signal peak.
- 3. If the marker in on the signal peak, the marker count function can be used in either the 1 kHz IF bandwidth or the original narrow IF bandwidth setting. If the marker is not on the signal peak, it should be moved to the signal peak and the marker counter function should not be used with a IF bandwidth setting of less than 1 kHz. (U)

#### Mass storage hardware failure

Indicates a failure of the floppy disk controller or a failure in communications between the main processor and the floppy disk controller. Try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative, (H)

#### Mass storage medium overflow

Reported when a disk has no more room available to write data. Try a new disk. (U)

#### Mass storage system error

Indicates a failure of the floppy disk controller or a failure in communications between the main processor and the floppy disk controller. Try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative.

#### Mass storage volume not present

An attempt has been made to read a disk that is neither LIF nor DOS format or a communications failure between the main processor and the floppy disk subsystem. If the disk in use is LIF or DOS format, try turning the instrument off, wait a few seconds, then turn the instrument on again. If the condition persists, contact your HP representative. (U) (H)

#### MEAS UNCAL

The measurement is uncalibrated. Check the sweep time, span, and bandwidth settings, or press (AUTO COUPLE), AUTO ALL. (U)

#### Medium changed or not in drive

Reported if disk is removed during disk access cycle. Try the operation without removing the disk. (U)

#### Medium uninitialized

Indicates that a file operation has been attempted on an uninitialized disk, or on a disk that is neither LIF nor DOS format. Be sure that any disk on which file operations are attempted is properly formatted. The format softkeys, in the (CONFIG) menu, may be used to format a disk, but any information on the disk will be erased during the formatting process. (U)

# No points defined

Indicates the specified limit line or amplitude correction function cannot be performed because no limit line segments or amplitude correction factors have been defined. (U)

#### Operation failed on some files

Reported if, during a purge operation on a file specifier that contains wildcards, the number of files actually purged does not match the original number of files found that match the file specifier. Check the disk using the catalog function. (U)

# Operation not allowed on open file

May be due to conflicting file operations invoked simultaneously from the front-panel keys and the remote I/O port. Attempt the operation again. (U)

#### OVEN COLD

Indicates that the EMI receiver has been powered up for less than 5 minutes. (The actual temperature of the precision frequency oven is not measured.) (M)

#### PARAMETER ERROR: _ _ _

The specified parameter is not recognized by the instrument. See the appropriate programming command description to determine the correct parameters. (U)

#### PASSCODE NEEDED

Indicates that the function cannot be accessed without the pass code. (U)

#### Permission denied

Indicates that a file write-operation was attempted on either a read-only file or on a directory. Check the disk using the catalog function and try the operation on an appropriate file again. (U)

# Possibly corrupt file

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, ((ENTER)), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

# POS-PK FAIL

Indicates the positive-peak detector has failed. (H)

#### RCVR Limits not allowed in SA mode

This error is encountered when an attempt is made to enable limit-line display, limit-margin display, or limit testing of limits defined in Receiver mode when the instrument is operating in Signal Analysis mode. To correct the problem, either purge the limits or switch to Receiver mode. (U)

#### Read data error

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, (ENTER), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

#### Record address error

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, (ENTER), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

#### Record not found

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, (ENTER), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

#### REF UNLOCK

Indicates that the frequency reference is not locked to the external reference input. Check that the 10 MHz REF OUTPUT connector is connected to the EXT REF IN connector, or, when using an external reference, that an external 10 MHz reference source of sufficient amplitude is connected to the EXT REF IN connector. (U) and (H)

Require 1 signal > PEAK EXCURSION above THRESHOLD Indicates that the N dB PTS routine cannot locate a signal that is high enough to measure. The signal must be greater than the peak excursion above the threshold level to measure. (U)

Require 3 signals > PEAK EXCURSION above THRESHOLD Indicates that the % AM routine cannot locate three signals that are high enough to measure. The signals must be greater than the peak excursion above the threshold level to measure. (U)

Require 4 signals > PEAK EXCURSION above THRESHOLD Indicates that the TOI routine cannot locate four signals that are high enough to measure. The signals must be greater than the peak excursion above the threshold level to measure. (U)

#### Required option not installed

Some instrument functions require that an option be installed in the instrument. See the description for the function in the User's Guide for more information about which option is required. (U)

#### **RF Filter Section Absent**

This message is displayed if the bypass command is executed when the RF filter section is not connected to, or is not communicating with, the receiver RF section. (U) and (H)

#### RFFS Error: COMMAND

The RF filter section has received a command that it does not recognize. Assure that there is no cable connected to the RF filter

section Service Bus interface. If the condition persists, and there is no cable connected to the RF filter section Service Bus interface, contact your HP representative. (U)

# RFFS Error: HARDWARE

The RF filter section has experienced a hardware failure. If the condition persists after presetting the instrument or cycling power, contact your HP representative. (H)

#### RFFS Error: TIMEOUT

Communication failure between the receiver RF section and the RF filter section. Check power to the RF filter section and check that the AUX interface cable is properly connected between both instruments. (U) (H)

# RFFS Service Bus Active

This message appears in the active function area of the receiver RF section display when an external controller communicates with the RF filter section via the RF filter section Service Bus interface. (H)

**RF PRESEL ERROR** For an HP 8546A/HP 85462A only. Indicates that the preselector peak routine cannot be performed. (H)

**RF PRESEL TIMEOUT** For an HP 8546A/HP 85462A only. Indicates that the preselector peak routine cannot be performed. (H)

#### SA Limits not allowed in RCVR mode

This error is encountered when an attempt is made to enable limit-line display, limit-margin display, or limit testing of limits defined in Signal Analysis mode when the instrument is operating in Receiver mode. To correct the problem, either delete the limits or switch to Signal Analysis mode. (U)

## SAMPLE FAIL

Indicates the sample detector has failed. (H)

#### SIGNAL CLIPPED

Indicates that the current FFT measurement sweep resulted in a trace that is above the top graticule line on the display. If this happens, the input trace (trace A) has been "clipped," and the FFT data is not valid. (U)

#### Signal not found

Indicates the PEAK ZOOM routine did not find a valid signal. (U)

# Signals do not fit expected % AM pattern

Indicates that the % AM routine cannot perform the percent AM measurement because the onscreen signals do not have the characteristics of a carrier with two sidebands, (U)

#### Signals do not fit expected TOI pattern

Indicates that the TOI routine cannot perform the third-order intermodulation measurement because the onscreen signals do not have the characteristics of two signals and two distortion products. (U)

#### SMPLR UNLCK

Indicates that the sampling oscillator circuitry is not functioning

properly. If this message appears, check that the external frequency reference is correctly connected to the EXT REF INPUT. (U) and (H)

#### SOFTKEY OVFL

Softkey nesting exceeds the maximum number of levels. (U)

#### SRQ _ _ _

The specified service request is active. (M)

#### STEP GAIN/ATTN FAIL

Indicates the step gain has failed. (H)

#### TABLE FULL

Indicates the upper or lower table of limit lines contains the maximum number of entries allowed. Additional entries to the table are ignored. (U)

#### TG SIGNAL NOT FOUND

Indicates the tracking generator output signal cannot be found. For the receiver RF section, check that the TRACKING GENERATOR OUTPUT is connected to the RF INPUT connector with an appropriate cable. For the EMI receiver, check that the cable between the TRACKING GENERATOR OUTPUT and TRACKING GENERATOR is properly connected. (U)

#### TG UNLVL

This message can indicate the following: that the source power is set higher or lower than the instrument can provide, that the frequency span extends beyond the specified frequency range of the tracking generator, or that the calibration data for the tracking generator is incorrect. (U)

#### Too many open files

This error may be due to conflicting disk operations invoked from the front-panel keys and the remote I/O port, or it may indicate that the disk is corrupt. After pressing the "HOLD" key, (ENTER), on the front panel, retry the operation. If the operation fails again, check the disk using the catalog function. (U)

#### Too many signal with valid N dB points

Indicates the N dB PTS function has located two or more signals that have amplitudes within the specified dB from the signal peak. If this happens, you should decrease the span of the instrument so that only the signal that you want to measure is displayed. (U)

#### Trace A is not available

Indicates that trace A is in the store-blank mode and cannot be used for limit-line testing. Use CLEAR WRITE A or VIEW A to change trace A from the store-blank mode to the clear write mode, and then turn on limit-line testing. (U)

#### Unable to replace file

Reported if an attempt is made to append data to a file and the file cannot be extended. Try the operation using another disk. (U)

# USING DEFAULTS self cal needed

Indicates that the current correction factors are the default correction factors and that the self-calibration routines need to be performed. For either an HP 8546A or an HP 85462A, also perform the CAL YTF self-calibration routine. (U)

#### VID-BW FAIL

Indicates the averaging bandwidths have failed. (H)

# Wildcard matches > 1 item

An attempt was made to use the wildcard matching character on an operation that requires a specific file name. For example, an attempt to load from a file name that contains a wildcard character. Try the operation using a specific file name. (U)

# Wildcards not allowed

An attempt was made to use the wildcard matching character on an operation that requires a specific file name. For example, an attempt to load from a file name that contains a wildcard character. Try the operation using a specific file name. (U)

# Write protected

Indicates that a write operation was attempted on a disk that is write protected. Move the write-protect tab on the floppy disk to the unprotected position, reinsert the disk in the disk drive and attempt the operation again. (U)

# Nonrecoverable System Errors

Certain situations can create error conditions from which the main processor cannot recover. In the event that the processor detects a nonrecoverable error, the instrument will be initialized, the display will be blanked, and special error messages will be written to the display.

The following is a sample nonrecoverable system error message display.

13:18:20 DEC 13, 1993, Rev: 931210   SR: 0000   PC: 00FFB370   00FF6F1E: 00009300   00: 00000000   A0: 00FF803E   00FF6F22: 00000000   00: 00000000   A1: 00FF803E   00FF6F26: 00000000   00: 00FF803E   A2: 00FF803C   00FF6F2A: 00FF803E   00FF803E   00FF803E   00FF6F2E: 000031B1   00: 00: 00: 00: 00: 00: 00: 00: 00: 0						
O0:         00000000         A0:         00FFB238         00FF6F22:         00000000           O1:         00000000         A1:         00FF803E         00FF6F26:         00000000           O2:         00FFB238         A2:         00FF803C         00FF6F2A:         00FF803E           O3:         00FF803E         A3:         00FF82FE         00FF6F2E:         000031B1           O4:         00008E7D         A4:         00FF82F4         00FF6F32:         0004065E           O5:         00FF80E8         A5:         00FC6948         00FF6F36:         0004EDE8           O6:         00FFB39A         A6:         FFFFFFFE         00FF6F3A:         00FF8000           O7:         00FFB392         A7:         00FF6F1E         00FF6F3E:         00FF88AE						
01:       00000000       A1:       00FF803E       00FF6F26:       00000000         02:       00FFB238       A2:       00FF803C       00FF6F2A:       00FF803E         03:       00FF803E       A3:       00FF82FE       00FF6F2E:       000031B1         04:       00008E7D       A4:       00FF82F4       00FF6F32:       0004065E         05:       00FF80E8       A5:       00FC6948       00FF6F36:       0004EDE8         06:       00FFB39A       A6:       FFFFFFFE       00FF6F3A:       00FF8000         07:       00FFB392       A7:       00FF6F1E       00FF6F3E:       00FF88AE						
O2:       00FFB238       A2:       00FF803C       00FF6F2A:       00FF803E         O3:       00FF803E       A3:       00FFB2FE       00FF6F2E:       000031B1         O4:       00008E7D       A4:       00FFB2F4       00FF6F32:       0004065E         O5:       00FF80E8       A5:       00FC6948       00FF6F36:       0004EDE8         O6:       00FFB39A       A6:       FFFFFFFE       00FF6F3A:       00FF8000         O7:       00FFB392       A7:       00FF6F1E       00FF6F3E:       00FF88AE						
03:       00FF803E       A3:       00FFB2FE       00FF6F2E:       000031B1         04:       00008E7D       A4:       00FFB2F4       00FF6F32:       0004065E         05:       00FF80E8       A5:       00FC6948       00FF6F36:       0004EDE8         06:       00FFB39A       A6:       FFFFFFE       00FF6F3A:       00FF8000         07:       00FFB392       A7:       00FF6F1E       00FF6F3E:       00FF88AE						
04:       00008E7D       A4:       00FFB2F4       00FF6F32:       0004065E         05:       00FF80E8       A5:       00FC6948       00FF6F36:       0004EDE8         06:       00FFB39A       A6:       FFFFFFFE       00FF6F3A:       00FF8000         07:       00FFB392       A7:       00FF6F1E       00FF6F3E:       00FF88AE						
D5:       00FF80E8       A5:       00FC6948       00FF6F36:       0004EDE8         D6:       00FFB39A       A6:       FFFFFFFE       00FF6F3A:       00FF8000         D7:       00FFB392       A7:       00FF6F1E       00FF6F3E:       00FF88AE						
D6:       00FFB39A       A6:       FFFFFFFE       00FF6F3A:       00FF8000         D7:       00FFB392       A7:       00FF6F1E       00FF6F3E:       00FF88AE						
D7:         00FFB392         A7:         00FF6F1E         00FF6F3E:         00FF88AE						
00FF6F42: 00FF87E0						
001101111. 001101110						
00FF $6$ F $46$ : $00$ FF $B03$ C						
00FF $6$ F $4$ A: $000$ C $9$ AEA						
00 FF 6F 4E: 00 FF 8890						
00FF6F52: $040800FF$						
00 FF 6F 56: 000 900 FF						
00FF6F5A: $B23$ A $0000$						
WARNING: Config Settings Defaulted						
Press COPY to print error report and						
advise your local HP representative						
Press PRESET to resume operation						

When a nonrecoverable error message is displayed, the instrument will only respond to the front-panel COPY and PRESET keys. If you have a printer configured and connected to the instrument, and if no remote controller is currently connected to the I/O port through which the printer is connected, you can generate a hardcopy of the diagnostic part of the error message by pressing the front-panel COPY key.

In order to resume instrument operation following a nonrecoverable system error, press the front-panel PRESET key. The instrument will resume operation from its preset state.

Among the conditions which can contribute to the occurrence of a nonrecoverable system error are:

- Hardware failure of the main processor
- Hardware failure of system memory available to the main processor
- Errors in the primary system control program
- Attempted execution of unsupported system commands

Nonrecoverable system errors may occur when attempting to load an improper file type into the machine. For example, loading a file with an incorrect format into a limit line or amplitude correction table may generate this error.

If nonrecoverable system errors occur regularly, contact your  $\operatorname{HP}$  representative.

# **SRQ**

# **Service Requests**

This appendix describes the receiver service request (SRQ) capability. A service request is an instrument output that tells the operator or computer that a specific event has taken place in the instrument.

When writing programs, service requests can be used to interrupt the computer program sequence, causing the program to branch to a subroutine. For example, by using service requests, the computer can perform other operations while the receiver is sweeping. When the sweep is completed, the computer can service the receiver by changing the receiver state or reading data from the memory.

#### Note

Service requests do not work with computers that have an RS-232 interface. Not all service requests are available with some HP-IB computers. Refer to the manuals supplied by your computer's manufacturer.

When making a service request, the receiver places the I/O interface SRQ line true and the receiver displays SRQ with an octal coded number. Setting the SRQ line true announces to the computer that the receiver requires attention. The computer can then command the receiver to send its "status byte." The status byte indicates the type of service request. The status byte is the binary equivalent of the octal SRQ number.

#### Note

If the instrument display annotation has been blanked, the service request notation will not appear.

A serial polling technique must be used by the computer to test for service requests. The receiver does not respond to parallel polling.

A service request can be cleared from the display by doing an instrument preset.

#### **Status Byte Definition**

The status byte sent by the receiver determines the nature of the service request. The meaning of each bit of the status byte is explained in Table A-1.

Table A-1. Status Byte Definition

Bit	Message	Display Message
0 (LSB)	Overload Detected	SRQ 101
1	Unit Key Pressed	SRQ 102
2	End of sweep	SRQ 104
3	Hardware broken	SRQ 110
4	Command complete	SRQ 120
5	Illegal spectrum analyzer command	SRQ 140
6	Universal HP-IB service request HP-IB RQS bit	=
7	Unused	_

The display message is an octal number based on the binary value of the status byte. This octal number always begins with a "1" since this is translated from bit 6, the universal service request bit. The status byte for an illegal receiver command (SRQ 140) is as follows:

bit number	7 6	5 4 3	2 1 0
status byte	0 1	1 0 0	0 0 0

This displays the octal equivalent of the status byte binary number: SRQ 140

The octal equivalent is based on the whole binary number: 01100000 (binary) = 140 (octal)

One simple way to determine the octal equivalent of the binary number is to partition the binary number three bits at a time from the least significant bit, and treat each part as a single binary number:

binary	0 1	1 0 0	0 0 0
octal	1	4	0

The decimal equivalent of the octal number is determined as follows:

$$140 \text{ (octal)} = 1 \times (8) + 4 \times (8) + 0 \times (8) = 96 \text{ (decimal)}$$

More than one service request can be sent at the same time. For example, if an illegal receiver command (SRQ 140) and the end of a sweep (SRQ 104) occurred at the same time, SRQ 144 appears on the receiver display, because both bit 5 and bit 2 are set as shown below:

bit number	7 6	5 4 3	2 1 0	
status byte	0 1	1 0 0	1 0 0	•
octal value	1	4	4	= SRQ 144

# **Service Request Activating Commands**

With the exceptions of SRQ 101, SRQ 140, and SRQ 110, service requests can only be activated from a computer. (SRQ 101, SRQ 140, and SRQ 110 are activated at instrument preset.) Your programmer's guide describes service request activating commands under RQS and SRQ.

# **Index**

- **0** 0-2.9 Gz BAND 0, 4-5, 4-25
- 1 10 MHz reference DAC setting, 4-33 +10V REF DETECTOR, 4-2, 4-9 -10V REF DETECTOR, 4-9 120 kHz EMI BW, 4-10 150 kHz - 30 MHz, 4-10
- 2 200 Hz EMI BW, 4-11 200 MHz - 1 GHZ, 4-11 2.75-6.5 BAND 1, 4-6, 4-25 2v REF DETECTOR, 4-2, 4-6
- 3 30 MHz 300 MHz, 4-9 3 dB POINTS, 4-7 3rd ORD MEAS, 4-7
- **6** 6 dB POINTS, 4-8
- 9 99% PWR BW, 4-10 9 kHz - 150 kHz, 4-8 9 kHz EMI BW, 4-8
- A ABCDEF, 4-13 ABORT, 4-13 A -> C, 4-12 ac coupling, 4-51 ACTIVE, 4-13 active function clearing, 4-93 addressing printer, 4-148 address of plotter, 4-137 ADD TO LIST, 4-13 Adjust Color, 4-14 ADVISORY, 4-14 A < -> B, 4-11 ALC INT EXT, 4-14 alpha characters, 4-13, 4-90, 4-190, 4-206 % AM, 4-4 A-B -> A ON OFF, 4-12AMPLITUDE, 4-15 amplitude accuracy, 4-50 amplitude correction factors edit done, 4-70

```
select amplitude, 4-168
 select frequency, 4-170
 select point, 4-172
amplitude demodulation, 4-61
amplitude menus, 4-15
amplitude modulation, 4-4
amplitude scale, 4-167
amplitude units, 4-16
  dBm, 4-53
  dB\mu V, 4-54
  dBmV, 4-54
  Volts, 4-203
  Watts, 4-203
AMPL SCL LOG LIN, 4-15
Amptd Units, 4-16
ANNOTATN, 4-16
ANNOTATN ON OFF, 4-16
ANTENNA -> DISK, 4-17
Antenna Factors, 4-17
ANTENNA ON OFF, 4-17
Antenna Units, 4-18
APND CAT ITEM, 4-18
ATTEN AUTO MAN, 4-18
attenuation coupling, 4-19
attenuator-error factors, 4-176
AUTO ALL, 4-19
AUTO CAL ON OFF, 4-19
AUTO COUPLE, 4-20
AUTOEXEC ON OFF, 4-21
AUTO-MEASURE, 4-20
AUTO RANGE, 4-21
AUTORANG ON OFF, 4-21
Aux Conn Control, 4-22
AUX CTRL, 4-22
auxiliary connector input, 4-65
auxiliary interface
  connector, 4-22
  control line A, 4-44
  control line B, 4-44
  control line C, 4-44
  control line D, 4-45
available memory, 4-35
AV DWELL TIME, 4-22
AVERAGE, 4-23
average video bandwidth coupling, 4-19
AVG BW AUTO MAN, 4-23
AV/IF BW RATIO, 4-23
```

В BACKGRND, 4-24 Band Lock, 4-25 band locking, 4-28 bandwidth functions, 4-29 BAUD RATE, 4-25 B -> C, 4-24B < -> C, 4-24bias-current DAC adjustment, 4-33 binary, A-2 BLACK FILL, 4-26 BLACK LEVEL, 4-26 BLANK A, 4-26 BLANK B, 4-27 BLANK C, 4-27 BLUE, 4-27 BLUE FILL, 4-27 B-DL -> B, 4-24BND LOCK ON OFF, 4-28 BRIGHT, 4-28 BW, 4-29

 $\mathbf{C}$ CABLE -> DISK, 4-29 Cable Factors, 4-29 CABLE ON OFF, 4-30 CAL 85422, 4-30 CAL 85462, 4-30 CAL ALL, 4-30 CAL AMP, 4-31 Cal At Time, 4-31 CAL CHECK, 4-31 CAL FETCH, 4-31 CAL FREQ, 4-32 CALIBRATE, 4-32 calibration attenuator-error factors, 4-176 CAL INPUT 1, 4-32 CAL INPUT 2, 4-32 CAL MXR, 4-2, 4-33 CAL STORE, 4-33 CAL TIMEBASE, 4-2, 4-33 CAL TRK GEN, 4-34 CAL YTF, 4-34 CATALOG ALL, 4-34 CATALOG DISK, 4-35 Catalog Internal, 4-35 CATALOG PREFIX, 4-37 CATALOG REGISTER, 4-37 CATALOG VARIABLS, 4-38 CENTER FREQ, 4-38 center frequency, 4-38 window zone, 4-206 center-frequency step size, 4-38 CF STEP AUTO MAN, 4-38

change prefix

edit done, 4-70 Change Prefix, 4-39 Change Title, 4-40 characters, 4-13, 4-90, 4-190, 4-206 CLEAR ANNOTATN, 4-41 clearing a service request, A-1 clearing the active function, 4-93 CLEAR MARK, 4-41 CLEAR WRITE A, 4-41 CLEAR WRITE B, 4-42 CLEAR WRITE C, 4-43 CLR ALL MARKS, 4-43 CNTL A 0 1, 4-44 CNTL B 0 1, 4-44 CNTL C 0 1, 4-44 CNTL D 0 1, 4-45 CNT RES AUTO MAN, 4-51 COARSE TUNE DAC, 4-2, 4-45 COLOR BARS, 4-45 COLOR MONOCHRM, 4-46 command complete, A-1 commands front panel execution, 4-78 COMPLMNT MARKS, 4-46 CONFIG, 4-46 CONFIG DONE, 4-47 configuration plotter, 4-137 printer, 4-148 connector, auxiliary interface, 4-22 continuous sweep, 4-190 control line A auxiliary interface, 4-44 control line B auxiliary interface, 4-44 control line C auxiliary interface, 4-44 control line D auxiliary interface, 4-45 COPY, 4-47 COPY DEV PRNT PLT, 4-49 COPY SCREEN, 4-50 correction factors, 4-50 data display, 4-65 default, 4-54 self-calibration, 4-31 storing, 4-33 Correctn Factors, 4-50 CORRECTN ON OFF, 4-51 CORRECT ON OFF, 4-50 COUPLE AC DC, 4-51 coupled functions menu, 4-20 coupled sweep time, 4-192 coupling ac or dc, 4-51

all functions, 4-19 creating new programs, 4-129

# D DAC bias current adjustment, 4-33 extra fine-tune, 4-204 fine tune, 4-82 mixer bias, 4-125 sweep time, 4-191 YTF coarse tune, 4-205 YTF fine-tune, 4-205 DACS, 4-2, 4-53 data recall, 4-154 DATEMODE MDY DMY, 4-53 dBm, 4-53 $dB\mu V$ , 4-54 dBmV, 4-54 dc coupling, 4-51 deactivating the active function, 4-93 DEFAULT CAL DATA, 4-54 DEFAULT COLORS, 4-55 DEFAULT CONFIG, 4-55 Define List, 4-56 Define Report, 4-56 DEFINE USER KEY, 4-56 DELETE ALL SIGS, 4-57 DELETE FACTORS, 4-57 DELETE FILE, 4-57 DELETE LIMIT, 4-59 DELETE MARKED, 4-59 DELETE POINT, 4-59 DELETE SEGMENT, 4-60 DELETE SIGNAL, 4-60 Delete Signals, 4-61 delta marker, 4-115 DELTA MEAS, 4-61 DEMOD AM FM, 4-61 DEMOD ON OFF, 4-62 demodulation AM, 4-61 dwell time, 4-68 FM, 4-61 FM gain, 4-84 FM offset, 4-84 FM span, 4-85 on and off, 4-62 speaker on off, 4-185 squelch, 4-185 DESKJET, 4-62 DESKJET 500, 4-62 DESKJET 500C, 4-63 DESKJET 550C, 4-63 detection mode positive peak, 4-64

sample, 4-64 detector quasi peak, 4-152 DETECTOR PK QP AV, 4-63 DETECTOR SMP PK, 4-64 disable peak detector reset, 4-67 Disk Config, 4-64 display two windows, 4-52 DISPLAY, 4-64 DISPLAY CAL DATA, 4-2, 4-65 DISPLAY CNTL I, 4-65 Display Config, 4-66 DISPLAY -> DISK, 4-65 display line, 4-67 Display Sys Data, 4-2, 4-66 display zone change span, 4-208 find left peak, 4-207 find right peak, 4-207 move center, 4-206 DISPOSE USER KEY, 4-66 Dispose User Mem, 4-66 DLP editor, 4-76 DLP editor function appending, 4-18 double display, 4-52 DROOP, 4-2, 4-67 DSP LINE ON OFF, 4-67 DWELL TIME, 4-68

# $\mathbf{E}$ EDIT ANNOTATN, 4-68 EDIT ANTENNA, 4-68 EDIT CABLE, 4-69 EDIT CAT ITEM, 4-69 Edit Colors, 4-69 EDIT DONE, 4-70 EDIT FLATNESS, 4-2, 4-71 editing DLPs, 4-76 EDIT LAST, 4-71 Edit Limit, 4-72 EDIT LIMIT, 4-72 EDIT LIST, 4-72 EDIT LOWER, 4-73 EDIT MID/DELT, 4-73 Editor, 4-76 EDIT OTHER, 4-74 EDIT PA FLATNESS, 4-2, 4-74 EDIT UP/LOW, 4-74 EDIT UPPER, 4-75 EDIT UPR LWR, 4-75 EMI bandwidth

120 kHz, 4-10 200 Hz, 4-11 9 kHz, 4-8 EMI RECEIVER, 4-76 end of sweep, A-1 EPSON MX, 4-77 ERASE STATEALL, 4-77 ERASE TRACEALL, 4-77 erase user programs and variables, 4-66 error messages, 5-1 ERRORS, 4-77 errors, non recoverable, 5-14 exchange trace A and B, 4-11 exchange trace B and C, 4-24 execute a command front panel, 4-78 EXECUTE TITLE, 4-2, 4-78 EXIT, 4-78 EXIT CATALOG, 4-78 EXIT EDIT, 4-79 EXIT GRAPH, 4-79 EXIT LAST CAL, 4-80 EXIT MEASURE, 4-80 EXIT SHOW, 4-80 expanding a window, 4-208 EXTERNAL, 4-81 external/internal leveling, 4-14 EXTERNAL PREAMPG, 4-81

fast Fourier transform, 4-82 fatal errors, 5-14 FFT MEAS, 4-82 FINE TUNE DAC, 4-2, 4-82, 4-204 fixed, limit line type, 4-105 FLAT, 4-83 flatness factory defaults, 4-95 flatness correction constants, 4-71, 4-83 Flatness Data, 4-2, 4-83 floppy disk delete file, 4-57 FM COIL DRIVE, 4-2, 4-84 FM GAIN, 4-2, 4-84 FM OFFSET, 4-2, 4-84 FM SPAN, 4-2, 4-85 format date, 4-53 FORMAT DOS DISK, 4-85 FORMAT LIF DISK, 4-85 FREE RUN, 4-86 FREQ DIAG, 4-2, 4-86 FREQ OFFSET, 4-87 FREQ SCL LOG LIN, 4-87 FREQ STEP, 4-88 frequency

F

stop, 4-188
FREQUENCY, 4-88
frequency demodulation, 4-61
frequency, improving accuracy, 4-111
frequency offset, 4-87
frequency span, 4-184
changing to full span, 4-89
front panel execution of programming commands, 4-78
FRQ DISC NORM OFF, 4-2, 4-86
FRQ SCAN ON OFF, 4-89
FULL SPAN, 4-89
FULL WHITE, 4-89
function coupling, 4-19

Gauss, 4-90
GEO DST TEST, 4-90
GHIJKL, 4-90
GND REF DETECTOR, 4-2, 4-90
GRATICUL, 4-91
GRAT ON OFF, 4-91
GRAY SCALE, 4-91
GREEN, 4-92
GREEN FILL, 4-92
GRID, 4-92

 $\mathbf{H}$ HALF FILL, 4-93 hardware broken, A-1 hardware error messages, 5-1 harmonic band menu, 4-25 harmonic band slope and offset adjust, 4-34 harmonic lock, 4-28 highest peak finding next, 4-130 highest signal peak, 4-184 HI VOLT TEST, 4-93 HOLD, 4-93 HORIZ LINES, 4-93 HP Paintjet, 4-135 HSL RGB, 4-94 HUE, 4-94

I IDNUM, 4-2, 4-94
IF BW AUTO MAN, 4-95
IF GAINS, 4-2, 4-95
illegal spectrum analyzer command, A-1
informational messages, 5-1
INIT FLT, 4-2, 4-95
INPT LOCK ON OFF, 4-96
Input, 4-96
INPUT, 4-96
INPUT 1, 4-96
INPUT 1 9k-50M, 4-97
INPUT 1 PREAMP, 4-97
INPUT 2, 4-97

INPUT 2 1-6.5G, 4-98 INPUT 2 20M-2.9G, 4-97 INPUT 2 BYPASS, 4-98 INPUT 2 PREAMP, 4-98 input and output auxiliary control, 4-22 input attenuation control, 4-18 input impedance, 4-99 INPUT Z  $50\Omega$   $75\Omega$ , 4-99 instrument preset, 4-142 Inst Setup, 4-99 INTENSITY, 4-99 intermeditate frequency bandwidth coupling, 4-19 internal/external leveling, 4-14 internal memory, 4-35 cataloging functions, 4-35 catalog variables, 4-38 delete file, 4-57 erase user programs and variables, 4-66 program and variable cataloging, 4-34 saving to, 4-197 state and trace register status, 4-37 INTERNAL -> STATE, 4-100 Internal -> Trace, 4-100

## **K** key menus, 3-1, 3-2-21

 $\mathbf{L}$ LASERJET, 4-101 LASERJET II. 4-101 LASERJET III, 4-101 Last Cal, 4-101 Last Hrd Key Menu, 4-102 LAST SPAN, 4-102 Limit 1, 4-102 LIMIT 1 ON OFF, 4-103 Limit 2, 4-103 LIMIT 2 ON OFF, 4-103 LIMIT LINE 1, 4-104 limit lines delete point, 4-59 delete segment, 4-60 displaying, 4-108 edit lower table, 4-73 edit mid/delta amplitude, 4-73 edit table, 4-72 edit upper and lower tables, 4-74, 4-75 edit upper table, 4-75 fixed and relative, 4-105 flat type, 4-83 point, 4-138 purge, 4-150 recall table, 4-156 save table, 4-164 select amplitude, 4-168

select frequency, 4-170 select frequency or time, 4-106 select lower amplitude, 4-171 select middle amplitude, 4-171 select segment, 4-173 select type, 4-174 select upper amplitude, 4-175 slope type, 4-181 testing, 4-109 Limit Lines, 4-104 LIMIT LINES, 4-104 LIMITS -> DISK, 4-105 LIMITS FIX REL, 4-105 LIMITS FRQ TIME, 4-106 LINE, 4-107 LINEARITY, 4-107 LINEARITY CHECK, 4-107 linear scale, 4-167 linear sweep, 4-190 LIN ON OFF, 4-107 LIST -> DISK, 4-108 LIST ON OFF, 4-108 LMT DISP Y N AUTO, 4-108 LMT TEST ON OFF, 4-109 LOAD FILE, 4-109 (LOCAL), 4-46, 4-110 local operation, 4-46, 4-110 lock harmonic band, 4-28 lock internal state and trace registers, 4-167 logarithmic sweep, 4-190 LOGF SPD, 4-111 LOG ON OFF, 4-111 log scale, 4-167 lower limit line editing, 4-73 LUMIN-OSITY, 4-111 MAIN COIL DR, 4-2, 4-112 MAIN SPAN, 4-2, 4-112 MAN TRK ADJUST, 4-112 manual tracking adjustment, 4-112 MARGIN 1 ON OFF, 4-113 MARGIN 2 ON OFF, 4-113 MARK ALL DUPLICAT, 4-113 MARK ALL SIGNALS, 4-114

MARGIN 1 ON OFF, 4-113
MARGIN 2 ON OFF, 4-113
MARK ALL DUPLICAT, 4-113
MARK ALL SIGNALS, 4-114
marker
menu of controls, 4-126
selection, 4-168
trace selection, 4-127
MARKER, 4-115
MARKER 1 ON OFF, 4-118
MARKER 2 ON OFF, 4-118
MARKER 3 ON OFF, 4-119
MARKER 4 ON OFF, 4-119

M

MARKER ALL OFF, 4-119 MARKER AMPTD, 4-120 MARKER -> CF, 4-116 MARKER -> CF STEP, 4-116 marker counter, 4-125 MARKER FUNCTION, 4-120 MARKER ->MINIMUM, 4-117 marker noise, 4-126 MARKER NORMAL, 4-120 marker pause, 4-126 dwell time, 4-68 MARKER -> PK-PK, 4-117 marker readout modes, 4-127 MARKER -> REF LVL, 4-117 MARKERS, 4-121 MARKER ->START, 4-118 MARKER ->STOP, 4-118 marker tracking, 4-128 MARKER TUNE SPN, 4-121 MARKER  $\Delta$ , 4-115 MARKER ΔSPAN, 4-116 MARK LWR DUPLICAT, 4-114 MARK SIGNAL, 4-114 MARK TO END, 4-114 MAX HOLD A, 4-122 MAX HOLD B, 4-122 maximum mixer level, 4-122 MAX MXR LVL, 4-122 MEAS SNG CONT, 4-123 MEAS STEPPED, 4-123 MEASURE AT MKR, 4-124 Measure Detector, 4-124 MEAS/USER, 4-123 MEM LOCKED, 4-124, 4-167 memory amount available, 4-35 menus, 3-1  $\mu$ A/m, 4-5  $\mu V/m$ , 4-5 mid/delta limit line editing amplitude, 4-73 MIN HOLD C, 4-125 minimizing scan time, 4-111 minimum to marker, 4-117 -10V REF DETECTOR, 4-2 MIXER BIAS DAC, 4-2, 4-125 mixer input level maximum, 4-122 MK COUNT ON OFF, 4-125 MK NOISE ON OFF, 4-126 MK PAUSE ON OFF, 4-126 MKR, 4-126 MKR ->, 4-127MK READ F T I P, 4-127 MK TRACE AUTO ABC, 4-127 MK TRACK ON OFF, 4-128

MNOPQR, 4-128 MODE, 4-129 MONO-CHROME, 4-129 move trace A into C, 4-12 multipen plotter, 4-48

N NEW EDIT, 4-129
NEXT, 4-130
NEXT PAGE, 4-130
NEXT PEAK, 4-130
NEXT PK LEFT, 4-130
NEXT PK RIGHT, 4-131
NO CONVERSN, 4-131
non recoverable errors, 5-14
normal marker, 4-120
NORMLIZE ON OFF, 4-132
NORMLIZE POSITION, 4-132
No User Menus, 4-131

O octal to binary, A-2
ON/OFF, 4-132
operation
local, 4-110
OPTICAL FILTER, 4-133
optimizing frequency accuracy, 4-111
OTHER -> DISK, 4-133
Other Factors, 4-133
OTHER ON OFF, 4-134
OUTPUT, 4-134
output power, 4-186
OUTPUT REPORT, 4-134
output screen data, 4-47
OVLD ON OFF, 4-134

P PAINTJET PRINTER, 4-135 PALETTE BARS, 4-135 parallel polling, A-1 pass code, 4-54 peak next, 4-130 next left, 4-130 next right, 4-131 peak detection mode positive/negative, 4-64 PEAK EXCURSN, 4-135 Peak Menu, 4-136 peak response routine, 4-197 peak search outside of the zone, 4-207 PEAK SEARCH, 4-136 peak to peak measurement, 4-117 percent amplitude modulation, 4-4 phase lock on/off, 4-4  $\phi$  LOCK ON OFF, 4-2, 4-4

```
PK DWELL TIME, 4-136
PK-PK MEAS, 4-137
Plot Config, 4-137
PLOTTER ADDRESS, 4-137
plotter configuration, 4-46
plotting, 4-47, 4-49
PLT MENU ON OFF, 4-138
PLTS/PG 1 2 4, 4-138
POINT, 4-138
point deletion, 4-59
positive peak detection mode, 4-64
POWER ON IP LAST, 4-139
power-on state of spectrum analyzer, 4-139
PREAMP, 4-140
preamplifier gain, 4-81
PREAMP ON OFF, 4-140
predetermined correction factors, 4-54
prefix
 catalog of, 4-37
 entry, 4-39
 selection, 4-172
PRESEL DAC, 4-2, 4-141
PRESEL DEFAULT, 4-141
preselector default, 4-141
preselector peak, 4-141
PRESEL PEAK, 4-141
PRESET, 4-142
preset conditions
 receiver, 4-142
 signal analysis, 4-143
preset conditions receiver mode, 4-142
preset conditions signal analysis mode, 4-143
PRESET RECEIVER, 4-145
PRESET SPECTRUM, 4-146
Print Config, 4-148
printer
 HP Paintiet, 4-47
PRINTER ADDRESS, 4-148
printer configuration, 4-46
PRINTER SETUP, 4-148
Printer Type, 4-149
printing, 4-47, 4-49
 HP PaintJet, 4-135
print menu, 4-150
Print Options, 4-148
PRN/PG 12, 4-149
program cataloging, 4-34
program (DLP) editor, 4-76
program editing and creating, 4-76
programming command
 front panel execution, 4-78
PROTECT ON OFF, 4-149
PRT MENU ON OFF, 4-150
pTesla, 4-150
PURGE LIMITS, 4-150
```

```
\mathbf{Q}
     QP/AVG 10X OFF, 4-152
     QP DET ON OFF, 4-3, 4-152
     QPD OFFSET, 4-3, 4-153
     QPD RST ON OFF, 4-3, 4-153
     QP DWELL TIME, 4-152
     QP GAIN ON OFF, 4-3, 4-153
     quasi-peak
       detector, 4-152
     QUASI-PEAK, 4-154
     QUIETJET, 4-154
R
     real-time clock, 4-193
       set date, 4-176
       set time, 4-177
       time and date display, 4-193
     RECALL, 4-154
     RECALL ANTENNA, 4-154
     RECALL CABLE, 4-155
     RECALL COLORS, 4-155
     Recall Disk, 4-155
     recalling a trace from internal memory, 4-100
     Recall Internal, 4-156
     RECALL LIMITS, 4-156
     RECALL LIST, 4-156
     RECALL OTHER, 4-157
     RECALL SETUP, 4-157
     RECALL TRACE, 4-157
     RECEIVER ADDRESS, 4-158
     receiver auto-coupled sweep time, 4-191
     RED, 4-158
     RED FILL, 4-158
     reference detector
       2V, 4-6
       ground, 4-90
     reference level, 4-158
     reference level offset, 4-159
     REF LVL, 4-158
     REF LVL OFFSET, 4-159
     relative, limit line type, 4-105
     REMEAS ALL SIGS, 4-159
     REMEAS MARKED, 4-160
     REMEAS SIGNAL, 4-160
     Re-measure, 4-160
     remote command
       front panel execution, 4-78
     remote operation, 4-46
     RESOLUTN LOW HIGH, 4-161
     RESTART, 4-161
```

 $\mathbf{S}$ sample detection mode, 4-64 SATUR-ATION, 4-161 SAVE, 4-162 SAVE ANTENNA, 4-162 SAVE CABLE, 4-162 SAVE COLORS, 4-163 save current state state register, 4-187 saved analyzer state, 4-100 Save Disk, 4-163 SAVE EDIT, 4-163 Save Internal, 4-164 SAVE LIMITS, 4-164 SAVE LIN GRAPH, 4-164 SAVE LIST, 4-165 SAVE LOG GRAPH, 4-165 SAVE OTHER, 4-166 Save/Rcl\ List, 4-166 SAVE SETUP, 4-166 saving to internal memory, 4-197 SAV LOCK ON OFF, 4-167 SCALE LOG LIN, 4-167 scan time, minimizing, 4-111 screen annotation on or off, 4-16 screen characters, 4-90, 4-128, 4-190, 4-206 screen data output, 4-47 screen graticule, 4-91 screen title, 4-40 characters, 4-13 segment deletion, 4-60 SELECT, 4-168 SELECT 1 2 3 4, 4-168 SELECT AMPLITUD, 4-168 Select Axis, 4-169 SELECT DELT AMP, 4-169 SELECT FREQ, 4-170 SELECT FRM LIST, 4-171 SELECT LWR AMPL, 4-171 SELECT MID AMPL, 4-171 SELECT POINT, 4-172 SELECT PREFIX, 4-172 SELECT SEGMENT, 4-173 SELECT TYPE, 4-174 SELECT UPR AMPL, 4-175 Selectv Mark, 4-175 self-calibration routines correction factors, 4-31 tracking generator, 4-34 serial polling, A-1 Service Cal, 4-2, 4-176 Service Diag, 4-2, 4-176 service functions, 4-2 Service Cal, 4-2 Service Diag, 4-2

service request, A-1 clearing, A-1 SET ATTN ERROR, 4-2, 4-176 SET DATE, 4-176 **SET TIME**, 4-177 SETTINGS ON OFF, 4-177 setup printer, 4-148 SETUP, 4-177 SETUP -> DISK, 4-178 SHOW COR ON OFF, 4-179 SHOW DET PK QP AV, 4-179 SHOW MKR ON OFF, 4-179 SHOW SETUP, 4-180 SHOW  $\Delta 1$  PK QP AV, 4-178 SHOW  $\Delta 2$  PK QP AV, 4-178 SHW INST CONFIG, 4-180 SIG LIST ON OFF, 4-180 SIGNAL ANALYSIS, 4-181 Signal Marking, 4-181 signal peak highest, 4-184 SINGLE, 4-181 single sweep, 4-190 SLOPE, 4-181 softkey locations, 3-1 SOFTKEYS, 4-182 SORT BY AVG AMP, 4-182 SORT BY DLTA LIM, 4-183 SORT BY FREQ, 4-182 SORT BY PK AMP, 4-183 SORT BY QP AMP, 4-183 Sort Signals, 4-183 source power, 4-186 space character, 4-206 span 0 Hz, 4-206 LAST SPAN, 4-102 window zone, 4-208 SPAN, 4-184 SPAN ZOOM, 4-184 SPEAKER ON OFF, 4-185 Special Colors, 4-185 spectrum analyzer configuration default, 4-55 spectrum analyzer state recalled, 4-139 split screen, 4-52 SQUELCH, 4-185 SRC ATN MAN AUTO, 4-186 SRC PWR OFFSET, 4-186 SRC PWR ON OFF, 4-186 SRC PWR STP SIZE, 4-187 SRQ, A-1 standard timebase, 4-33

start and stop frequencies, 4-116 START FREQ, 4-187 STATE -> INTRNL, 4-187 state of spectrum analyzer at power on, 4-139 state registers locking, 4-167 STATUS, 4-188 status byte, A-1 status byte definition, A-1 STEP LOG LIN, 4-188 step size, center frequency, 4-38 step-size coupling, 4-19 stimulus response mode, 4-191 STOP, 4-188 STOP FREQ, 4-188 store correction factors, 4-33 STORE FLATNESS, 4-2, 4-189 STOR PWR ON UNITS, 4-2, 4-189 STP GAIN ZERO, 4-3, 4-189 STUVWX, 4-190 subtract display line from trace B, 4-24 subtract trace B from A, 4-12 SWEEP, 4-190 sweep control continuous, 4-190 single, 4-190 SWEEP CONT SGL, 4-190 SWEEP LOG LIN, 4-190 SWEEP RAMP, 4-3, 4-191 sweep time, 4-192 sweep time coupling, 4-19 SWEEP TIME DAC, 4-3, 4-191 switch trace A and B, 4-11 SWP CPLG SR RECV, 4-191 SWP TIME AUTO MAN, 4-192 TEST, 4-192 Test Patterns, 4-192 THINKJET, 4-193 ThinkJet Printer mode switch settings, 4-47 THRESHLD ON OFF, 4-193 threshold line, 4-193 Time Date, 4-193 TIMEDATE ON OFF, 4-194 trace A -> C, 4-12A < -> B, 4-11A-B -> A, 4-12blank trace A, 4-26 blank trace B, 4-27 blank trace C, 4-27 B-DL -> B, 4-24clear write trace A, 4-41 clear write trace B, 4-42

Т

```
clear write trace C, 4-43
  move trace B into C, 4-24
  view mode, 4-200
TRACE, 4-194
trace A
  maximum hold, 4-122
TRACE A, 4-195
TRACE A B C, 4-194
trace B
  maximum hold, 4-122
TRACE B, 4-195
TRACE C, 4-196
Trace -> Disk, 4-196
Trace -> Intrnl, 4-197
trace registers
  locking, 4-167
TRACK GEN, 4-197
tracking generator
  frequency adjustment, 4-112
  internal/external leveling, 4-14
  output power, 4-186
  peak response, 4-197
  power sweep, 4-151
  power sweep range, 4-187
  self-calibration, 4-34
  source attenuator, 4-186
  source power offset, 4-186, 4-187
  source power step size, 4-187
TRACKING PEAK, 4-197
TRIG, 4-198
trigger, 4-198
  external, 4-81
  free run, 4-86
  line, 4-107
  video, 4-200
TUNE SLO FAST, 4-198
turning off markers, 4-119
turning off windows display, 4-204
two display windows, 4-52
type of limit line, 4-174
underscore
  character, 4-206
UNDO, 4-198
unit key pressed, A-1
units, amplitude, 4-16
universal HP-IB service request, A-1
upper and lower limit lines
  editing, 4-74
user-created error messages, 5-1
User Menus, 4-199
```

U

V variable cataloging, 4-34 VERT LINES, 4-199 VID AVG ON OFF, 4-199 VIDEO, 4-200 video averaging, 4-199 VIEW A, 4-200 VIEW B, 4-201 VIEW C, 4-201 VIEW CAL ON OFF, 4-201 VIEW PK QP AV, 4-202 VIEW Δ OFF, 4-200 VISION ENHANCE1, 4-202 VOIts, 4-203

W Watts, 4-203 WHITE DOTS, 4-203 WHITE FILL, 4-203 windows ON, 4-52 ZOOM, 4-208 WINDOWS OFF, 4-204

## X X FINE TUNE DAC, 4-3

Y YTF DRIVER, 4-3, 4-204 YTF slope and offset adjustment, 4-34 YTF SPAN, 4-3, 4-205 YTF TUNE COARSE, 4-3, 4-205 YTF TUNE FINE, 4-3, 4-205 YZ_# Spc Clear, 4-206

Z ZERO SPAN, 4-206 ZONE CENTER, 4-206 ZONE PK LEFT, 4-207 ZONE PK RIGHT, 4-207 ZONE SPAN, 4-208 ZOOM, 4-208 zooming a window, 4-208