



Agilent Technologies
E1472A/73A/74A/75A
50 Ohm and 75 Ohm
RF Multiplexers/Expanders
User's Manual



Agilent Technologies

Manual Part Number: E1472-90003
Printed September 2012
Printed in Malaysia E0912

NOTICE: In August 2014, Agilent Technologies' former Test and Measurement business became Keysight Technologies. This document is provided as a courtesy but is no longer kept current and thus will contain historical references to Agilent. For more information, go to **www.keysight.com**.



Contents

E1472A/73A/74A/75A RF Multiplexers User's Manual

| | |
|--|-----------|
| Front Matter..... | 5 |
| Agilent Technologies Warranty Statement | 5 |
| U.S. Government Restricted Rights | 5 |
| Documentation History | 6 |
| Safety Symbols | 6 |
| Warnings | 6 |
| Chapter 1 - Getting Started | 9 |
| Using This Chapter | 9 |
| How to Use this Manual | 9 |
| RF Multiplexers Description | 10 |
| General Description | 11 |
| Basic Operation | 11 |
| Typical Configuration | 12 |
| Instrument Definition | 12 |
| Programming the RF Multiplexers..... | 13 |
| Addressing the Multiplexers | 13 |
| Initial Operation | 16 |
| Chapter 2 - Configuring the RF Multiplexers | 17 |
| Using This Chapter | 17 |
| Warnings and Cautions..... | 17 |
| Setting the Address Switch | 18 |
| Selecting the Interrupt Priority..... | 19 |
| Expanding the RF Multiplexer | 20 |
| Selecting the Relay Drive Level..... | 22 |
| Connecting User Inputs to E1472A/E1473A..... | 24 |
| Cabling Guidelines | 24 |
| Connecting User Inputs to E1474A/E1475A..... | 25 |
| Cabling Guidelines | 25 |
| Cables and Connectors | 28 |
| Cables | 28 |
| Connectors | 29 |
| Chapter 3 - Using the RF Multiplexers | 31 |
| Using This Chapter | 31 |
| RF Multiplexer Commands..... | 31 |
| Switching Channels | 32 |
| Saving and Recalling States | 34 |
| Detecting Error Conditions | 34 |
| Synchronizing the RF Multiplexer | 36 |

| | |
|---|---------------|
| Chapter 4 - RF Multiplexer Command Reference | 37 |
| Using This Chapter | 37 |
| Command Types | 37 |
| Common Command Format | 37 |
| SCPI Command Format | 37 |
| SCPI Command Reference..... | 39 |
| [ROUTe:] | 40 |
| [ROUTe:]CLOSe | 40 |
| [ROUTe:]CLOSe? | 41 |
| [ROUTe:]OPEN? | 41 |
| SYSTem | 43 |
| SYSTem:CDEscription? | 43 |
| SYSTem:COPTion? | 43 |
| SYSTem:CPON | 44 |
| SYSTem:CTYPe? | 44 |
| SYSTem:ERRor? | 45 |
| Common Commands Quick Reference | 46 |
| SCPI Commands Quick Reference..... | 47 |
| Appendix A - RF Multiplexer Specifications | 49 |
| Appendix B - Register-Based Programming | 51 |
| About This Appendix..... | 51 |
| Addressing the Registers | 51 |
| Reading the Registers | 52 |
| Manufacturer ID Register | 52 |
| Device Type Register | 52 |
| Status/Control Register | 52 |
| Remote Module ID Registers | 53 |
| Channel Enable Registers | 53 |
| Writing to the Registers..... | 53 |
| Status/Control Register | 53 |
| Channel Enable Registers | 54 |
| Selecting Channels Using Your Own Relays | 57 |
| Appendix C - RF Multiplexer Error Messages | 61 |
| Appendix D - Relay Life | 63 |
| Replacement Strategy..... | 63 |
| Relay Life Factors | 63 |
| End-of-Life Determination | 63 |
| Index | 65 |

AGILENT TECHNOLOGIES WARRANTY STATEMENT

AGILENT PRODUCT: E1472A/73A/74A/75A RF Multiplexers

DURATION OF WARRANTY: 3 years

1. Agilent Technologies warrants Agilent hardware, accessories and supplies against defects in materials and workmanship for the period specified above. If Agilent receives notice of such defects during the warranty period, Agilent will, at its option, either repair or replace products which prove to be defective. Replacement products may be either new or like-new.
 2. Agilent warrants that Agilent software will not fail to execute its programming instructions, for the period specified above, due to defects in material and workmanship when properly installed and used. If Agilent receives notice of such defects during the warranty period, Agilent will replace software media which does not execute its programming instructions due to such defects.
 3. Agilent does not warrant that the operation of Agilent products will be interrupted or error free. If Agilent is unable, within a reasonable time, to repair or replace any product to a condition as warranted, customer will be entitled to a refund of the purchase price upon prompt return of the product.
 4. Agilent products may contain remanufactured parts equivalent to new in performance or may have been subject to incidental use.
 5. The warranty period begins on the date of delivery or on the date of installation if installed by Agilent. If customer schedules or delays Agilent installation more than 30 days after delivery, warranty begins on the 31st day from delivery.
 6. Warranty does not apply to defects resulting from (a) improper or inadequate maintenance or calibration, (b) software, interfacing, parts or supplies not supplied by Agilent, (c) unauthorized modification or misuse, (d) operation outside of the published environmental specifications for the product, or (e) improper site preparation or maintenance.
 7. TO THE EXTENT ALLOWED BY LOCAL LAW, THE ABOVE WARRANTIES ARE EXCLUSIVE AND NO OTHER WARRANTY OR CONDITION, WHETHER WRITTEN OR ORAL, IS EXPRESSED OR IMPLIED AND AGILENT SPECIFICALLY DISCLAIMS ANY IMPLIED WARRANTY OR CONDITIONS OF MERCHANTABILITY, SATISFACTORY QUALITY, AND FITNESS FOR A PARTICULAR PURPOSE.
 8. Agilent will be liable for damage to tangible property per incident up to the greater of \$300,000 or the actual amount paid for the product that is the subject of the claim, and for damages for bodily injury or death, to the extent that all such damages are determined by a court of competent jurisdiction to have been directly caused by a defective Agilent product.
 9. TO THE EXTENT ALLOWED BY LOCAL LAW, THE REMEDIES IN THIS WARRANTY STATEMENT ARE CUSTOMER'S SOLE AND EXCLUSIVE REMEDIES. EXCEPT AS INDICATED ABOVE, IN NO EVENT WILL AGILENT OR ITS SUPPLIERS BE LIABLE FOR LOSS OF DATA OR FOR DIRECT, SPECIAL, INCIDENTAL, CONSEQUENTIAL (INCLUDING LOST PROFIT OR DATA), OR OTHER DAMAGE, WHETHER BASED IN CONTRACT, TORT, OR OTHERWISE.
- FOR CONSUMER TRANSACTIONS IN AUSTRALIA AND NEW ZEALAND: THE WARRANTY TERMS CONTAINED IN THIS STATEMENT, EXCEPT TO THE EXTENT LAWFULLY PERMITTED, DO NOT EXCLUDE, RESTRICT OR MODIFY AND ARE IN ADDITION TO THE MANDATORY STATUTORY RIGHTS APPLICABLE TO THE SALE OF THIS PRODUCT TO YOU.

U.S. Government Restricted Rights

The Software and Documentation have been developed entirely at private expense. They are delivered and licensed as "commercial computer software" as defined in DFARS 252.227- 7013 (Oct 1988), DFARS 252.211-7015 (May 1991) or DFARS 252.227-7014 (Jun 1995), as a "commercial item" as defined in FAR 2.101(a), or as "Restricted computer software" as defined in FAR 52.227-19 (Jun 1987)(or any equivalent agency regulation or contract clause), whichever is applicable. You have only those rights provided for such Software and Documentation by the applicable FAR or DFARS clause or the Agilent standard software agreement for the product involved.



E1472A/73A/74A/75A RF Multiplexers User's Manual
Edition 4

Copyright © 1990-1992, 2000 Agilent Technologies, Inc. All rights reserved.

Documentation History

All Editions and Updates of this manual and their creation date are listed below. The first Edition of the manual is Edition 1. The Edition number increments by 1 whenever the manual is revised. Updates, which are issued between Editions, contain replacement pages to correct or add additional information to the current Edition of the manual. Whenever a new Edition is created, it will contain all of the Update information for the previous Edition. Each new Edition or Update also includes a revised copy of this documentation history page.

| | |
|------------------|----------------|
| Edition 1 | January, 1990 |
| Edition 2 | October, 1991 |
| Edition 3 | November, 1992 |
| Edition 4 | November, 2000 |
| Edition 4, Rev 1 | September 2012 |


Safety Symbols



Instruction manual symbol affixed to product. Indicates that the user must refer to the manual for specific **WARNING** or **CAUTION** information to avoid personal injury or damage to the product.



Indicates the field wiring terminal that must be connected to earth ground before operating the equipment — protects against electrical shock in case of fault.



Frame or chassis ground terminal—typically connects to the equipment's metal frame.



Alternating current (AC)



Direct current (DC).



Warning. Risk of electrical shock.

WARNING

Calls attention to a procedure, practice, or condition that could cause bodily injury or death.

CAUTION

Calls attention to a procedure, practice, or condition that could possibly cause damage to equipment or permanent loss of data.

WARNINGS

The following general safety precautions must be observed during all phases of operation, service, and repair of this product. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the product. Agilent Technologies assumes no liability for the customer's failure to comply with these requirements.

Ground the equipment: For Safety Class 1 equipment (equipment having a protective earth terminal), an uninterruptible safety earth ground must be provided from the mains power source to the product input wiring terminals or supplied power cable.

DO NOT operate the product in an explosive atmosphere or in the presence of flammable gases or fumes.

For continued protection against fire, replace the line fuse(s) only with fuse(s) of the same voltage and current rating and type. DO NOT use repaired fuses or short-circuited fuse holders.

Keep away from live circuits: Operating personnel must not remove equipment covers or shields. Procedures involving the removal of covers or shields are for use by service-trained personnel only. Under certain conditions, dangerous voltages may exist even with the equipment switched off. To avoid dangerous electrical shock, DO NOT perform procedures involving cover or shield removal unless you are qualified to do so.

DO NOT operate damaged equipment: Whenever it is possible that the safety protection features built into this product have been impaired, either through physical damage, excessive moisture, or any other reason, REMOVE POWER and do not use the product until safe operation can be verified by service-trained personnel. If necessary, return the product to Agilent for service and repair to ensure that safety features are maintained.

DO NOT service or adjust alone: Do not attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present.

DO NOT substitute parts or modify equipment: Because of the danger of introducing additional hazards, do not install substitute parts or perform any unauthorized modification to the product. Return the product to Agilent for service and repair to ensure that safety features are maintained.

Declaration of Conformity

Declarations of Conformity for this product and for other Agilent products may be downloaded from the Internet. There are two methods to obtain the Declaration of Conformity:

- Go to <http://regulations.corporate.agilent.com/DoC/search.htm> . You can then search by product number to find the latest Declaration of Conformity.
- Alternately, you can go to the product web page (www.agilent.com/find/E1472A), click on the Document Library tab then scroll down until you find the Declaration of Conformity link.

Notes:

Chapter 1

Getting Started

Using This Chapter

This chapter describes the RF Multiplexer and Expander modules and contains information on how to program them using Standard Commands for Programmable Instruments (SCPI). This chapter contains the following sections:

- How to Use This Manual.9
- RF Multiplexers Description10
- Programming the RF Multiplexers13

How to Use this Manual

This manual shows how to operate, configure, and program the E1472A 50 Ohm RF Multiplexer, E1473A 50 Ohm RF Multiplexer Expander, E1474A 75 Ohm RF Multiplexer, and E1475A 75 Ohm RF Multiplexer Expander modules. The RF Multiplexer is a VXIbus C-Size register-based slave device, and can operate in a C-size VXIbus mainframe using a command module such as the E1406. For other manufacturers' mainframes, refer to the applicable manual supplied by the manufacturer.

NOTE *Except where noted, the term “RF Multiplexer” refers to the E1472A 50 Ohm RF Multiplexer and E1474A 75 Ohm RF Multiplexer Modules. The term “Expander” refers to the E1473A 50 Ohm RF Multiplexer Expander, and E1475A 75 Ohm RF Multiplexer Expander Modules.*

Most information in this manual applies to RF Multiplexer operations in a command module. Standard Commands for Programmable Instruments (SCPI) is the programming language. For non-SCPI programming, see Appendix B for register-based programming.

RF Multiplexers Description

Figure 1-1 shows the 50 Ohm and 75 Ohm RF Multiplexer and 50 Ohm and 75 Ohm RF Multiplexer Expander modules switching diagram. During power off, power on and reset, channel 0 is connected to COM on each bank.

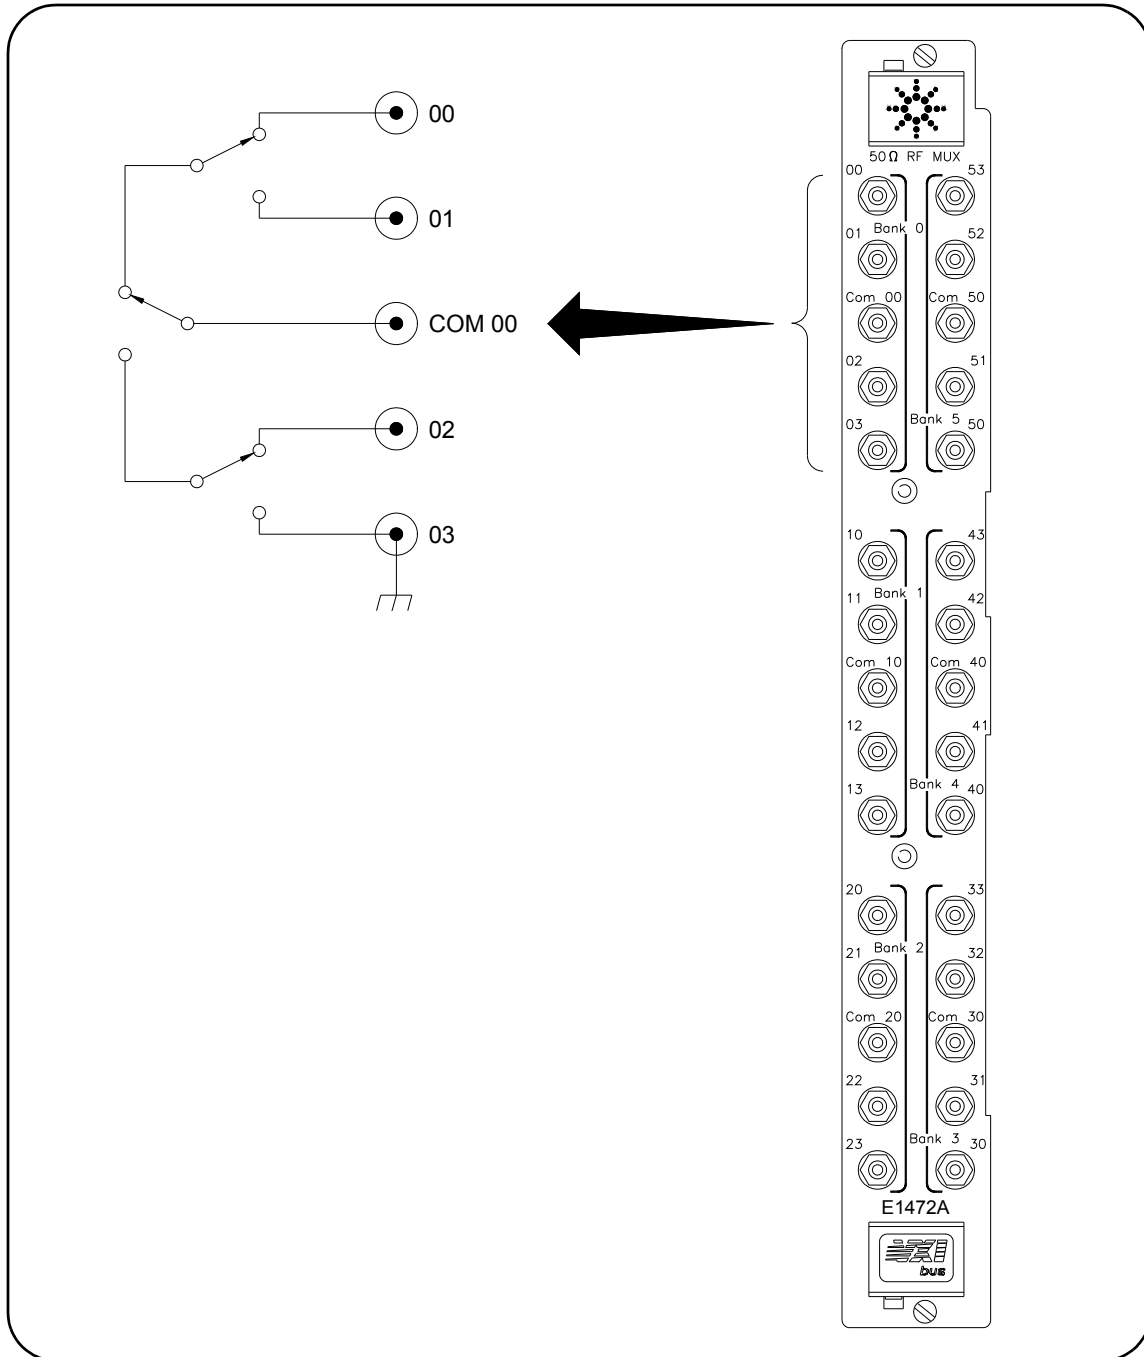


Figure 1-1. RF Multiplexers/Expanders Switching Diagram

General Description

The RF Multiplexer (6 x 4:1) and the Expander (6 x 4:1) modules are VXIbus C-Size register-based products which provide bidirectional switching for user inputs and outputs. Switching consists of connecting one channel to common in that bank. The RF Multiplexer can operate in a C-Size VXI mainframe using a command module such as an E1406.

Up to two Expander modules can be controlled by a single RF Multiplexer module, providing a total of eighteen (4:1) multiplexer banks. These Expander modules can either be inserted into the C-Size mainframe next to the RF Multiplexer, or can be located up to eight meters from the RF Multiplexer using the remote expander cables. Locating the Expander module close to the external device keeps connecting cable lengths to a minimum, thereby reducing the possibility of cross-talk and insertion loss of high frequency signals.

You may connect E1475A Expander or E1473A Expander to the E1472A or E1474A Multiplexer. The drivers on both modules can support either of the expander relay modules.

Basic Operation

The RF Multiplexer modules and Expander module consists of six banks of channels (bank 0 through bank 5) to form six 4:1 multiplexers. The switching sections of the RF Multiplexer and Expander modules are identical. See Figure 1-1 for a simplified switching diagram. Banks are arranged as follows:

- Bank 0 includes channels 00 through 03 and Com 00.
- Bank 1 includes channels 10 through 13 and Com 10.
- Bank 2 includes channels 20 through 23 and Com 20.
- Bank 3 includes channels 30 through 33 and Com 30.
- Bank 4 includes channels 40 through 43 and Com 40.
- Bank 5 includes channels 50 through 53 and Com 50.

In the remainder of this manual, channels are referred to as n0 through n3 and Com n0, where n is the bank number (0 through 5). Each channel is switched (connected to its common) by closing the appropriate (nonlatching) relays. Channels n0 through n3 can be switched to Com n0 for all banks. Only one channel in each bank can be connected to its common at a time.

User inputs/outputs to each channel are via SMB connectors. When a channel is CLOSeD, it is internally connected to the COMmon connector. When a channel is open, it is internally disconnected. Open channels are not terminated. At power-off, power-on, or reset, channel n0 is switched to the COM n0 connector, and all other channels (n1 through n3) are open (non-terminated) for all banks.

Typical Configuration

The RF Multiplexer and Expander relays are configured in a “tree” structure which provides high isolation and low VSWR (voltage standing wave ratio). Each channel can switch user inputs up to 24 Watts (42V peak). User input frequencies to the 50 Ohm RF Multiplexer and Expander modules can be from DC to 3 GHz. User input frequencies to the 75 Ohm RF Multiplexer and Expander modules can be from DC to 1.3 GHz. The RF Multiplexer can be configured for several arrangements, such as standard, tree, or matrix (see Chapter 4 for more information).

For a Standard Commands for Programmable Instruments (SCPI) environment, one or more RF Multiplexers (with or without Expanders connected) can be defined as a *switchbox* instrument. For a switchbox instrument, all RF Multiplexer channels within the instrument can be addressed using a single interface address.

Instrument Definition

Plug-in modules installed in a mainframe or used with a command module are treated as independent instruments each having a unique secondary GPIB address. Each instrument is also assigned a dedicated error queue, input and output buffers, status registers and, if applicable, dedicated mainframe/command module memory space for readings or data. An instrument may be composed of a single plug-in module (such as a counter) or multiple plug-in modules (for a Switchbox or Scanning Voltmeter Instrument).

Programming the RF Multiplexers

To program the RF Multiplexers using SCPI, you must select the controller language, interface address, and SCPI commands to be used. Guidelines to select SCPI commands for the RF Multiplexers follow. See the specific command module manual for interface addressing and controller language information.

NOTE *This discussion applies to SCPI programming. See Appendix B for details on programming RF Multiplexer registers.*

Addressing the Multiplexers

To address specific channels within an RF Multiplexer, you must specify the SCPI command and RF Multiplexer channel address. For the RF Multiplexer, use CLOSe (*channel_list*) to switch (connect) channels.

RF Multiplexer Channel Addresses

For the RF Multiplexer, the channel address (*channel_list*) has the form (@*ccmmnn*) where *cc* = RF Multiplexer card number (01-99), *mm* = RF Multiplexer/Expander module number (00-02), and *nn* = channel number (00-03, 10-13, 20-23, 30-33, 40-43, or 50-53). Use the form:

- (@*ccmmnn*) for a single channel
- (@*ccmmnn*,*ccmmnn*) for multiple channels

RF Multiplexer Card Numbers

The RF Multiplexer card number depends on the switchbox configuration (single-module or multiple-module) set for the RF Multiplexers. (Leading zeroes can be ignored for the card number.)

NOTE *The Expander module(s) card number is the same as the RF Multiplexer to which it is connected.*

- **Single-module.** For a single-module switchbox, the card number is always 01.
- **Multiple-module.** For a multiple-module switchbox, the RF Multiplexer module with the lowest logical address is always card number 01. The card number with the next successive logical address is 02, etc.

Figure 1-2 illustrates the card numbers and logical addresses of a typical multiple-module switchbox. The logical addresses in Figure 1-2 apply to RF Multiplexers installed in a VXI mainframe with a command module. See your specific command module manual for more information on switchboxes and logical addressing. For uses in other systems or mainframes, see the appropriate manuals.

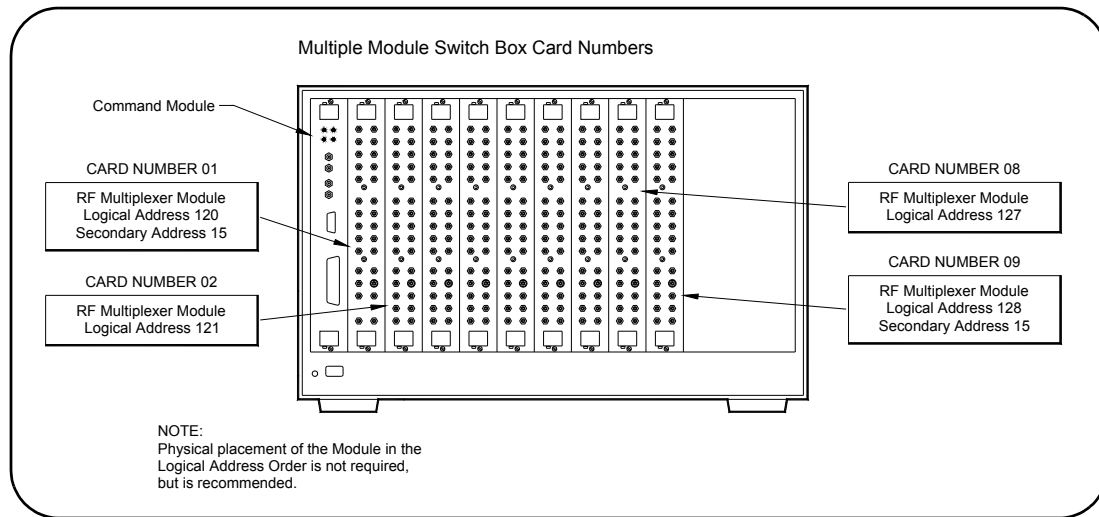


Figure 1-2. Card Numbers for Multiple-Module Switches

Module Numbers The module number identifies the module (RF Multiplexer, Expander #1, or Expander #2) within the card. The number depends on the desired module (RF Multiplexer, Expander #1, or Expander #2). Figure 1-3 illustrates the module numbers of a typical card.

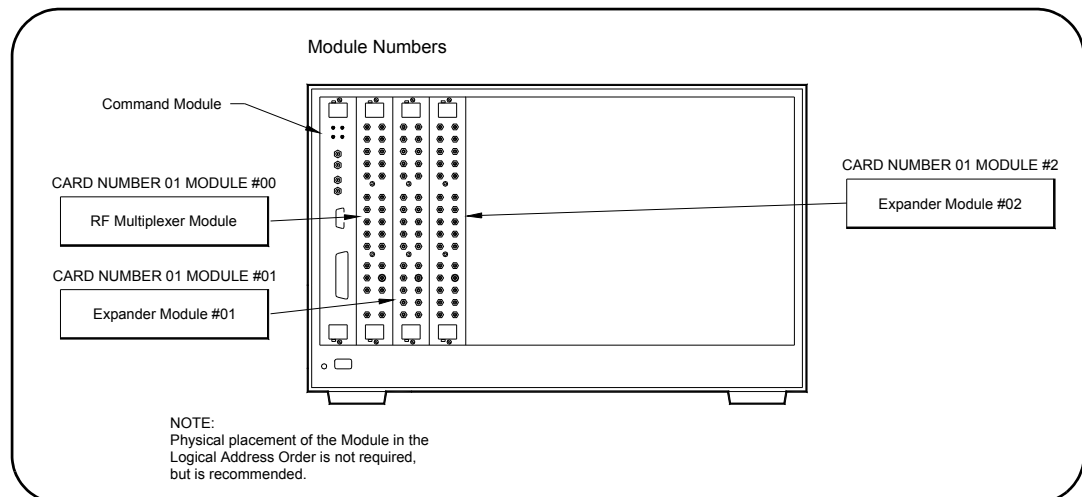


Figure 1-3. Typical Module Numbers

- **RF Multiplexer.** Module number is 00. If the RF Multiplexer does not have Expander module(s) connected, the module number can be omitted.
- **Expander module #1.** Module number is 01. Used to select the Expander module (if installed) connected to the RF Multiplexer RMD 3/RMD 2 internal ribbon connector.
- **Expander module #2.** Module number is 02. Used to select the Expander module (if installed) connected to the RF Multiplexer RMD 5/RMD 4 internal ribbon connector.

Channel Numbers

The channel numbers are 00-03, 10-13, 20-23, 30-33, 40-43, and 50-53. The channel is addressed using channel numbers. Use commas (,) to form a channel list. Only valid channels can be accessed in a channel list.

NOTE

The RF Multiplexer will accept and execute channel ranges (ccmmnn:ccmmnn) without generating an error, but the result is to close the last channel in each bank within the range specified. For example, after CLOSe (@010101:010151) is executed, card 01, module 01 channels 03, 13, 23, 33, 43, and 51 would remain closed.

Example: RF Multiplexer Channel List

Channel Lists:

CLOSe (@10001)

Connect channel 01 to COM 00 on the RF Multiplexer module, card 01.

CLOSe (@10101,20101)

Connect channel 01 to COM 00 on the Expander #1 module, cards 01 and 02.

SCPI Command Format

You can send SCPI commands in either short or long form. A long form example is:

CLOSe (@10102)

The same command shown without the lower case letters is the short form. The command then becomes:

CLOS (@10102)

Some commands are shown with brackets ([]). These are implied or optional commands you do not have to execute. For example, the ROUTe command is an implied command and is shown as:

[ROUT:]CLOS (@10102)

Thus, to execute these commands, enter:

CLOS (@10102)

See Chapter 3 for more information about SCPI commands and how to send them.

Initial Operation

You can use the following program example to verify initial RF Multiplexer operation by closing a channel and querying channel closure. The example first resets the switchbox and then closes channel 02 of a single RF Multiplexer module (card number 1) in the switchbox.

The program next queries the channel closure state. A returned "1" shows that the command to close the channel has been sent to the switchbox. A returned "0" shows that the command to close the channel has not been sent to the switchbox.

This example uses BASIC as the program language. The computer interfaces to the mainframe using GPIB. The GPIB interface select code is 7, the primary address is 09, and the secondary address is 15. See the specific command module user's guide for addressing information.

| | |
|--------------------------------|---|
| 10 OUTPUT 70915;"*RST" | <i>!Resets the module. Switches all channel n0 to COM n0.</i> |
| 20 OUTPUT 70915;"CLOS (@102)" | <i>!Connect channel 02 to COM 00.</i> |
| 30 OUTPUT 70915;"CLOS? (@102)" | <i>!Query channel 02.</i> |
| 40 ENTER 70915;Value | <i>!Enter results into value.</i> |
| 50 PRINT Value | <i>!Display results (should return "1").</i> |
| 60 END | <i>!End program.</i> |

Chapter 2

Configuring the RF Multiplexers

Using This Chapter

This chapter shows how to connect external wiring to the RF Multiplexer and Expander connectors and how to configure the modules for operation.

| | |
|--|----|
| • Warnings and Cautions | 17 |
| • Setting the Address Switch | 18 |
| • Selecting the Interrupt Priority | 19 |
| • Expanding the RF Multiplexer | 20 |
| • Selecting the Relay Drive Level | 22 |
| • Connecting User Inputs to E1472A/73A | 24 |
| • Connecting User Inputs to E1474A/75A | 25 |
| • Cables and Connectors | 28 |

Warnings and Cautions

WARNING

SHOCK HAZARD. Only service-trained personnel who are aware of the hazards involved should install, remove, or configure the RF Multiplexer. Before you remove any installed module, disconnect AC power from the mainframe and from other modules that may be connected to the RF Multiplexer.

CHANNEL WIRING INSULATION. All channels that have a common connection must be insulated so that the user is protected from electrical shock in the event that two or more channels are connected together. This means wiring for all channels must be insulated as though each channel carries the voltage of the highest voltage channel.

CAUTION

MAXIMUM POWER. The maximum power that can be applied to any SMB connector is 24 W (24 VA). The maximum voltage that can be applied to any SMB connector is 42V peak. The maximum current that can be applied to any SMB connector is 1A DC/AC RMS.

STATIC ELECTRICITY. Static electricity is a major cause of component failure. To prevent damage to the electrical components in the RF Multiplexer, observe anti-static techniques whenever removing a module from the mainframe or whenever working on a module.

Setting the Address Switch

The logical address switch (LADDR) factory setting is 120. You may have changed the setting during module installation. Valid address values are from 0 to 255. If the RF Multiplexer is used with a command module in a C-Size mainframe, see the command module user's guide for addressing information. Otherwise, see Figure 2-1 to change the setting.

NOTE *The address switch selected value must be a multiple of 8 if the module is the first module in a “switchbox” used in a VXL mainframe, and is being instructed by SCPI commands.*

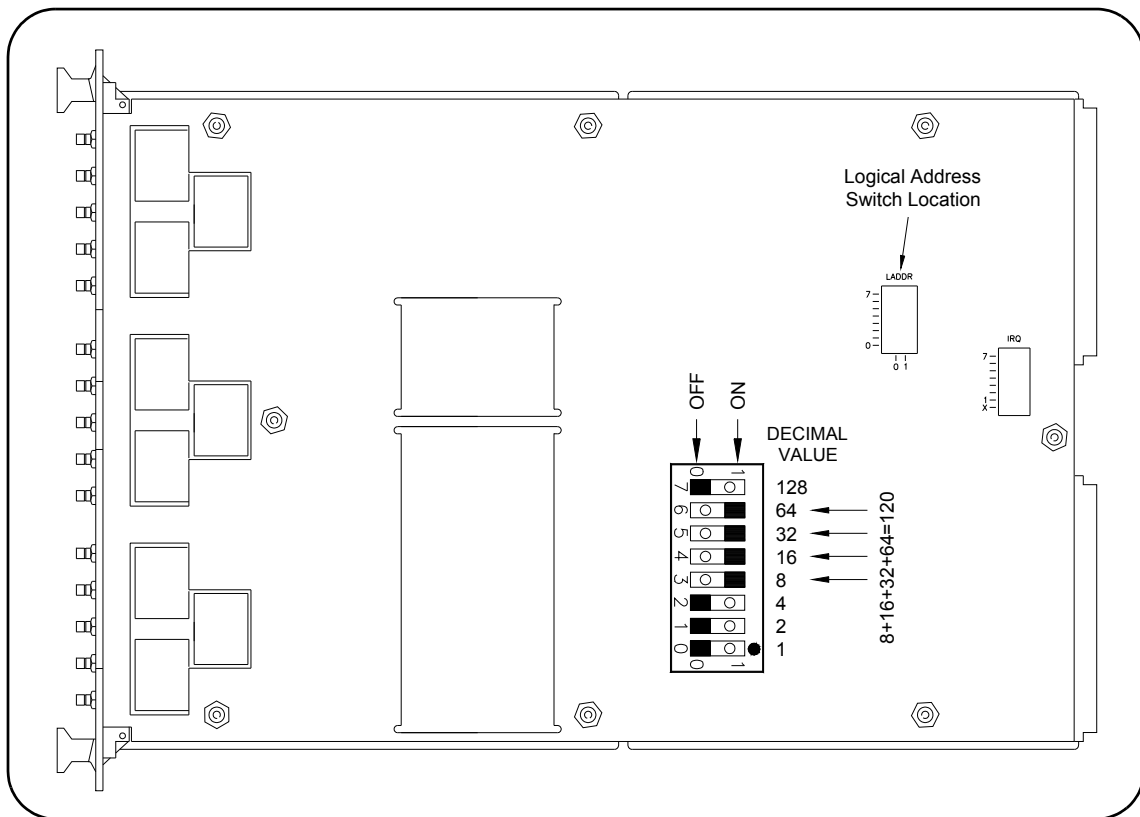


Figure 2-1. Address Selection

Selecting the Interrupt Priority

The RF Multiplexer module generates an interrupt after a channel has been closed. These interrupts are sent to, and acknowledgements are received from, the command module via the VXIbus backplane interrupt lines.

For most applications where the RF Multiplexer module is installed in a C-Size mainframe, the interrupt priority jumper does not have to be moved. This is because the VXIbus interrupt lines have the same priority and interrupt priority is established by installing modules in slots numerically closest to the command module. Thus, slot 1 has a higher priority than slot 2, slot 2 has a higher priority than slot 3, etc.

See Figure 2-2 to change the interrupt priority. You can select eight different interrupt priority levels. Level 1 is the lowest priority and Level 7 is the highest priority. Level X disables the interrupt. The module's factory setting is Level 1. To change, remove the 4-pin jumper (part number 1258-0247) from the old priority location and reinstall in the new priority location (Figure 2-2 shows a priority change from 1 to 7). If the 4-pin jumper is not used, the two jumper locations must have the same interrupt priority level selected (see Figure 2-2).

NOTE *Level X interrupt priority should not be used under normal operating conditions. Changing the priority level jumper is not recommended. Do not change unless specifically instructed to do so.*

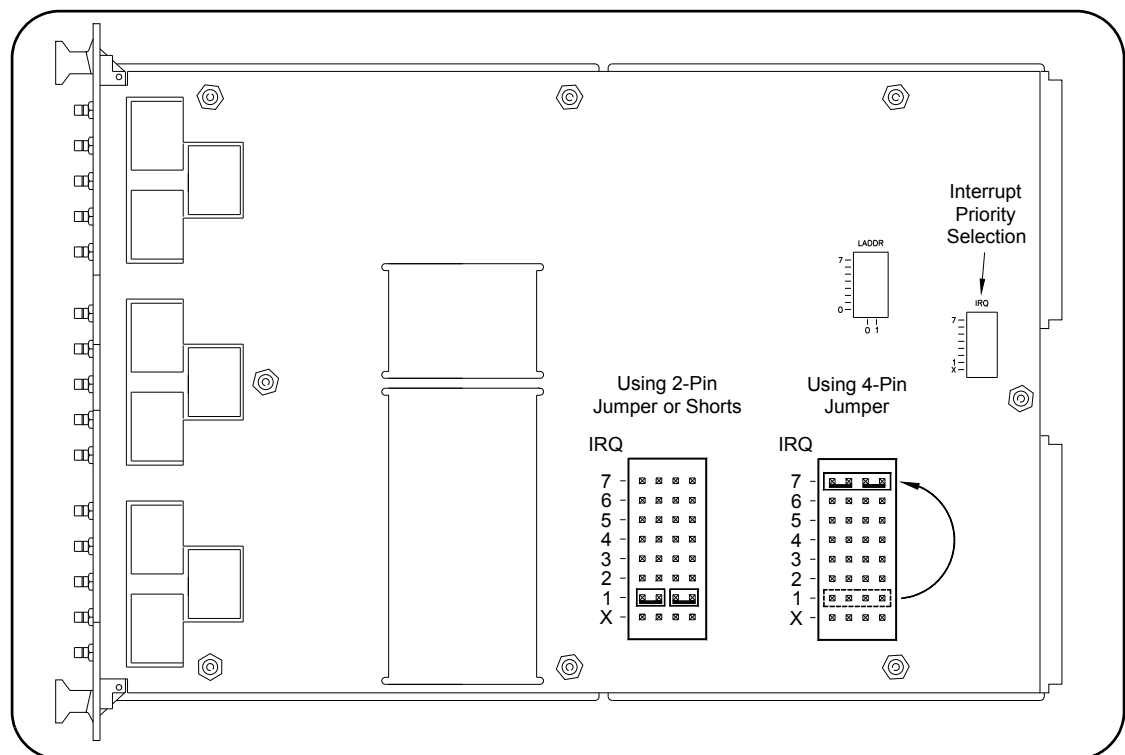


Figure 2-2. Interrupt Priority Selection

Expanding the RF Multiplexer

Each RF Multiplexer module is capable of controlling up to two Expander modules, providing a total of eighteen (4:1) banks. The Expander modules can be physically located in the C-Size mainframe next to the RF Multiplexer, or up to eight meters away using extension cables. Use Figure 2-3 and the following procedure to connect the Expander modules.

- 1 Verify a 3-1 cable (part number E1472-61601) is installed in the Remote Module Driver (RMD) 2/4/5 cable slot. Cable can be connected without removing the shield.
- 2 Cut the cable ties holding the cables, and pull the cables through the slots in the shield.
- 3 Mark the 3-1 cables as shown in Figure 2-3 (cross out unused RMD number).
- 4 Connect the 3-1 cables to the Expander modules as follows:
 - RMD3 cable to Expander (module 01) Bank 3-5 connector.
 - RMD2 cable to Expander (module 01) Bank 0-2 connector.
 - RMD5 cable to Expander (module 02) Bank 3-5 connector.
 - RMD4 cable to Expander (module 02) Bank 0-2 connector.

NOTE *RMD1 cable is connected to E1472A/74A (module 00) Bank 3-5 connector, and RMD0 cable is connected to E1472/74A (module 00) Bank 0-2 connector at the factory. These connections are not accessible with the shield in place and should not be moved.*

- 5 If the Expander module is physically located (up to eight meters) away from the mainframe, you can daisy chain up to 10 extender cables (part number E1473-80002) for each RMD connection (see Figure 2-3, module 02).
- 6 Fold and tie unused RMD cables.

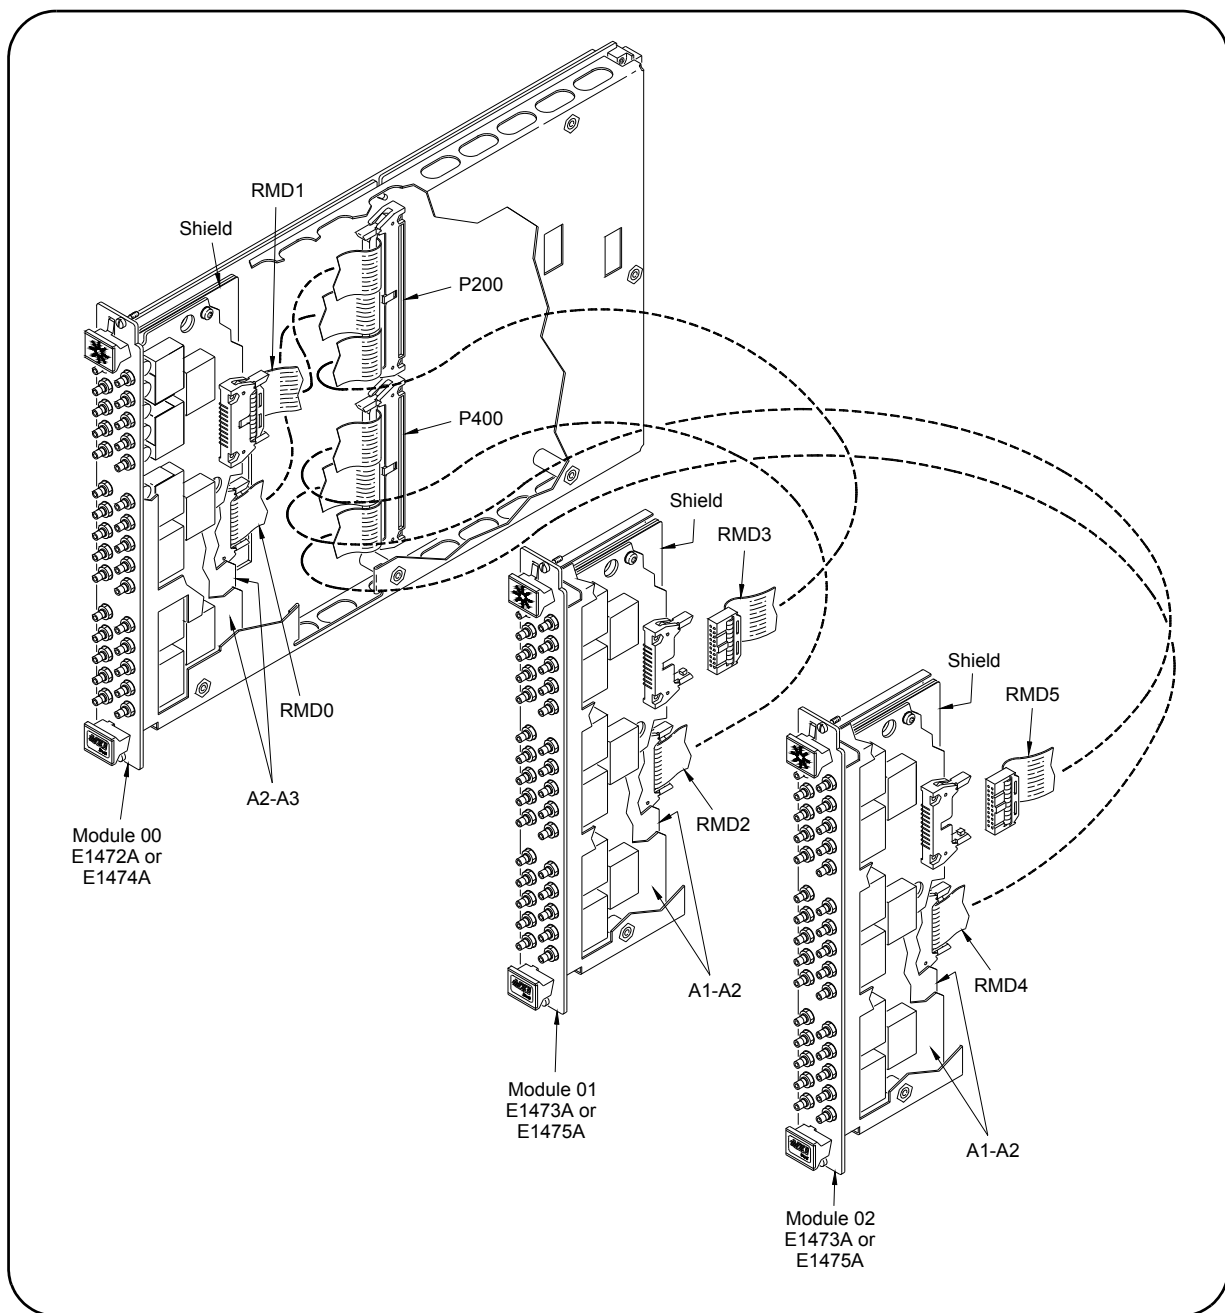


Figure 2-3. Expander Module Connections

Selecting the Relay Drive Level

The relay drive level is set at the factory to +12 Vdc. This is the level used by both the RF Multiplexer module and the Expander module relays.

NOTE *DO NOT CHANGE the relay drive level if using E1472A, E1473A, E1474A, or E1475A modules.*

If external relays of +5 Vdc or +24 Vdc are used with the RF Multiplexer module, the drive level must be changed as follows:

- 1 Position the RF Multiplexer on a flat surface.
- 2 Using a TORX T-10 driver, remove the eight screws (part number 0515-1135).
- 3 From the rear, carefully lift shield enough to access jumpers.

CAUTION **POSSIBLE RELAY DAMAGE.** Relays may be permanently damaged if the incorrect relay drive level is selected. Change the relay drive level only when ALL relays used (modules 00 AND 01 AND 02) require a +5V or +24V drive level.

CAUTION **POSSIBLE SHIELD DAMAGE.** The shield is connected to the front panel and will be damaged if bent too far. Do not move the RF Multiplexer module from the flat surface with the shield in this condition. It may be necessary to loosen the SMB connector nuts to access the jumpers.

- 4 Move both jumpers (part number 1258-0141) from the +12 Vdc position to the desired drive level. Jumper J200 sets the voltage drive level for the relay modules connected to P200. Jumper J400 sets the voltage drive level for the relay modules connected to P400.
- 5 Reinstall the eight screws.

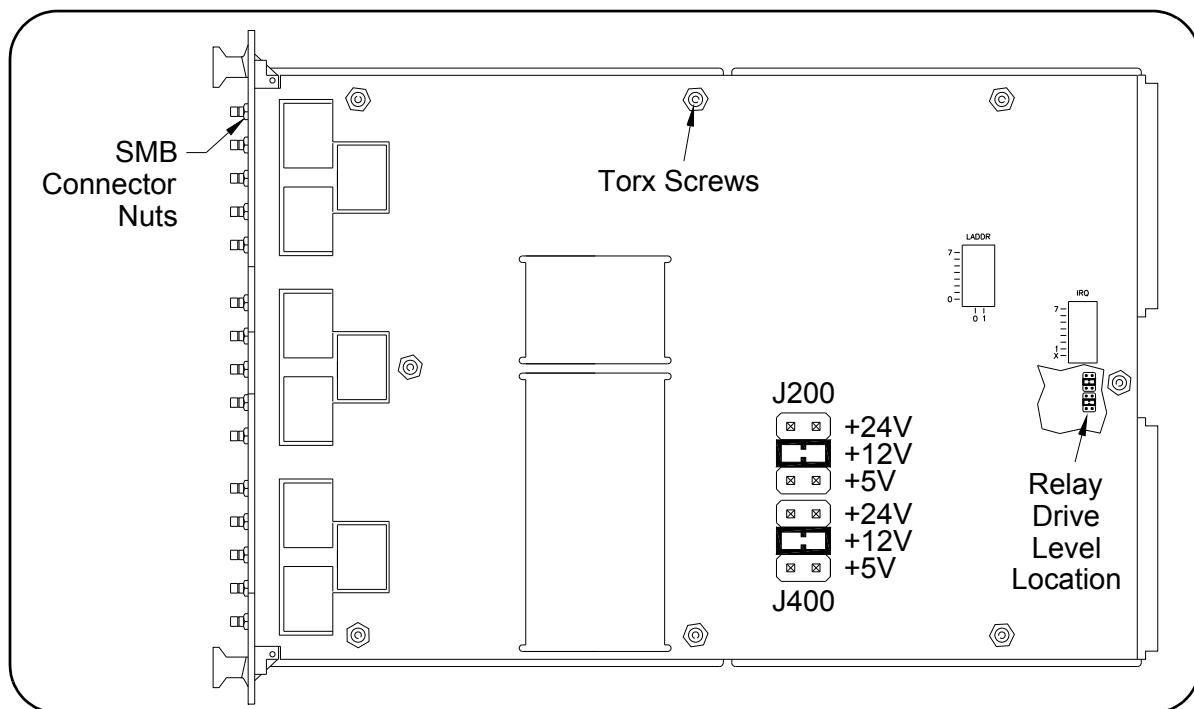


Figure 2-4. Relay Drive Level Selection

Connecting User Inputs to E1472A/E1473A

User inputs to the E1472A RF Multiplexer and E1473A Expander modules are via user-supplied female 50 Ohm SMB connectors to the male 50 Ohm SMB connectors on the modules. Figure 2-5 shows the RF Multiplexer 50 Ohm SMB connectors and associated channel numbers.

Cabling Guidelines

- For best high-frequency performance, user cabling should have at least two braided shields or one braid and a foil wrap.
- Always use shielded coaxial cables with the characteristic impedance of 50 Ohms. Keep cables as short as possible, especially in high-frequency circuits or pulse circuits where a rise/fall time is critical.
- Long cables can add delay time which can cause timing problems. All test equipment, such as counters, spectrum analyzers, and oscilloscopes must be terminated in the characteristic impedance (50 Ohms) to minimize reflection loss.

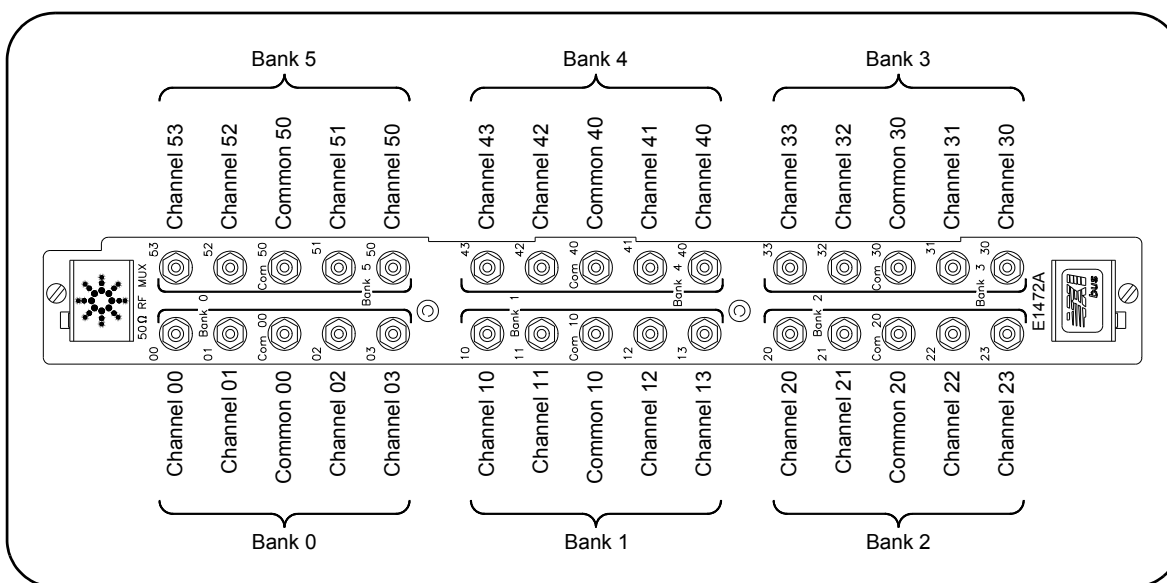


Figure 2-5. 50 Ohm SMB Connector Locations

Connecting User Inputs to E1474A/E1475A

User inputs to the RF Multiplexer and Expander modules are via user-supplied female 75 Ohm SMB connectors to the male 75 Ohm SMB connectors on the modules. Figure 2-6 shows the RF Multiplexer 75 Ohm SMB connectors and associated channel numbers.

Cabling Guidelines

- The 75 Ohm connectors only work with one braided shield or one braid and a foil wrap.
- Always use shielded coaxial cables with the characteristic impedance of 75 Ohm. Keep cables as short as possible, especially in high-frequency circuits or pulse circuits where a rise/fall time is critical.
- Long cables can add delay time which can cause timing problems. All test equipment, such as counters, spectrum analyzers, and oscilloscopes must be terminated in the characteristic impedance (75 Ohm) to minimize reflection loss.
- The 75 Ohm SMB connectors are significantly different than the standard 50 Ohm SMB connectors. Carefully plug the connectors in and out to minimize damage to the connector. The 75 Ohm SMB mating connectors and accessories are available only from Agilent or E.F. Johnson Co.¹
- See Examples 1 and 2 for information on connectors and accessories.

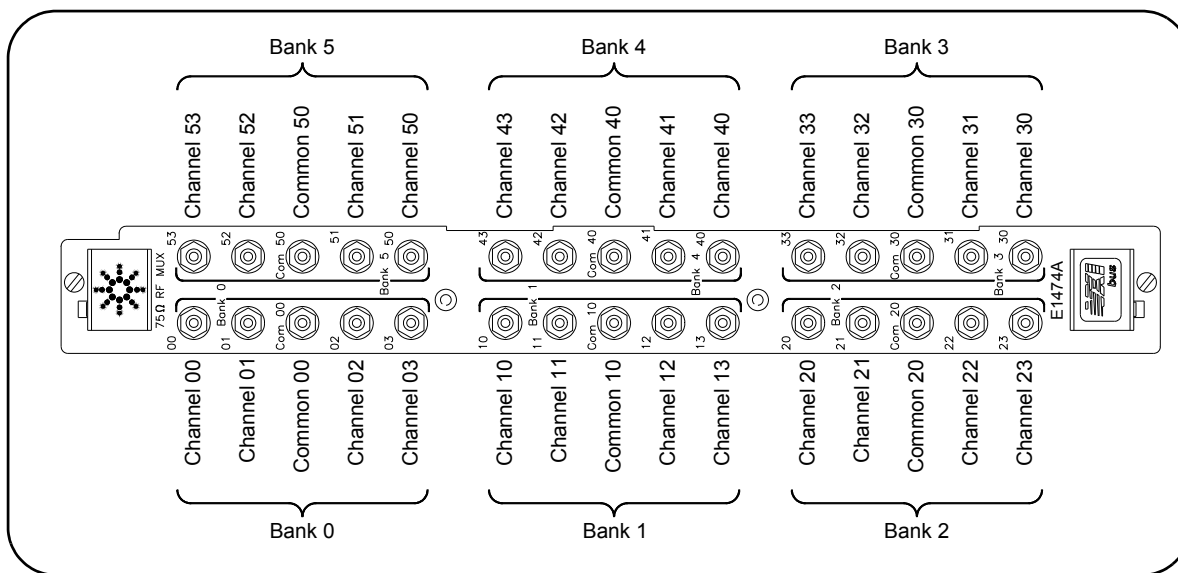


Figure 2-6. 75 Ohm SMB Connector Locations

1. E.F. Johnson Co., 299 Johnson Ave., Waseca, MN 56093-0514. Telephone: 1-800-247-8256, FAX: 1-507-835-6287

Example 1: Connection to a Network Analyzer

Figure 2-7 shows how to connect the E1474A/E1475A RF multiplexer to an 8753 Network Analyzer with an 85046B 75 Ohm S-Parameter test set. Similar connections can be used for other devices. The Type N plug is available from Trompeter Electronics¹ (part number UPL 95-5). The cable used is RG179.

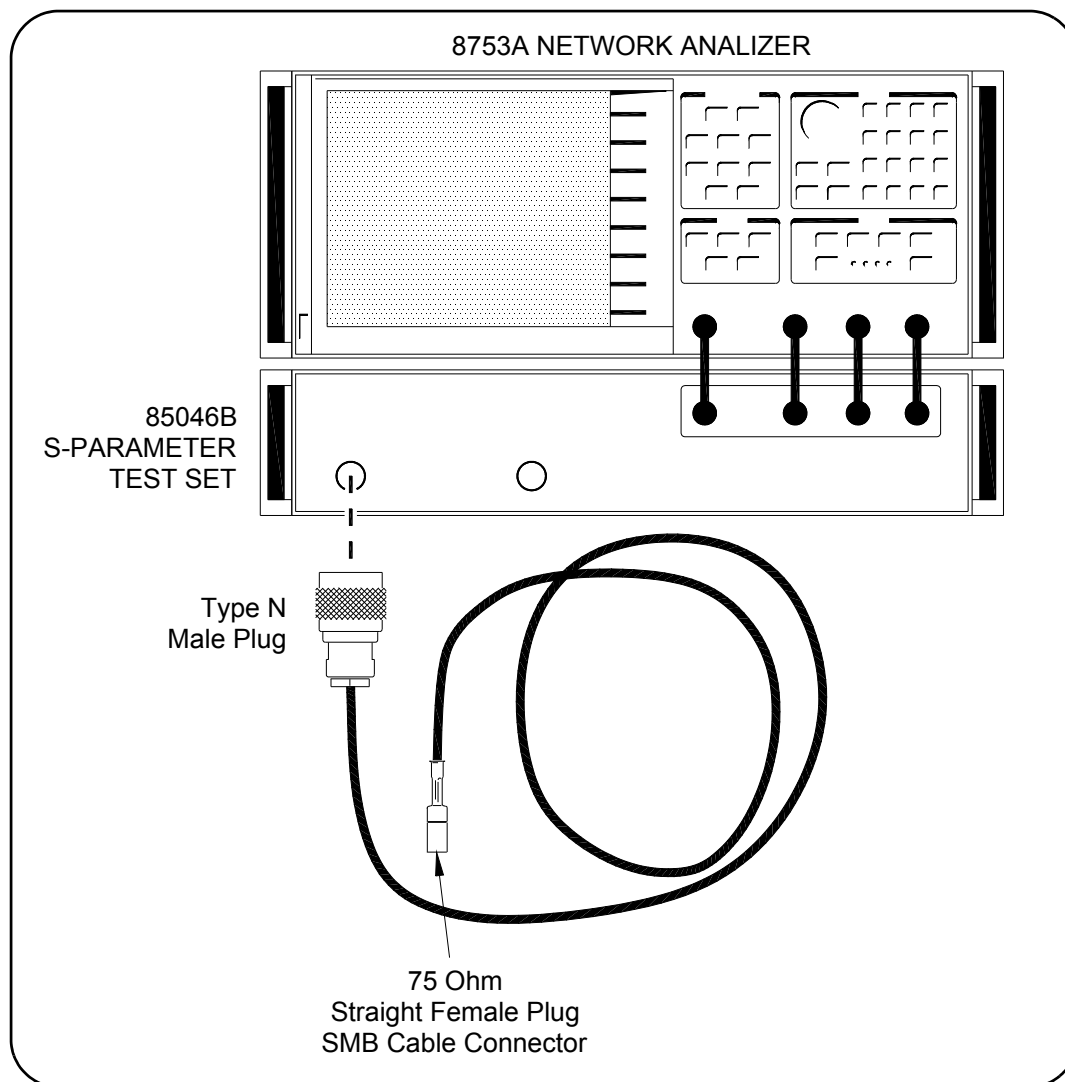


Figure 2-7. Connection to Network Analyzer with 75 Ohm S-Parameter Test Set

1. Trompeter Electronics, 31186 La Baya Drive, Westlake Village, CA. 91362-4047.
Telephone (818) 707-2020

Example 2: Connection to a Network Analyzer

Figure 2-8 shows how to connect the E1474A/E1475A RF multiplexer to an 8753 Network Analyzer with an 85046A 50 Ohm S-Parameter test set. Similar connections can be used for other devices.

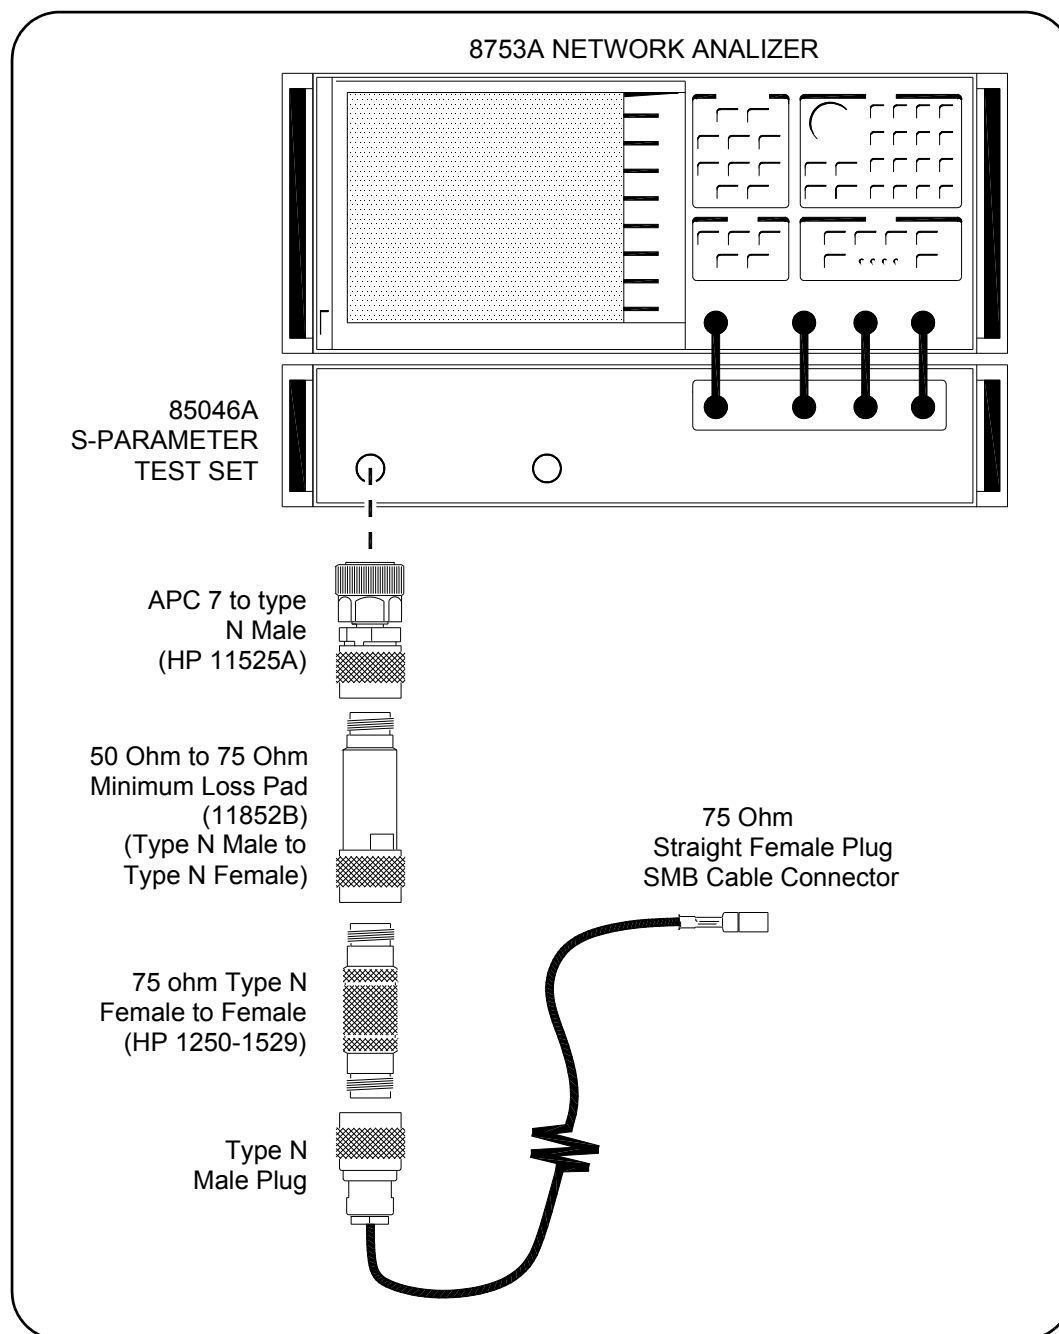


Figure 2-8. Connection to Network Analyzer with 50 Ohm S-Parameter Test Set

Cables and Connectors

Cables

The following tables list 50 Ohm and 75 Ohm cables and connectors available from Agilent. Some 75 Ohm connectors are also available from E.F. Johnson Company.

Table 2-1. Right-Angle SMB Female (Plug) to Right-Angle SMB Female (Plug)

| Length | 50 Ohm Part Number | 75 Ohm Part Number |
|-------------|--------------------|--------------------|
| 55mm (2") | 8120-5627 | 8120-5589 |
| 75mm (3") | 8120-5628 | 8120-5590 |
| 125mm (5") | 8120-5629 | 8120-5591 |
| 175mm (7") | 8120-5630 | 8120-5592 |
| 330mm (13") | 8120-5631 | 8120-5593 |
| 430mm (17") | 8120-5632 | 8120-5594 |
| 925mm (36") | 8120-5633 | 8120-5595 |




Table 2-2. Straight SMB Female (Plug) to Straight SMB Female (Plug)

| Length | 50 Ohm Part Number | 75 Ohm Part Number |
|-------------|--------------------|--------------------|
| 125mm (5") | 8120-5091 | 8120-5584 |
| 175mm (7") | 8120-5623 | 8120-5585 |
| 330mm (13") | 8120-5624 | 8120-5586 |
| 430mm (17") | 8120-5625 | 8120-5587 |
| 925mm (36") | 8120-5626 | 8120-5588 |





Table 2-3. Right-Angle SMB Female (Plug) to Bulkhead SMB Male (Jack)

| Length | 50 Ohm Part Number | 75 Ohm Part Number |
|-------------|--------------------|--------------------|
| 125mm (5") | 8120-5608 | 8120-5579 |
| 175mm (7") | 8120-5609 | 8120-5580 |
| 330mm (13") | 8120-5610 | 8120-5581 |
| 430mm (17") | 8120-5611 | 8120-5582 |
| 925mm (36") | 8120-5612 | 8120-5583 |






Table 2-4. Right-Angle SMB Female (Plug) to Bulkhead BNC Male (Plug)

| Length | 50 Ohm Part Number | 75 Ohm Part Number |
|-------------|--------------------|--------------------|
| 125mm (5") | 8120-5603 | 8120-5598 |
| 175mm (7") | 8120-5604 | 8120-5599 |
| 330mm (13") | 8120-5605 | 8120-5600 |
| 430mm (17") | 8120-5606 | 8120-5601 |
| 925mm (36") | 8120-5607 | 8120-5602 |




Table 2-5. Right-Angle SMB Female (Plug) to Bulkhead-mount BNC Female (Jack)^a

| Length | 50 Ohm Part Number | 75 Ohm Part Number |
|-------------|--------------------|--------------------|
| 125mm (5") | 8120-5613 | 8120-5618 |
| 175mm (7") | 8120-5614 | 8120-5619 |
| 325mm (13") | 8120-5615 | 8120-5620 |
| 425mm (17") | 8120-5616 | 8120-5621 |
| 925mm (36") | 8120-5617 | 8120-5622 |

a. SMB jacks are "male", SMB plugs are "female", BNC jacks are "female", and BNC plugs are "male".

Connectors

Tables 2-6 and 2-7 list available 75 Ohm and 50 Ohm SMB connectors. See Figure 2-9 for a diagram of each connector.

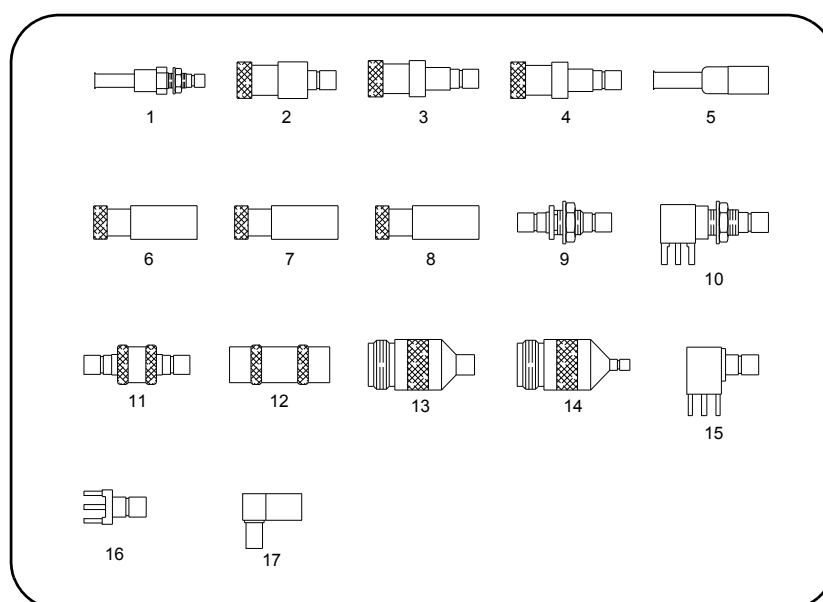


Figure 2-9. SMB Connector Drawings

Table 2-6. 75 Ohm SMB Connectors

| Dwg Nbr | Description | Agilent P. N. | Johnson P. N. |
|----------------|---|----------------------|----------------------|
| 1 | Jack (male) Straight Bulkhead SMB Cable Connector | 1250-2341 | 131-8303-401 |
| 2 | Jack (male) Load | 1250-2342 | 131-8701-801 |
| 3 | Jack (male) Short | 1250-2358 | 131-8701-811 |
| 4 | Jack (male) Open | 1250-2354 | 131-8701-821 |
| 5 | Plug (female) Straight SMB Cable Connector | 1250-2336 | 131-8403-001 |
| 6 | Plug (female) 75 Ohm Load | 1250-2343 | 131-8801-801 |
| 7 | Plug (female) Short | 1250-2359 | 131-8801-311 |
| 8 | Plug (female) Open | 1250-2355 | 131-8801-821 |
| 9 | In-series Adapter Jack - Bulkhead Jack | 1250-2337 | 131-8901-401 |
| 10 | Right-Angle Bulkhead Jack | 1250-2356 | 131-8701-501 |
| 11 | Male Jack to Male Jack | 1250-2378 | 131-8901-801 |
| 12 | Female plug to Female Plug | 1250-2377 | 131-8901-811 |
| 13 | 75 Ohm Type N Jack to 75 Ohm SMB Female Plug | N/A | 134-1069-021 |
| 14 | 75 Ohm Type N Jack to 75 Ohm SMB Male Jack | N/A | 134-1069-031 |
| 15 | Right Angle Jack Receptacle | 1250-2339 | 131-8701-301 |
| 16 | Straight Jack Receptacle | 1250-2335 | 131-8701-201 |
| 17 | Right Angle Crimp Type Plug | 1250-2340 | 131-8403-101 |

Table 2-7. 50 Ohm SMB Connectors

| Dwg No. | Description | Part Number |
|----------------|---|--------------------|
| 1 | Jack (male) Straight Bulkhead SMB Cable Connector | 1250-1902 |
| 5 | Plug (female) Straight SMB Cable Connector | 1250-1907 |
| 6 | Plug (female) 50 Ohm Load | 1250-0676 |
| 7 | Plug (female) Short | 1250-0911 |
| 9 | In-series Adapter Jack - Bulkhead Jack | 1250-1593 |
| 11 | Male Jack to Male Jack | 1250-0669 |
| 12 | Female plug to Female plug | 1250-0672 |
| 15 | Right Angle Jack Receptacle | 1250-0543 |
| 16 | Straight Jack Receptacle | 1250-0257 |
| 17 | Right Angle Crimp Type Plug | 1250-1901 |

Chapter 3

Using the RF Multiplexers

Using This Chapter

This chapter uses typical examples to show how to use the RF Multiplexer and Expander modules. This chapter contains the following sections:

- RF Multiplexer Commands 31
- Switching Channels 32
- Saving and Recalling States 34
- Detecting Error Conditions 34
- Synchronizing the RF Multiplexer 36

RF Multiplexer Commands

Table 3-1. RF Multiplexer Commands Used in Chapter 3

| Command | Description |
|-----------------------------|---|
| [ROUT:]CLOS <channel_list> | Close the channels in the <channel_list> |
| [ROUT:]CLOS? <channel_list> | Queries the state of the channels in the <channel_list> |
| [ROUT:]OPEN? <channel_list> | Queries the state of the channels in the <channel_list> |
| *CLS | Clears all switchbox status register. |
| *ESE | Enables event status register |
| *RST | Sets the hardware and software to a known state |
| *SRE | Enables status register |

NOTE When the RF Multiplexer is switched off, switched on, or *RST (reset), all banks close channel n0 to COMmon. When the RF Multiplexer is powered up or down, signals connected to the channel n0 connector will also be connected to the COMmon connector.

Switching Channels

For general purpose switch operation, you can connect a signal by closing a specific channel to its COMmon. One channel per bank will be connected to COMmon at all times, and only one channel per bank can be closed at a time. Switching configurations include standard, matrix, and tree. The following channel configurations are possible.

- Close channels 00 to 03 by connecting a channel to COM00.
- Close channels 10 to 13 by connecting a channel to COM10.
- Close channels 20 to 23 by connecting a channel to COM20.
- Close channels 30 to 33 by connecting a channel to COM30.
- Close channels 40 to 43 by connecting a channel to COM40.
- Close channels 50 to 53 by connecting a channel to COM50.

Use CLOSe *channel_list* to close a channel to COMmon. *channel_list* has the form (@ccmmnn) for a single channel, and (@ccmmnn,ccmmnn,...) for two or more channels.

- cc = card number (01-99).
- mm = module number (00-02).
- nn = channel number (00-03, 10-13, 20-23, 30-33, 40-43, 50-53).

NOTE *The following examples are shown using multiple configurations (multiple-module switchbox and single module switchbox with Expander modules) to illustrate programming differences. All the examples shown could have been performed using only one E1472A or E1474A RF Multiplexer module.*

Example: Standard Switching

You can use standard switching to switch channels n0-n3 to COM n0 (where n = Switching bank number 0 to 5). One channel per bank can be connected to its common at a time. This example connects channel 11 to COM10 of an RF Multiplexer in a standard configuration. The RF Multiplexer without Expander modules is defined as a single-multiplexer switchbox instrument. In Figure 3-1, execute CLOS (@111) to connect COM 10 to channel 11 .

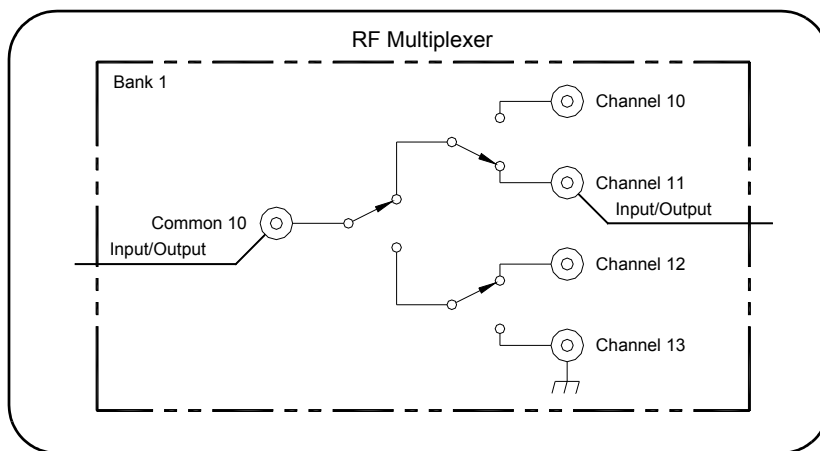


Figure 3-1. Example: RF Multiplexer Standard Switching

Example: Tree Switching

Use tree switching to provide signal routing while maintaining characteristic impedance. With tree switching, signal delay time is more than doubled since the signal must pass through two or more channel banks plus extra cabling. Keep cables as short as possible, especially between channel banks, to minimize delay.

This example uses two RF Multiplexers in a tree configuration to connect COM 10 of RF Multiplexer number 01 to channel 13 of RF Multiplexer 02. The two RF Multiplexers form a multiple-multiplexer switchbox instrument. In Figure 3-2, execute CLOS (@111,213) to connect COM 10 to channel 13.

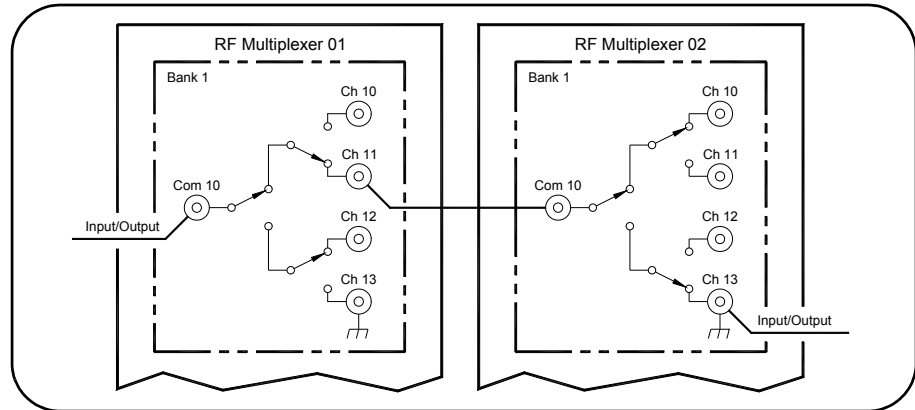


Figure 3-2. Example: RF Multiplexer Tree Switching

Example: Matrix-Type Switching

You can use matrix-type switching to provide connection of up to four devices under test (DUT) to up to four test instruments. With this configuration, only one channel in bank 0 (one “row”) can be connected to one channel in bank 1 (one “column”) at a time.

This example uses one RF Multiplexer and one Expander in a matrix-type configuration to connect channel 03 of the RF Multiplexer (module 00) to channel 11 of the Expander (module 01). The RF Multiplexer and Expander modules are defined as a single-multiplexer switchbox instrument. In Figure 3-3, execute CLOS (@10003,10111) to connect channel 03 to channel 11.

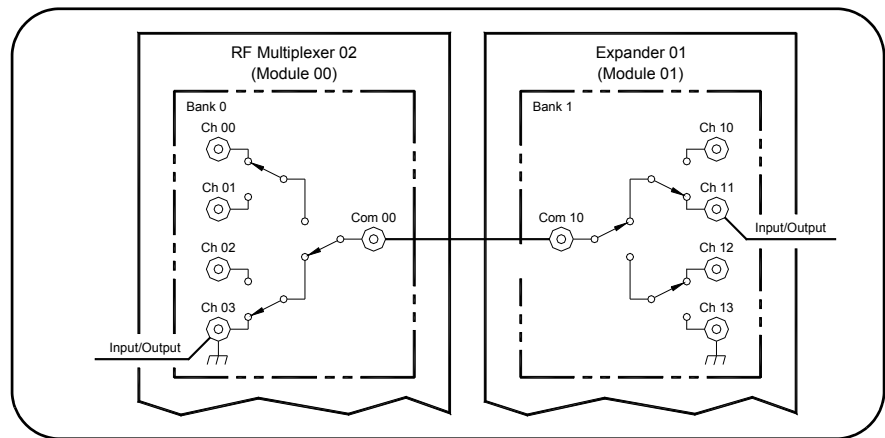


Figure 3-3. Example: Multiplexer/Expander Matrix Type Switching

Saving and Recalling States

The `*SAV <numeric_state>` command saves the current instrument state. The state number (0-9) is specified in the `<numeric_state>` parameter. The channel states (channel closed to common) are saved.

The `*RCL <numeric_state>` command recalls a previously saved state. Enter the number (0-9) in the `<numeric_state>` parameter of the desired saved state. If `*SAV` was not previously executed using the selected number, the RF Multiplexer will configure to the reset values (channel 0 to COMMon on all banks).

Detecting Error Conditions

There are two general approaches to error checking. The simplest, but most time consuming, is to ask the instrument whether there are errors at every step of the switching process. This is called "polling" and is illustrated in the following example.

Example: Polling Method of Error Checking

```
05 DIM Err_num$ [256]
10 OUTPUT 70915; "CLOS(@101);:SYST:ERR?"
20 ENTER 70915;Err_num$
30 IF VAL (Err_num$) <> 0 THEN
40   PRINT "Error";Err_num$
50   STOP
60 END IF
70 . . . (program continues)
```

Example: Error Checking Using Interrupts

The other approach involves the use of interrupts. The following program is a method of checking for errors using interrupts as you program the RF Multiplexer. The program monitors the RF Multiplexer's Standard Event Status Register for an error condition.

If no errors occur, the RF Multiplexer functions as programmed. If errors do occur, the RF Multiplexer interrupts the computer, and the error codes and messages are read from the error queue. This approach requires less checking but is more complex. This BASIC example uses a GPIB select code of 7, primary address of 09, and secondary address of 15 for the RF Multiplexer.

```
10 !Call computer subprogram "Errmsg" if an RF Multiplexer programming
20 !error occurs. Enable the computer to respond to an interrupt from the
30 !RF Multiplexer.
35 !
40 ON INTR 7 CALL Errmsg
50 ENABLE INTR 7:2
```

```

60 !
70 !Unmask the Event Status bit in the RF Multiplexer's Status
80 !Register. Unmask the RF Multiplexer error conditions in its
90 !Standard Event Status Register.
100 OUTPUT 70915;"*SRE 32"
110 OUTPUT 70915;"*ESE 64"
120 !
130 !At this point, the RF Multiplexer is programmed for the
140 !intended application.
145 !
150 OUTPUT 70915;" . . .
160 OUTPUT 70915;" . . .
170 ENTER 70915; . . .
180 PRINT . . .
190 END
200 !
210 !When an error occurs, clear the RF Multiplexer to regain
220 !control. Execute a Serial Poll to clear the service request
230 !bit in the Status Register. Read all error messages in the
240 !RF Multiplexer error queue. Clear all bits in the RF Multiplexer
250 !Standard Event Status Register.
255 !
260 SUB Errmsg
270   DIM Message$(256)
280   CLEAR 70915
290   B=SPOLL (70915)
300   REPEAT
310     OUTPUT 70915; "SYST:ERR?"
320     ENTER 70915; Code, Message$
330     PRINT Code,Message$
340   UNTIL Code=0
350   OUTPUT 70915;"*CLS"
360   STOP
370 SUBEND

```

Synchronizing the RF Multiplexer

This section discusses synchronizing the RF Multiplexer module to other instruments when making measurements. In the following example the RF Multiplexer switches a signal to be measured by a counter. This program verifies that switching is complete before the counter begins a measurement.

This example uses a GPIB select code of 7, primary address of 09, and secondary address of 06 for the Counter and a GPIB select code of 7, primary address of 09, and secondary address of 15 for the RF Multiplexer.

```
10  ! Close channel 01 and request confirmation the channel is closed.
20  OUTPUT 70915;"CLOSE (@101);*OPC?"
25  ENTER 70915;OPC_value
30  !Read confirmation.
35  OUTPUT 70915;"CLOSE? (@101)"
40  ENTER 70915;A
50  !At this point (channel is closed) the measurement can be made.
60  OUTPUT 70906: "MEAS:FREQ?"
70  ENTER 70906:Meas_value
80  END
```

Chapter 4

RF Multiplexer Command Reference

Using This Chapter

This chapter describes Standard Commands for Programmable Instruments (SCPI) commands and summarizes IEEE 488.2 Common (*) commands applicable to the RF Multiplexer. See the *Agilent Command Module User's Guide* for additional information on SCPI and common commands.

- Command Types 37
- SCPI Command Reference39
- Common Commands Quick Reference46
- SCPI Commands Quick Reference47

Command Types

Commands are separated into two types: IEEE 488.2 Common Commands and SCPI Commands.

Common Command Format

The IEEE 488.2 standard defines the Common Commands that perform functions like reset, self-test, status byte query, etc. Common commands are four or five characters in length, always begin with the asterisk character (*), and may include one or more parameters. The command keyword is separated from the first parameter by a space character. Some examples of Common Commands are:

```
*RST *ESR 32 *STB?
```

SCPI Command Format

The SCPI commands perform functions like closing switches, querying instrument states, or retrieving data. A subsystem command structure is a hierarchical structure that usually consists of a top level (or root) command, one or more lower level sub commands, and their parameters. The following example shows a typical subsystem:

```
[ROUTe:]  
  CLOSe <channel_list>
```

[ROUTe:] is the root command, :CLOSe is the second level sub command, and <channel_list> is a parameter.

Command Separator

A colon (:) always separates one command from the next lower level command, such as ROUTe:CLOSE?. Colons separate the root command from the second level (ROUTe:CLOSE?). If a third level exists, the second level is also separated from the third level by a colon.

Abbreviated Commands

The command syntax shows most commands as a mix of upper and lower case letters. The upper case letters indicate the abbreviated spelling for the command. For shorter program lines, send only the abbreviated form. For better program readability, you may send the entire command. The instrument will only accept either the abbreviated form or the entire command.

For example, if the command syntax shows CLOSE, CLOS and CLOSE are both acceptable forms. Other forms of CLOSE, such as CL or CLO will generate an error. You may use upper or lower case letters. Therefore, CLOSE, and CIOSe are both acceptable.

Implied Commands

Implied commands are those which appear in square brackets ([]) in the command syntax. (The brackets are not part of the command and are not sent to the instrument.) Suppose you send a second level command but do not send the preceding implied command. In this case, the instrument assumes you intend to use the implied command and it responds as if you had sent it. Examine the portion of the ROUTe subsystem shown below:

```
[ROUTe:]  
CLOSE? <channel_list>
```

The root command ROUTe: is an implied command. To make a query about a channel's present status, you can send either of the following command statements:

```
ROUT:CLOSE? <channel_list> or CLOSE? <channel_list>
```

Parameters

This table contains explanations and examples of parameter types that can be used.

| Parameter Type | Explanations and Examples |
|----------------|---|
| Numeric | Accepts all commonly used decimal representations of numbers including optional signs, decimal points, and scientific notation, such as 123 or 1.23E2; -123 or -1.23E2; .123, 1.23E-1, or 1.23000E-01. Special cases include MIN, MAX, and DEF. MIN selects minimum value available, MAX selects maximum value available, and DEF selects default or reset value. |
| Boolean | Represents a single binary condition that is either true or false (1 or ON; 0 or OFF) |
| Discrete | Selects from a finite number of values. These parameters use mnemonics to represent each valid setting. An example is the TRIGger:SOURce <source> command where <source> can be BUS, HOLD, or IMMEDIATE. |

Linking Commands

Linking IEEE 488.2 Common Commands with SCPI Commands. Use a semicolon between the commands. For example:

*RST;*RCL 1 or CLOS (@101);*SAV 1

Linking Multiple SCPI Commands. Use both a semicolon and a colon between the commands. For example:

CLOS (@101);:CLOS? (@101)

SCPI also allows several commands within the same subsystem to be linked with a semicolon. For example:

ROUT:CLOS (@101);:ROUT:CLOS? (@101)

or

ROUT:CLOS (@101);CLOS? (@101)

SCPI Command Reference

This section describes Standard Commands for Programmable Instruments (SCPI) for the RF Multiplexer. Commands are listed alphabetically by subsystem and also within each subsystem.

[ROUTe:]

The ROUTe command subsystem controls switching operations for the RF Multiplexer in a switchbox.

Subsystem Syntax [ROUTe:]
CLOSE <channel_list>
CLOSE? <channel_list>
OPEN? <channel_list>

[ROUTe:]CLOSE

ROUTe:]CLOSE <channel_list> closes the RF Multiplexer channels specified by *channel_list*. *channel_list* has the form (@ccmmnn) where *cc* = card number (01-99), *mm* = module number (00-02), and *nn* = channel number (00-03, 10-13, 20-23, 30-33, 40-43, or 50-53).

Parameters

| Name | Type | Range | Item |
|----------------|-------------------------------|--|---|
| <channel_list> | numeric numeric numeric | 01-99 00-02 00-03 10-13 20-23 30-33 40-43 50-53 | card (<i>cc</i>) module (<i>mm</i>) channel (<i>nn</i>) |

Comments **Closing Channels:** To close a single channel, use [ROUTe:]CLOSE (@ccmmnn); for multiple channels use [ROUTe:]CLOSE (@ccmmnn,ccmmnn,...) or any combination. Closure order for multiple channels with a single command is not guaranteed.

Channel Range: The RF Multiplexer will accept and execute channel ranges (*ccmmnn:ccmmnn*) without generating an error, but the result is to close the last channel in each bank within the range specified. For example, after CLOSE (@010101:010151) is executed, card 01, module 01 channels 03, 13, 23, 33, 43, and 51 would remain closed.

Module Number: The module number can be omitted when Expander modules are not connected to the RF Multiplexer. Module numbers must be specified when one or more Expander modules are connected to the RF Multiplexer module.

Related Commands: [ROUTe:]OPEN?, [ROUTe:]CLOSE?

***RST Condition:** All banks with channel 0 connected to COMmon.

Example Closing RF Multiplexer Channels

This example closes channels 100 and 202 of a two-card switchbox (card numbers 01 and 02).

```
CLOS (@101,202)                                !101 connects channel 01 to
                                                !COM00 on card #1 and 202
                                                !connects channel 02 to COM00
                                                !on card #2.
```

[ROUTe:]CLOSe?

[ROUTe:]CLOSe?<channel_list> returns the current state of the channel(s) queried. *channel_list* has the form (@ccmmnn) (see [ROUTe:]CLOSe for definition). The command returns 1 if channel(s) are closed or returns 0 if channel(s) are open.

Comments **Query is Software Readback:** The [ROUTe:]CLOSe? command returns the current software state of the channel(s) specified. It does not account for relay hardware failures. A maximum of 127 channels at a time can be queried for a multi-module switchbox.

Example Query Channel Closure

This example closes channels 01 and 02 of a two-module switchbox (card number 01, module 00 and 01) and queries channel closure. Since the channels are programmed to be closed, 1,1 is returned.

```
CLOS (@10001,10102)                            !Connect channel 01 to COM00 on
                                                !the RF Multiplexer module (00)
                                                !and channel 02 to COM00 on the
                                                !Expander module (01).

CLOS? (@10001,10102)                            !Query module 00 - channel 01
                                                !and module 01 - channel 02
                                                !closure state.
```

[ROUTe:]OPEN?

[ROUTe:]OPEN?<channel_list> returns the current state of the channel(s) queried. *channel_list* has the form (@ccmmnn) (see [ROUTe:]CLOSe for definition). The command returns 1 if channel(s) are open or returns 0 if channel(s) are closed.

Comments **Query is Software Readback:** The ROUTe:OPEN? command returns the current software state of the channels specified. It does not account for relay hardware failures. A maximum of 127 channels at a time can be queried for a multi-module switchbox.

Example Query Channel Open State

This example closes channels 01 and 02 of a single card two-module switchbox (card number 01, module 00 and 01) and queries channel closure. Since the channels are programmed to be closed, 0,0 is returned.

| | |
|----------------------|---|
| CLOS (@10001,10102) | <i>!Connect channel 01 to COM00 on !the RF Multiplexer module (00) !and channel 02 to COM00 on the !Expander module (01).</i> |
| OPEN? (@10001,10102) | <i>!Query module 00 - channel 01 !and module 01 - channel 02 open !states.</i> |

SYSTem

The SYSTem subsystem returns the error numbers and error messages in the error queue of a switchbox, and returns the types of descriptions of cards and modules in a switchbox.

Subsystem Syntax SYSTem
:CDEscription? <number>
:COPT? <number>
:CPON <number> |ALL
:CTYPe? <number>
:ERRor?

SYSTem:CDEscription?

SYSTem:CDEscription?<number> returns the description of a selected card in a switchbox.

Parameters

| Name | Type | Range of Values | Default Value |
|----------|---------|-----------------|---------------|
| <number> | numeric | 01 to 99 | N/A |

Comments **RF Multiplexer Module Description:** The SYSTem:CDEscription? <number>command returns: "Hex 4:1 75 Ohm RF Mux" or "Hex 4:1 50 Ohm RF Mux".

Example **Reading the Description of Card #1 Module**
SYST:CDES? 1 *!Return the description*

SYSTem:COPTion?

SYSTem:COPTion? <number> returns the number of Expander Modules connected to a selected RF Multiplexer (card) in a switchbox.

Parameters

| Name | Type | Range of Values | Default Value |
|----------|---------|-----------------|---------------|
| <number> | numeric | 01 to 99 | N/A |

Comments RF Multiplexer/Expander modules installed: The SYSTem:COPTion? <number> command returns:

E1472A,E1473A,E1473A or E1474A,E1475A,E1475A

where the E1472A and E1474A are the RF Multiplexer modules, and the E1473A,E1473A or E1475A,E1475 indicates that two expander modules are connected. A “0” in place of the “E1473” or “E1475” indicates that the Expander module(s) are not installed.

Example Reading the Model Number of Card #1 Module

SYST:COPT? 1 *!Return the module configuration
!for card 1*

SYSTem:CPON

SYSTem:CPON <number> |ALL sets the selected module (card) in a switchbox to its power-on state.

Parameters

| Name | Type | Range of Values | Default Value |
|----------|---------|-----------------|---------------|
| <number> | numeric | 01 to 99 ALL | ALL |

Comments RF Multiplexer Module Power-On State: The power-on state is all channels (relays) open. Note that SYSTem:CPON ALL and *RST connects X0 to COM X0 in all banks of all modules in a switchbox, while SYSTem:CPON <number> connects X0 to COMX0 in only the module (card) specified in the command.

Example Setting Card #1 Module to Power-On State

SYST:CPON 1 *!Sets card #1 to power-on state*

SYSTem:CTYPE?

SYSTem:CTYPE? <number> returns the card type of a selected module in a switchbox.

Parameters

| Name | Type | Range of Values | Default Value |
|----------|---------|-----------------|---------------|
| <number> | numeric | 01 to 99 | N/A |

Common Commands Quick Reference

The following table lists the IEEE 488.2 Common (*) Commands that can be executed by the RF Multiplexer module. The operation of some of these commands is described in Chapter 3 of this manual. For more information on Common Commands, see the appropriate command module user's guide or the ANSI/IEEE Standard 488.2-1987.

| Command | Title | Description |
|-------------|------------------------------|---|
| *CLS | Clear status register | Clears all Event Registers, the Request for OPC flag, and all Queues (except output queue). |
| *ESE <mask> | Event status enable | Sets bits in the Event Status Enable Register. |
| *ESE? | Event status enable query | Queries current contents in Event Status Enable Register. |
| *ESR? | Event status register query | Queries and clears contents in Standard Event Status Register. |
| *IDN? | Identification query | Returns identification string of the switchbox. |
| *OPC | Operation complete | Sets the Request for OPC flag when all pending operations have completed. Sets OPC bit in Standard Event Register. |
| *OPC? | Operation complete query | Returns a 1 to the output queue when all pending operations have completed. Synchronize between multiple instruments. |
| *RCL <n> | Recall saved state | Recalls previously stored RF Multiplexer configuration. <n>(0 to 9) is the location in memory where the desired (previously stored) set-up is located. |
| *RST | Reset | Connects channel 0 to COM 0 on all banks. |
| *SAV <n> | Save state | Stores the present RF Multiplexer configuration in memory. Stores present settings of the channel states. <n> (0 to 9) is location in memory where the current set-up is to be stored. |
| *SRE <mask> | Service request enable | Used to set the Service Request Enable Register bits and corresponding Serial Poll Status Byte Register bits to generate a service request. |
| *SRE? | Service request enable query | Query current contents in Service Request Enable Register. |
| *STB? | Read status byte query | Queries the current contents in the Status Byte Register. |
| *TRG | Trigger | Not applicable. |
| *TST? | Self-Test query | Returns +0 if self test passes. Returns +cc01 for firmware error. Returns +cc02 for bus error (communications problem with card). Returns +cc03 for bad ID information. Returns +cc10 if an interrupt was expected but not received. Returns +cc11 if the busy bit was not held ≈9 to 17 msec. |
| *WAI | Wait to Continue | Halts execution of commands and queries until the No Operation Pending message is true. |

SCPI Commands Quick Reference

The following table lists the SCPI commands that can be executed by the RF Multiplexer module. The operation of these commands is described in Chapter 3.

| Command Subsystem | Command/Parameter | Description |
|-------------------|--|--|
| [ROUTe:] | CLOSe <channel_list> CLOSe? <channel_list> OPEN? <channel_list> | Close Channel(s) Query Channel(s) closed Query channel(s) opened |
| SYSTem | :ERRor? CDEscription? <number> CTYPe? <number> :COPTion? <number> :CPON <number> ALL | Returns error number/message in a switchbox Error Queue. Returns description of module in a switchbox. Returns the module type. Returns the RF Multiplexer/Expander module configuration. Sets specified module to its power-on state. |

Notes:

Appendix A

RF Multiplexer Specifications

| Specification | 50 Ohm RF Multiplexer | 75 Ohm RF Multiplexer |
|---|--|--|
| Input Characteristics | | |
| Maximum Voltage | 42V peak (any center or chassis to any other center or chassis) | 42V peak (any center or chassis to any other center or chassis) |
| Maximum Current per channel or common | 1A DC or AC RMS | 1A DC or AC RMS |
| Maximum Power per channel or common | 24 W or 24 VA | 24 W or 24 VA |
| AC Performance | | |
| Insertion Loss (dB) | ($Z_L=Z_S=50\ \Omega$) (40°C, 95% RH) <10 MHz < 0.1 <100 MHz < 0.4 <500 MHz < 0.9 <1.3 GHz < 1.5 <3 GHz < 8.0 typical | ($Z_L=Z_S=75\ \Omega$) (40°C, 95% RH) <10 MHz < 0.3 <100 MHz < 0.4 <500 MHz < 0.8 <1.3 GHz < 1.0 |
| Crosstalk (dB) (channel-channel ¹ , or channel-common) | <10 MHz < -90 <100 MHz < -80 <500 MHz < -65 <1.3 GHz < -50 <3 GHz < -20 typical | <10 MHz < -85 <100 MHz < -75 <500 MHz < -65 <1.3 GHz < -45 |
| VSWR | <10 MHz < 1.05 <100 MHz < 1.15 <500 MHz < 1.25 <1.3 GHz < 1.35 <3 GHz < 1.5 | <10 MHz < 1.05 <100 MHz < 1.15 <500 MHz < 1.25 <1.3 GHz < 1.35 |
| Risetime | <300 psec | <300 psec |
| Signal Delay | <3 nsec | <3 nsec |
| DC Performance | | |
| Thermal Offset | < 6 μ V | < 6 μ V |
| Closed Channel Resistance | < 1 Ω (typical) | < 1 Ω (typical) |
| Insulation Resistance (any terminal to any terminal) | $\leq(40^\circ\text{C}, 65\% \text{ RH}) = > 10^8\Omega$ | $\leq(40^\circ\text{C}, 65\% \text{ RH}) = > 10^8\Omega$ |
| General | | |
| Relay Type | Non-latching armature relays | Non-latching armature relays |
| Typical Relay Life (operations) | With No Load: 5×10^6 With Maximum Rated Load: 10^5 | With No Load: 5×10^6 With Maximum Rated Load: 10^5 |
| Maximum Expander Module Cable Length | 8 Meters (for E1473A) | 8 Meters (for E1475A) |

¹ With one channel closed. Specifications valid at front panel SMB connectors without cables or adapters attached.

Notes:

Appendix B

Register-Based Programming

About This Appendix

This appendix contains the information you can use for register-based programming of the RF Multiplexers. The contents include:

- Addressing the Registers51
- Reading the Registers52
- Writing to the Registers53
- Selecting Channels Using Your Own Relays57

Addressing the Registers

The RF Multiplexer module is a register-based device. To read or write to specific registers, you must use the command register address. Complete command register address is determined by:

- The address space (determined by the command module and mainframe used)
- The module address (determined by the command module used and the module's logical address switch)
- The register offset (for the desired register).

Example: Addressing a Status/Control Register

This example shows how to address the Status/Control Register of an RF Multiplexer module in a C-Size VXI mainframe using an E1406 Command Module. Register addresses for modules are in address space VXI A16. The location of A16 within the E1406 Command Module starts at (1F000_h) (_h = HEX).

The A16 space is divided so modules are addressed only at locations beginning with C000_h within A16. Allocated for each module are 64 register addresses (40_h). The module base address is related to the logical address set by the module's logical address switch (LADDR). The module address is:

$$\text{module address}_h = (\text{logical address}_h) * 40_h + \text{C000}_h$$

For the RF Multiplexer module, the default logical address is 120 (78_h), so the module address within A16 = 78_h * 40_h + C000_h = DE00_h

The Status/Control Register offset is 04 h (from below), so the command register address is:

$$[\text{address space}]_h + [\text{module address}]_h + [\text{register offset}]_h = \\ 1F0000_h + DE00_h + 04_h = 1FDE04_h$$

Reading the Registers

You can read the following RF Multiplexer registers:

- Manufacturer ID Register (base+0_h)
- Device Type Register (base+0_h)
- Status/Control Register (base+04_h)
- Remote Module Register (base+06_h) [Module 00 status]
- Remote Module Register (base+08_h) [Module 01 status]
- Remote Module Register (base+0A_h) [Module 02 status]

- Module 00 Bank 00-02 Channel Enable Register (base+10_h)
- Module 00 Bank 03-05 Channel Enable Register (base+12_h)
- Module 01 Bank 00-02 Channel Enable Register (base+14_h)
- Module 01 Bank 03-05 Channel Enable Register (base+16_h)
- Module 02 Bank 00-02 Channel Enable Register (base+18_h)
- Module 02 Bank 03-05 Channel Enable Register (base+1A_h)

Manufacturer ID Register

Reading this register returns FFFF_h. This shows Hewlett-Packard is the manufacturer and the module is an A16 register-based device.

Device Type Register

Reading this register returns 0180_h if the device is the E1474A RF Multiplexer module, with or without Expander module(s) connected. The E1474A/E1475A use the same Device ID as the E1472A/E1473A. However, the relay module will generate a different remote module code to distinguish between the modules (see “Remote Module ID Registers” in this appendix).

Status/Control Register

The Status/Control Register informs the user about the modules status. Each relay requires about 15 msec execution time during which time the RF multiplexers are “busy”. Bit 7 of this register is used to inform the user of a “busy” condition.

In addition, the interrupt generated after a channel has been closed can be disabled. Bit 6 of this register is used to inform the user of the interrupt status. A read of the Status/Control register (base+04_h) returns:

- FFBF_h when the module is not busy and interrupt is enabled.
- FF3F_h when the module is busy and interrupt is enabled.
- FFFF_h when the module is not busy and interrupt is disabled.
- FF7F_h when the module is busy and interrupt is disabled.

Remote Module ID Registers

Reading these registers determines the number and location of E1473A and E1475A Expander modules connected to E1472A and E1474A RF Multiplexers.

Module 00 Status: The base +06_h register returns module 00 status (RF Multiplexer relays connected to the RMD0/1 connector). Returns FF11_h if the relays are connected, and FFFF_h if the relays are not connected. Returns FF00_h if E1472A/E1473A modules are connected. If you are using the E1474A to control additional E1473A or E1475A modules, use this register to verify the relay type.

Module 01 Status: The base +08_h register returns module 01 status (Expander module connected to the RMD2/3 connector). Returns FF11_h if a module is connected, and FFFF_h if a module is not connected. Returns FF00_h if E1472A/E1473A modules are connected. If you are using the E1474A to control additional E1473A or E1475A modules, use this register to verify the relay type.

Module 02 Status: The base +0A_h register returns module 02 status (Expander module connected to the RMD4/5 connector). Returns FF11_h if a module is connected, and FFFF_h if a module is not connected. Returns FF00_h if E1472A/E1473A modules are connected. If you are using the E1474A to control additional E1473A or E1475A modules, use this register to verify the relay type.

Channel Enable Registers

A read of the Channel Enable register (base +10_h to 1A_h) always returns FFFF_h, regardless of the channel states.

Writing to the Registers

You can write the following RF Multiplexer registers:

- Status/Control register (base +04_h)
- Module 00 Bank 0-2 Channel Enable register (base +10_h)
- Module 00 Bank 3-5 Channel Enable register (base +12_h)
- Module 01 Bank 0-2 Channel Enable register (base +14_h)
- Module 01 Bank 3-5 Channel Enable register (base +16_h)
- Module 02 Bank 0-2 Channel Enable register (base +18_h)
- Module 02 Bank 3-5 Channel Enable register (base +1A_h)

Status/Control Register

Writes to the Status/Control Register (base +04_h) enables you to reset the RF Multiplexer to turn-on conditions (channel 0 to COM 0 on all banks), and disable/enable the interrupt generated when channels are closed. To reset the RF Multiplexer, write a “1” to bit 0 of the Status/Control Register (base +04_h).

NOTE *It is necessary to write a “0” to bit 0 after the reset has been performed before any other commands can be programmed and executed.*

To disable the interrupt generated when channels are closed, write a “1” to bit 6 of the Status/Control Register (base +04_h).

NOTE *Typically, interrupts are only disabled to “peek-poke” a module. Refer to the operating manual of the command module used before disable the interrupt.*

Channel Enable Registers

Writes to the Channel Enable registers (base +10_h to 1A_h) enables you to close the desired channel to COMmon (see Figure B-1). For example, write a “1” to bits 3 and 2 of the (base +12_h) Module 00 Bank 3-5 Channel Enable register to close channel 33 on the RF Multiplexer Module. All other bits must be set to “0”. Only one channel per bank can be closed at a time. Any bit pattern not shown in Table B-1 results in the lowest-numbered channel being closed to COMmon.

Table B-1. Manufacturer ID Register

| b+00 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|-----------------|----|----|----|----|----|---|---|---|---|---|---|---|---|---|---|
| Write | Undefined | | | | | | | | | | | | | | | |
| Read* | Manufacturer ID | | | | | | | | | | | | | | | |

* Returns FFFF_h = Hewlett-Packard A16 only register-based.

Table B-2. Device Type Register

| b+02 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|-------------------|----|----|----|----|----|---|---|---|---|---|---|---|---|---|---|
| Write | Undefined | | | | | | | | | | | | | | | |
| Read | 0180 _h | | | | | | | | | | | | | | | |

Table B-3. Status/Control Registers

| b+04 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|-----------|----|----|----|----|----|---|---|---|---|-----------|---|---|---|---|---|
| Write* | Undefined | | | | | | | | | D | Undefined | | | | | R |
| Read** | Undefined | | | | | | | | B | D | Undefined | | | | | |

* R = Switch reset to power-on state (channel 0 to COMmon all banks) by writing (1) in bit #0.

* D = Disable Interrupt by writing (1) in bit #6.

** B = Status “busy” is (0) in bit #7.

** D = Status “Interrupt disable” is (1) in bit #6.

Table B-4. Remote Module 00 ID Register

| b+06 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|--------------|----|----|----|----|----|---|---|---|---|---|---|---|---|---|---|
| Write | Undefined | | | | | | | | | | | | | | | |
| Read* | Module 00 ID | | | | | | | | | | | | | | | |

* Returns FFFF_h when RF Multiplexer relays are not connected.

* Returns FF00_h when E1472A RF Multiplexer relays are connected.

* Returns FF11_h when E1474A RF Multiplexer relays are connected.

Table B-5. Remote Module 01 ID Register

| b+08 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|--------------|----|----|----|----|----|---|---|---|---|---|---|---|---|---|---|
| Write | Undefined | | | | | | | | | | | | | | | |
| Read* | Module 01 ID | | | | | | | | | | | | | | | |

* Returns FFFF_h when Expander module number 01 is not connected.

* Returns FF00_h when E1473A Expander module number 01 is connected.

* Returns FF11_h when E1475A Expander module number 01 is connected.

Table B-6. Remote Module 02 ID Register

| b+0A _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|--------------|----|----|----|----|----|---|---|---|---|---|---|---|---|---|---|
| Write | Undefined | | | | | | | | | | | | | | | |
| Read* | Module 02 ID | | | | | | | | | | | | | | | |

* Returns FFFF_h when Expander module number 02 is not connected.

* Returns FF00_h when E1473A Expander module number 02 is connected.

* Returns FF11_h when E1475A Expander module number 02 is connected.

Table B-7. RF Multiplexer Module 00 Banks 0-2 Channel Enable Registers - RMD0(*)

| b+10 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|----------------------------------|----|----|----|-------|--------------|------|------|------|--------------|------|------|------|--------------|------|------|
| Write* | | | | | CH 23 | CH22 CH23 | CH21 | CH20 | CH13 | CH12 CH13 | CH11 | CH10 | CH03 | CH02 CH03 | CH01 | CH00 |
| Read | Always Returns FFFF _h | | | | | | | | | | | | | | | |

* Write "1" closes channel to COMmon (only one channel per bank can be closed at one time). All other to "0".

Table B-8. RF Multiplexer Module 00 Banks 3-5 Channel Enable Registers - RMD1(*)

| b+12 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|----------------------------------|----|----|----|------|--------------|------|------|------|--------------|------|------|------|--------------|------|------|
| Write* | | | | | CH53 | CH52 CH53 | CH51 | CH50 | CH43 | CH42 CH43 | CH41 | CH40 | CH33 | CH32 CH33 | CH31 | CH30 |
| Read | Always Returns FFFF _h | | | | | | | | | | | | | | | |

* Write "1" closes channel to COMmon (only one channel per bank can be closed at one time). All other to "0".

Table B-9. Expander Module 01 Banks 0-2 Channel Enable Registers - RMD2(*)

| b+14 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|----------------------------------|----|----|----|------|--------------|------|------|------|--------------|------|------|------|--------------|------|------|
| Write* | | | | | CH23 | CH22 CH23 | CH21 | CH20 | CH13 | CH12 CH13 | CH11 | CH10 | CH03 | CH02 CH03 | CH01 | CH00 |
| Read | Always Returns FFFF _h | | | | | | | | | | | | | | | |

* Write “1” closes channel to COMmon (only one channel per bank can be closed at one time). All other to “0”.

Table B-10. Expander Module 01 Banks 3-5 Channel Enable Registers - RMD3(*)

| b+16 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|----------------------------------|----|----|----|------|--------------|------|------|------|--------------|------|------|------|--------------|------|------|
| Write* | | | | | CH53 | CH52 CH53 | CH51 | CH50 | CH43 | CH42 CH43 | CH41 | CH40 | CH33 | CH32 CH33 | CH31 | CH30 |
| Read | Always Returns FFFF _h | | | | | | | | | | | | | | | |

* Write “1” closes channel to COMmon (only one channel per bank can be closed at one time). All other to “0”.

Table B-11. Expander Module 02 Banks 0-2 Channel Enable Registers - RMD4(*)

| b+18 _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|----------------------------------|----|----|----|------|--------------|------|------|------|--------------|------|------|------|--------------|------|------|
| Write* | | | | | CH23 | CH22 CH23 | CH21 | CH20 | CH13 | CH12 CH13 | CH11 | CH10 | CH03 | CH02 CH03 | CH01 | CH00 |
| Read | Always Returns FFFF _h | | | | | | | | | | | | | | | |

* Write “1” closes channel to COMmon (only one channel per bank can be closed at one time). All other to “0”.

Table B-12. Expander Module 02 Banks 3-5 Channel Enable Registers - RMD5(*)

| b+1A _h | 15 | 14 | 13 | 12 | 11 | 10 | 9 | 8 | 7 | 6 | 5 | 4 | 3 | 2 | 1 | 0 |
|-------------------|----------------------------------|----|----|----|------|--------------|------|------|------|--------------|------|------|------|--------------|------|------|
| Write* | | | | | CH53 | CH52 CH53 | CH51 | CH50 | CH43 | CH42 CH43 | CH41 | CH40 | CH33 | CH32 CH33 | CH31 | CH30 |
| Read | Always Returns FFFF _h | | | | | | | | | | | | | | | |

* Write “1” closes channel to COMmon (only one channel per bank can be closed at one time). All other to “0”.

Selecting Channels Using Your Own Relays

Figure B-1 shows the pin-outs for connectors P200 and P400 on the driver portion of the module (see Figure 2-3). Connector P200 has connections for remote relay modules (RMD) 0, 1, and 3. Connector P400 has RMD 2, 4, and 5.

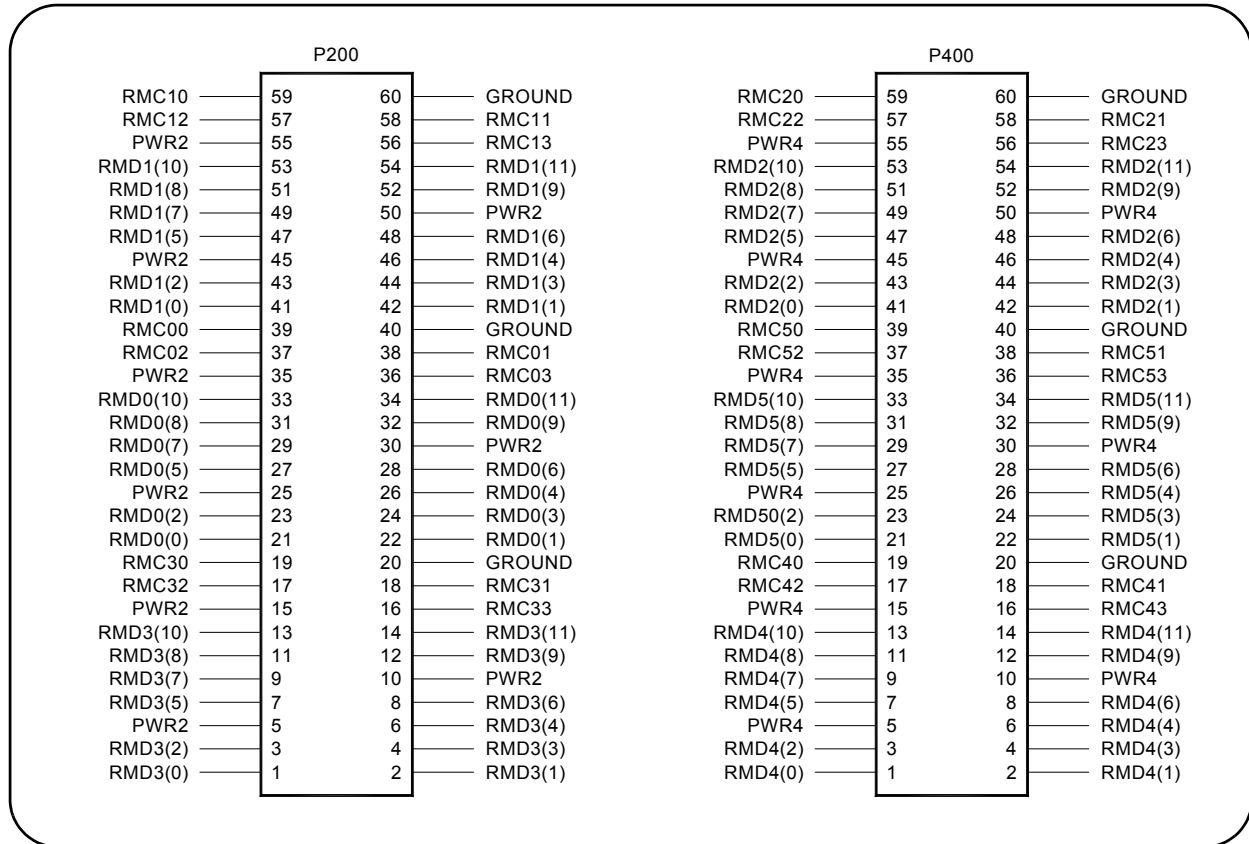


Figure B-1. P200 and P400 Connector Pin-outs

Figure B-2 shows a simplified schematic of a remote relay module (such as RMD,1 for example). P1 connector pins 1, 3, 4, and 5 set the Remote Module Code (RMC). For the 75 Ohm relay modules, the code is FF11_n. These pins set the code for RMC00-RMC03, RMC10-RMC13, RMC30-RMC33 on P200 and RMC20-RMC23, RMC40-RMC43, and RMC50-RMC53 on P400.

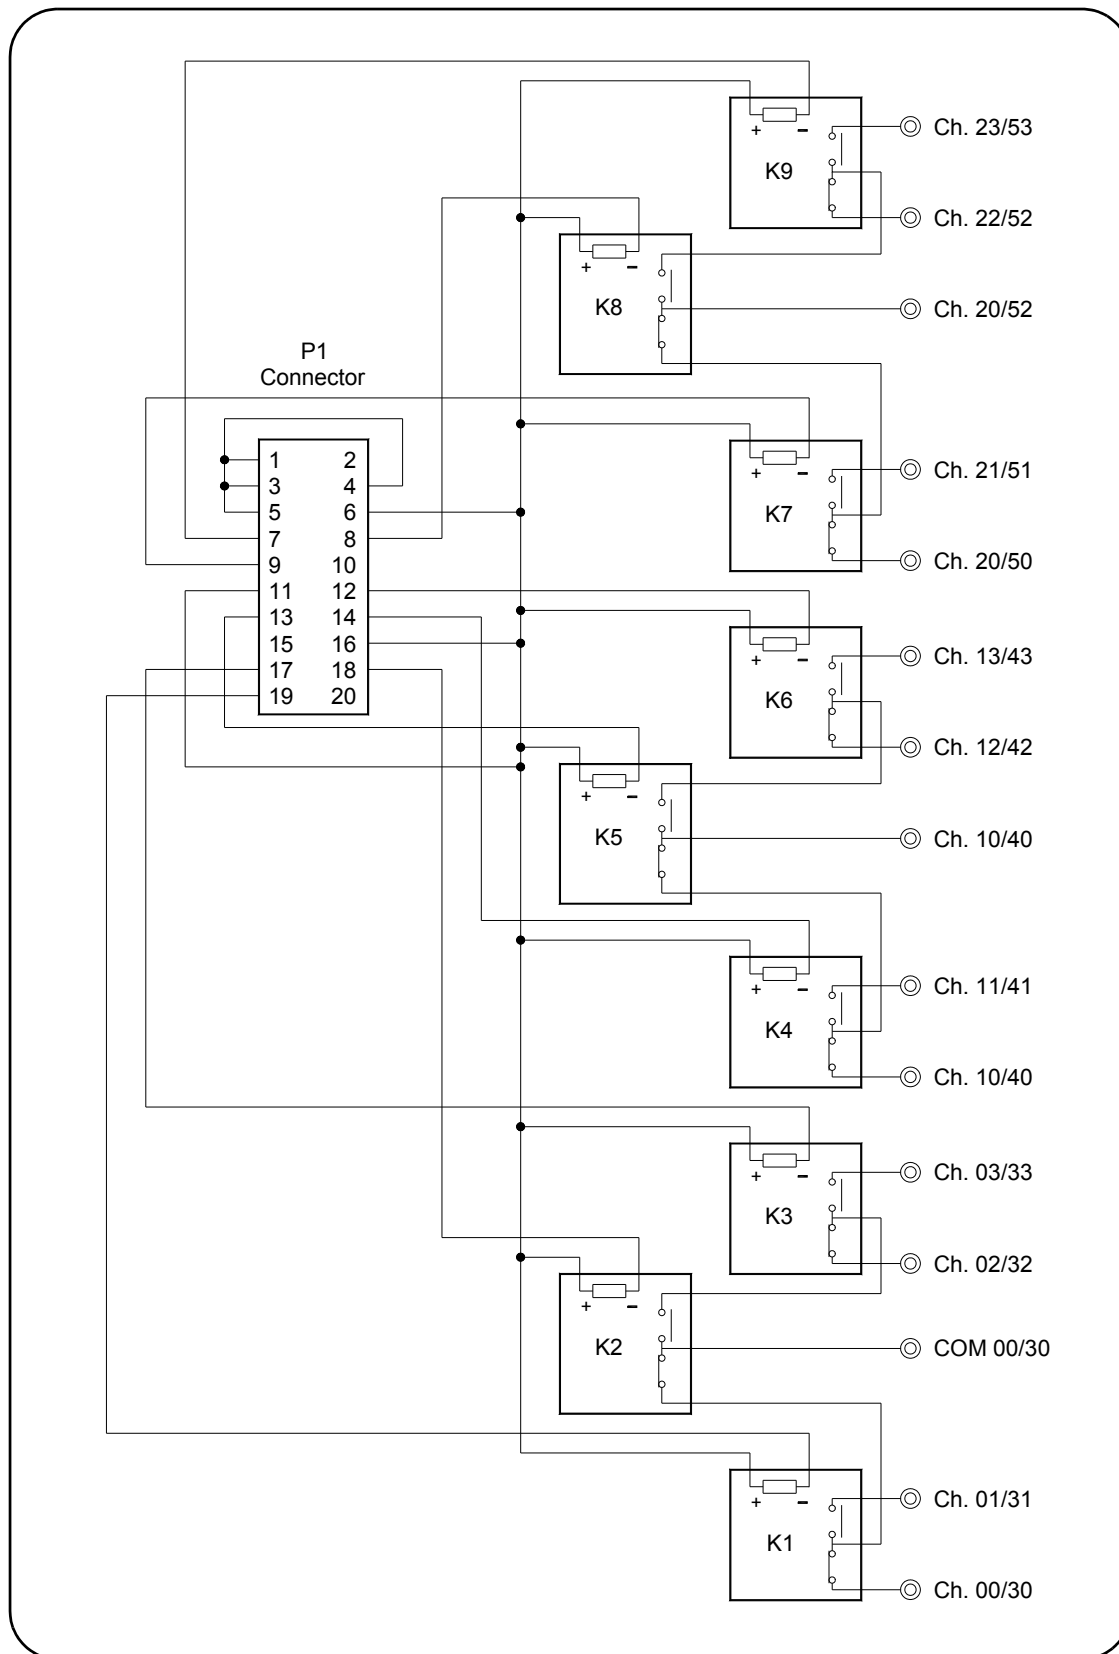


Figure B-2. Relay Module Simplified Schematic

Table B-13 lists the Relay Module P1 connector pins and connection points on P200 and P400.

Table B-13. Connector Pinouts

| Relay Module P1 Pins | Pin Names (x is RMD number) | P200 pin numbers | | | P400 pin numbers | | |
|-------------------------|--------------------------------|------------------|------|------|------------------|------|------|
| | | RMD0 | RMD1 | RMD3 | RMD2 | RMD4 | RMD5 |
| 1 | Ground | 60 | 40 | 20 | 60 | 40 | 20 |
| 2 | RMCx0 | 59 | 39 | 19 | 59 | 39 | 19 |
| 3 | RMCx1 | 58 | 38 | 18 | 58 | 38 | 18 |
| 4 | RMCx2 | 57 | 37 | 17 | 57 | 37 | 17 |
| 5 | RMCx3 | 56 | 36 | 16 | 56 | 36 | 16 |
| 6 | PWR2/PWR4 | 55 | 35 | 15 | 55 | 35 | 15 |
| 7 | RMDx(11) | 54 | 34 | 14 | 54 | 34 | 14 |
| 8 | RMDx(10) | 53 | 33 | 13 | 53 | 33 | 13 |
| 9 | RMDx(9) | 52 | 32 | 12 | 52 | 32 | 12 |
| 10 | RMDx(8) | 51 | 31 | 11 | 51 | 31 | 11 |
| 11 | PWR2/PWR4 | 50 | 30 | 10 | 50 | 30 | 10 |
| 12 | RMDx(7) | 49 | 29 | 9 | 49 | 29 | 9 |
| 13 | RMDx(6) | 48 | 28 | 8 | 48 | 28 | 8 |
| 14 | RMDx(5) | 47 | 27 | 7 | 47 | 27 | 7 |
| 15 | RMDx(4) | 46 | 26 | 6 | 46 | 26 | 6 |
| 16 | PWR2/PWR4 | 45 | 25 | 5 | 45 | 25 | 5 |
| 17 | RMDx(3) | 44 | 24 | 4 | 44 | 24 | 4 |
| 18 | RMDx(2) | 43 | 23 | 3 | 43 | 23 | 3 |
| 19 | RMDx(1) | 42 | 22 | 2 | 42 | 22 | 2 |
| 20 | RMDx(0) | 41 | 21 | 1 | 41 | 21 | 1 |

Example: Using the Register and Pin-out Maps

As an example of using the register information, assume you want to use the E1474 to close a remote 5V relay, K1 (see Figure B-2), connected to the RMD 2 connector (see Figure 2-3). First, change J400 on the driver board to the +5V position (see Figure 2-4).

NOTE *All relays connected through J400 must now be 5 volt relays.*

From the Register maps, Channel 01 on RMD2 is Bit 01. To close channel 01 (relay K1, Figure B-2) on RMD 2 [pin 19 of P1 (corresponds to pin 42 of P400) needs to be at 0 volts to turn on relay K1], send:

CLOSE (@010101)

or

VXI: WRIT *ladd*,20,2

where *ladd* is the logical address of the module.

Appendix C

RF Multiplexer Error Messages

Table C-1 lists the error messages associated with the RF Multiplexer module programmed by SCPI. See the appropriate mainframe manual for a complete list of error messages.

Table C-1. RF Multiplexer Error Messages

| Number | Title | Potential Cause |
|--------|--------------------------------------|--|
| -224 | Illegal Parameter | Attempting to execute a command with a parameter not applicable to the command. |
| 2000 | Invalid Card Number | Addressing a module (card) in a switchbox that is not part of the switchbox. |
| 2001 | Invalid Channel Number | Attempting to address a channel of module in a switchbox that is not supported by the module (e.g., channel 99 of a multiplexer module). |
| 2006 | Command not supported on this card | Sending a command to a module (card) in a switchbox that is unsupported by the module. |
| 2009 | Too many channels in channel list | Attempting to address more channels than available in the switchbox. |
| 2010 | Scan mode not supported on this card | Sending a command to a module (card) in a switchbox that is unsupported by the module. |
| 2600 | Function not supported on this card | Sending a command to a module (card) in a switchbox that is not supported by the module or switchbox. |
| 2601 | Channel list required | Sending a command requiring a channel list without the channel list. |

Notes:

Replacement Strategy

Electromechanical relays are subject to normal wear-out. Relay life depends on several factors. The replacement strategy depends on the application. If some relays are used more often or at a higher load than other relays, the relays can be individually replaced as needed.

If all relays see similar loads and switching frequencies, the entire circuit board can be replaced when the end of relay life approaches. The sensitivity of the application should be weighed against the cost of replacing relays with some useful life remaining.

NOTE *Relays that wear out normally or fail due to misuse should not be considered defective and are not covered by the product's warranty.*

Relay Life Factors

Some effects of loading and switching frequency on relay life follow.

- **Relay Load.** In general, higher power switching reduces relay life. In addition, capacitive/inductive loads and high inrush currents (for example, turning on a lamp or starting a motor) reduces relay life. Exceeding specified maximum inputs can cause catastrophic failure.
- **Switching Frequency.** Relay contacts heat up when switched. As the switching frequency increases, the contacts have less time to dissipate heat. The resulting increase in contact temperature also reduces relay life.

End-of-Life Determination

A preventive maintenance routine can prevent problems caused by unexpected relay failure. The end of life of a relay can be determined by using one or more of three methods: contact resistance maximum value, contact resistance variance, and/or number of relay operations. The best method (or combination of methods), as well as the failure criteria, depends on the application in which the relay is used.

- **Contact Resistance Maximum Value.** As the relay begins to wear out, its contact resistance increases. When the resistance exceeds a predetermined value, the relay should be replaced.
- **Contact Resistance Variance.** The stability of the contact resistance decreases with age. Using this method, the contact resistance is measured several (5-10) times, and the variance of the measurements is determined. An increase in the variance indicates deteriorating performance.
- **Number of Relay Operations.** Relays can be replaced after a predetermined number of contact closures. However, this method requires knowledge of the applied load and life specifications for the applied load.

A

- abbreviated commands, 38
- address space, 51
- addressing
 - channels, 13
 - multiplexers, 13
 - registers, 51

C

- cables, expander, 20
- cabling guidelines
 - E1472A/E1473A, 24
 - E1474A/E1475A, 25
- card numbers, 13
- cautions, 17
- Channel Enable registers, 53, 54
- channels, addressing, 13
- clearing the error queue, 45
- commands
 - command reference, SCPI, 39
 - command types, 37
 - format, SCPI, 15
 - linking, 39
 - parameters, 38
 - RF multiplexer, 31
 - separators, 38
- common commands
 - *CLS, 31, 46
 - *ESE, 31, 46
 - *ESE?, 46
 - *ESR?, 46
 - *IDN?, 46
 - *OPC, 46
 - *OPC?, 46
 - *RCL, 34, 46
 - *RST, 31, 46
 - *SAV, 34, 46
 - *SRE, 31, 46
 - *SRE?, 46
 - *STB?, 46
 - *TRG, 46
 - *TST, 46
 - *WAI, 46
- format, 37
- quick reference, 46

C (continued)

- configuration, typical, 12
- connecting user inputs
 - E1472A/E1473A, 24
 - E1474A/E1475A, 25
- crosstalk, 49

D

- declaration of conformity, 7
- definition, instrument, 12
- description
 - general, 11
 - RF multiplexers, 10
- detecting error conditions, 34
- Device Type register, 52
- documentation history, 6

E

- error conditions, detecting, 34
- error messages, 61
- error queue, clearing, 45
- examples
 - Addressing a Status/Control Register, 51
 - Closing RF Multiplexer Channels, 41
 - Initial Operation, 16
 - Matrix-Type Switching, 33
 - Querying Channel Closure, 41
 - Querying Channel Open State, 42
 - Reading Model Number, 44
 - Reading Model Number of Module, 45
 - Reading Module Description, 43
 - Reading the Error Queue, 45
 - Setting Module to Power-On State, 44
 - Standard Switching, 32
 - Tree Switching, 33
 - Using Register/Pin-out Maps, 60
- expander cables, 20
- expanding the multiplexers, 20

G

- general description, 11

I

implied commands, 38
insertion loss, 49
instrument definition, 12
interrupt priority, setting, 19

L

linking commands, 39
logical address, 51
logical address switch, setting, 18

M

Manufacturer ID register, 52
module address, 51
module numbers, 13–14
multiplexers
 addressing, 13
 expanding, 20
 programming, 13

N

numbers, error, 61

O

offset, register, 51
operation, basic, 11

P

programming the multiplexers, 13
programming, register-based, 51

R

reading registers, 52
register offset, 51
register-based programming, 51
registers
 addressing, 51
 reading, 52
relay drive level, selecting, 22
relay life, 63

R (continued)

relays
 end-of-life determination, 63
 relay life factors, 63
 replacement strategy, 63
Remote Module ID registers, 53
reset conditions, 31
restricted rights statement, 5
RF multiplexers description, 10
[ROUTE:] subsystem
 [ROUTE:]CLOSE, 31, 40
 [ROUTE:]CLOSE?, 31, 41
 [ROUTE:]OPEN?, 31, 41

S

safety symbols, 6
SCPI commands
 command reference, 39
 format, 15, 37
 quick reference, 47
specifications, 49
Status/Control register, 52–53
switchbox instrument, 12
switching channels, 32
SYSTEM subsystem
 SYSTEM:CDEscription?, 43
 SYSTEM:COPTion?, 43
 SYSTEM:CPON, 44
 SYSTEM:CTYPE?, 44
 SYSTEM:ERRor?, 45

W

warnings, 6, 17
warranty statement, 5
writing to registers, 53